

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016481.D
 Acq On : 04 Jun 2020 01:39
 Operator : SY/MD
 Sample : L2849-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETP7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	89	rVB	3586962	3656642	28.24%	13.668%
2	1.566	142	148	159	rVB	133471	158596	1.22%	0.593%
3	2.119	311	320	333	rBV2	317211	470268	3.63%	1.758%
4	2.457	419	425	428	rBV6	1717	1773	0.01%	0.007%
5	2.508	435	441	442	rBV4	2075	1911	0.01%	0.007%
6	2.733	507	511	514	rBV6	1438	1337	0.01%	0.005%
7	2.949	574	578	580	rBV3	1157	888	0.01%	0.003%
8	3.048	605	609	612	rBV5	1379	1221	0.01%	0.005%
9	3.068	612	615	617	rBV3	1017	612	0.00%	0.002%
10	3.171	643	647	650	rBV4	911	863	0.01%	0.003%
11	3.193	650	654	657	rVB4	1381	935	0.01%	0.003%
12	3.219	657	662	665	rBV6	1749	1676	0.01%	0.006%
13	3.283	677	682	685	rBV4	910	961	0.01%	0.004%
14	3.306	687	689	692	rVB4	1268	584	0.00%	0.002%
15	3.322	692	694	698	rVB5	1193	639	0.00%	0.002%
16	3.357	702	705	710	rBV6	760	789	0.01%	0.003%
17	3.405	715	720	722	rBV4	1766	1278	0.01%	0.005%
18	3.447	729	733	736	rBV5	1283	1161	0.01%	0.004%
19	3.672	801	803	806	rVB2	1371	545	0.00%	0.002%
20	3.708	810	814	816	rBV5	1300	824	0.01%	0.003%
21	3.740	822	824	827	rVB3	1187	519	0.00%	0.002%
22	3.936	859	885	918	rBV	5308463	12949099	100.00%	48.400%
23	4.376	1008	1022	1045	rVB	226595	544825	4.21%	2.036%
24	4.765	1140	1143	1145	rBV3	1351	728	0.01%	0.003%
25	4.791	1149	1151	1153	rVB2	1262	613	0.00%	0.002%
26	4.987	1210	1212	1217	rVB5	1344	777	0.01%	0.003%
27	5.071	1221	1238	1265	rBV2	558801	1439146	11.11%	5.379%
28	5.354	1322	1326	1332	rVB8	2106	2070	0.02%	0.008%
29	5.550	1383	1387	1388	rBV4	1035	611	0.00%	0.002%
30	5.640	1399	1415	1436	rBV	422914	847044	6.54%	3.166%
31	5.817	1467	1470	1472	rBV3	1118	565	0.00%	0.002%
32	5.888	1489	1492	1495	rVB4	1314	799	0.01%	0.003%
33	5.942	1495	1509	1522	rBV10	10050	25545	0.20%	0.095%
34	6.093	1543	1556	1581	rVB2	319347	640892	4.95%	2.395%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016481.D
 Acq On : 04 Jun 2020 01:39
 Operator : SY/MD
 Sample : L2849-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETP7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.232	1597	1599	1602	rBV4	2101	1699	0.01%	0.006%
36	6.441	1662	1664	1666	rBV2	1347	694	0.01%	0.003%
37	6.749	1758	1760	1763	rVB5	1186	603	0.00%	0.002%
38	6.781	1767	1770	1771	rBV3	1258	570	0.00%	0.002%
39	6.891	1802	1804	1807	rBV3	1203	527	0.00%	0.002%
40	6.926	1813	1815	1820	rBV5	776	699	0.01%	0.003%
41	6.961	1823	1826	1828	rBV3	1215	941	0.01%	0.004%
42	7.006	1829	1840	1858	rBV	159335	284862	2.20%	1.065%
43	7.206	1900	1902	1904	rBV2	1076	575	0.00%	0.002%
44	7.338	1930	1943	1960	rBV	661750	1129291	8.72%	4.221%
45	7.598	2022	2024	2027	rBV4	1178	713	0.01%	0.003%
46	7.643	2028	2038	2056	rVV	113196	196516	1.52%	0.735%
47	8.051	2163	2165	2168	rBV4	931	531	0.00%	0.002%
48	8.106	2168	2182	2202	rBV	403214	681133	5.26%	2.546%
49	8.415	2276	2278	2280	rBV3	999	551	0.00%	0.002%
50	8.505	2304	2306	2309	rBV3	1024	750	0.01%	0.003%
51	8.592	2330	2333	2335	rBV3	1423	804	0.01%	0.003%
52	8.698	2358	2366	2367	rBV6	1748	2235	0.02%	0.008%
53	8.875	2407	2421	2440	rBV	628179	1026941	7.93%	3.838%
54	9.161	2506	2510	2514	rBV7	2051	1705	0.01%	0.006%
55	9.196	2519	2521	2524	rVB3	2162	797	0.01%	0.003%
56	9.264	2540	2542	2545	rBV4	1522	660	0.01%	0.002%
57	9.341	2564	2566	2568	rBV3	1005	539	0.00%	0.002%
58	9.405	2583	2586	2589	rVB5	858	518	0.00%	0.002%
59	9.428	2589	2593	2595	rBV4	1211	948	0.01%	0.004%
60	9.492	2611	2613	2615	rBV	1269	598	0.00%	0.002%
61	9.649	2659	2662	2665	rBV4	1701	871	0.01%	0.003%
62	9.691	2672	2675	2676	rBV3	1142	693	0.01%	0.003%
63	9.720	2681	2684	2685	rBV3	1206	674	0.01%	0.003%
64	9.733	2685	2688	2691	rBV4	865	577	0.00%	0.002%
65	9.887	2733	2736	2738	rVB3	1110	606	0.00%	0.002%
66	9.952	2754	2756	2759	rBV4	914	652	0.01%	0.002%
67	10.026	2776	2779	2782	rBV4	1585	1264	0.01%	0.005%
68	10.122	2808	2809	2812	rBV3	1070	648	0.01%	0.002%
69	10.161	2818	2821	2823	rBV4	1240	769	0.01%	0.003%
70	10.193	2828	2831	2833	rBV3	1317	766	0.01%	0.003%
71	10.238	2834	2845	2861	rVV	422245	652824	5.04%	2.440%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016481.D
 Acq On : 04 Jun 2020 01:39
 Operator : SY/MD
 Sample : L2849-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETPP7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.395	2892	2894	2896	rBV2	1548	836	0.01%	0.003%
73	10.701	2985	2989	2993	rBV4	1238	910	0.01%	0.003%
74	10.788	3014	3016	3020	rVB3	1143	691	0.01%	0.003%
75	10.833	3027	3030	3031	rBV3	1051	589	0.00%	0.002%
76	10.932	3058	3061	3062	rBV2	1213	859	0.01%	0.003%
77	11.106	3112	3115	3116	rBV2	1045	573	0.00%	0.002%
78	11.154	3128	3130	3133	rBV3	1095	860	0.01%	0.003%
79	11.222	3147	3151	3154	rBV4	1361	959	0.01%	0.004%
80	11.270	3155	3166	3188	rVV	609749	942917	7.28%	3.524%
81	11.421	3211	3213	3215	rBV2	982	623	0.00%	0.002%
82	11.444	3218	3220	3222	rBV3	1233	561	0.00%	0.002%
83	11.646	3272	3283	3300	rBV	668843	1033857	7.98%	3.864%
84	11.997	3389	3392	3394	rVV3	1104	601	0.00%	0.002%
85	12.074	3413	3416	3420	rBV5	1254	967	0.01%	0.004%
86	12.099	3420	3424	3428	rBV7	1031	913	0.01%	0.003%
87	12.241	3466	3468	3470	rBV2	1286	716	0.01%	0.003%
88	12.254	3470	3472	3475	rBV3	822	598	0.00%	0.002%
89	12.562	3564	3568	3572	rBV6	1101	1065	0.01%	0.004%
90	12.890	3667	3670	3672	rBV4	993	616	0.00%	0.002%
91	12.910	3672	3676	3681	rVV8	1411	1573	0.01%	0.006%
92	13.099	3732	3735	3739	rBV5	1973	1669	0.01%	0.006%
93	13.119	3739	3741	3743	rBV2	926	525	0.00%	0.002%
94	13.382	3821	3823	3827	rVB4	1298	1078	0.01%	0.004%
95	13.511	3861	3863	3866	rBV3	1433	770	0.01%	0.003%
96	13.595	3886	3889	3893	rBV5	1952	1811	0.01%	0.007%
97	13.649	3903	3906	3907	rBV2	1327	616	0.00%	0.002%
98	14.070	4035	4037	4040	rBV4	1199	731	0.01%	0.003%
99	14.212	4079	4081	4083	rBV3	1481	698	0.01%	0.003%
100	14.575	4191	4194	4198	rBV4	1734	1613	0.01%	0.006%


Sum of corrected areas: 26754275

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016481.D
Acq On : 04 Jun 2020 01:39
Operator : SY/MD
Sample : L2849-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTP7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

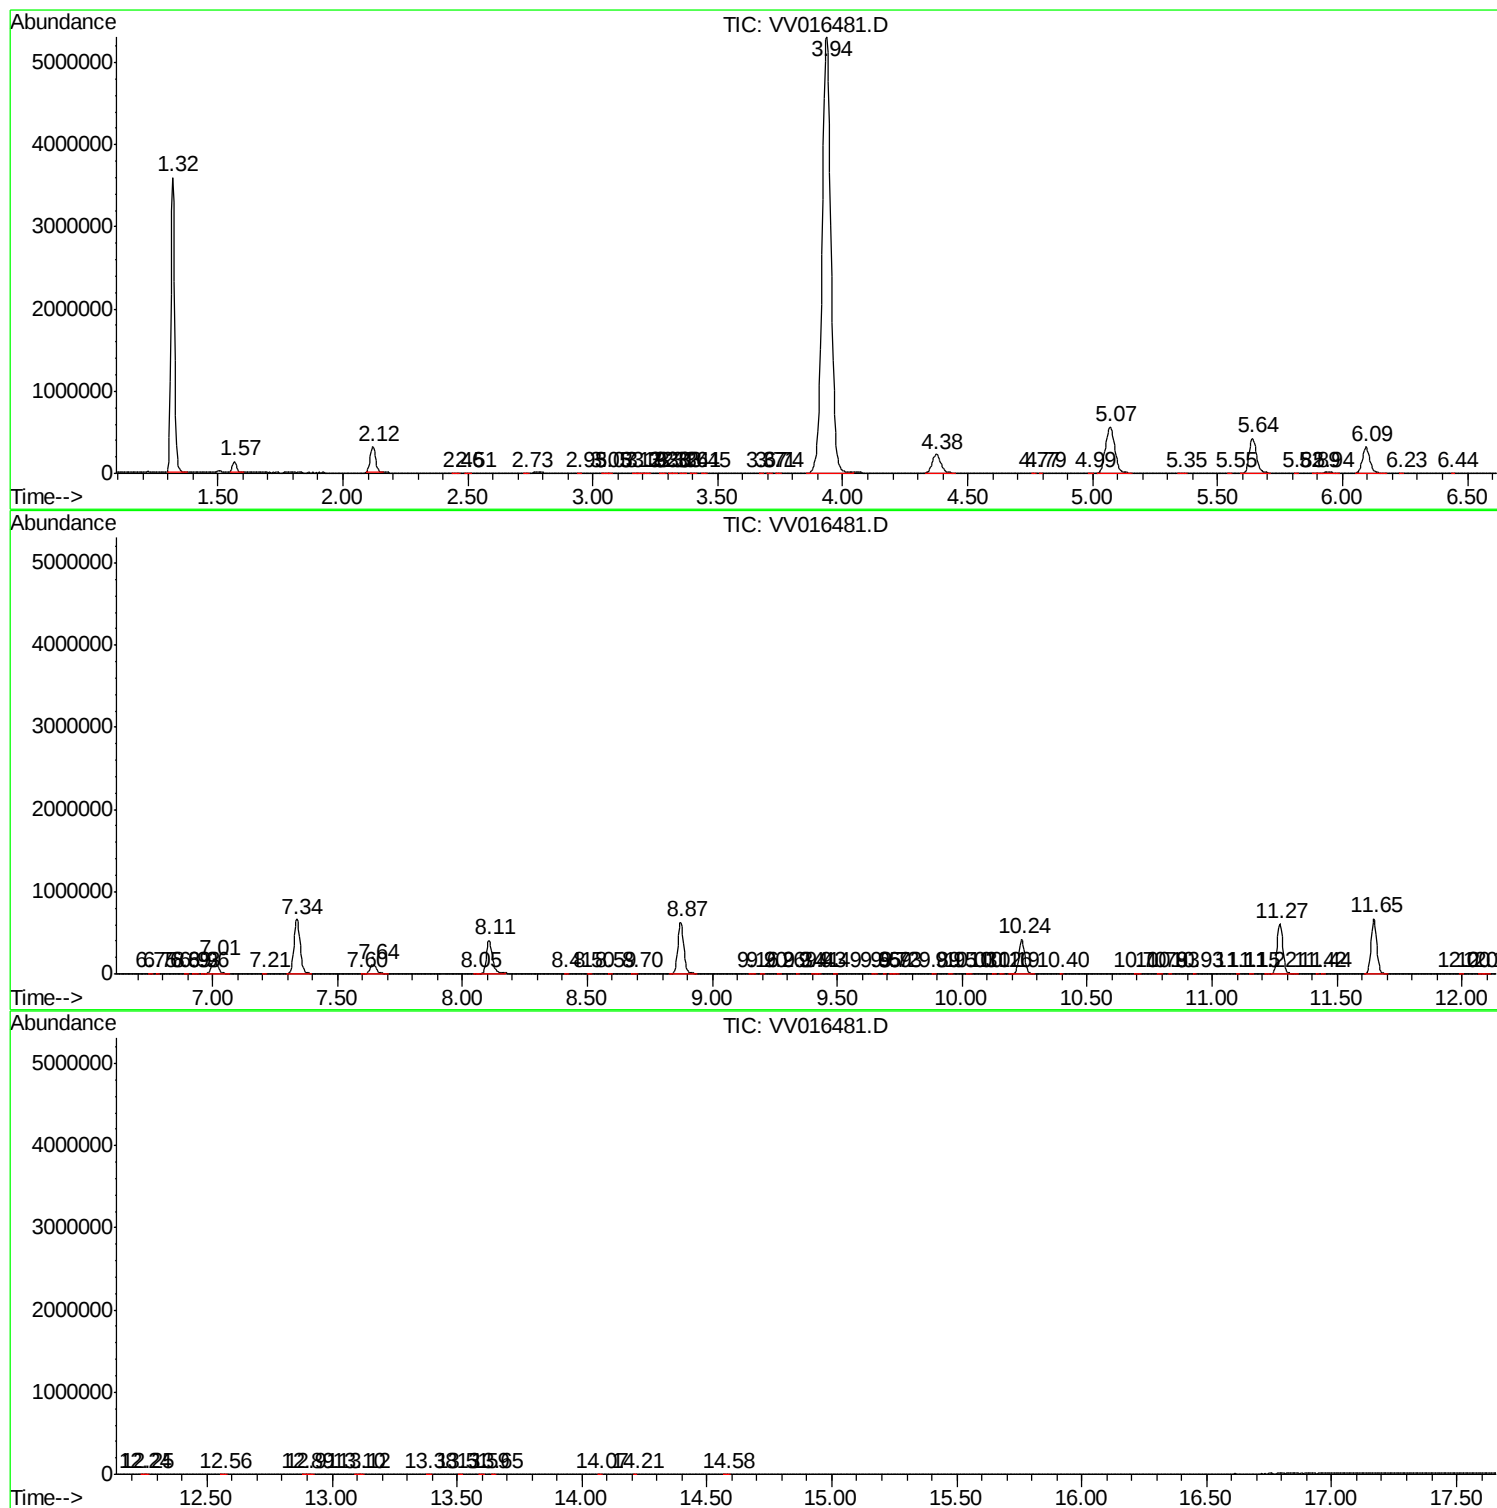

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016481.D
Acq On : 04 Jun 2020 01:39
Operator : SY/MD
Sample : L2849-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTP7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016481.D
Acq On : 04 Jun 2020 01:39
Operator : SY/MD
Sample : L2849-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTP7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc