

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016492.D
 Acq On : 04 Jun 2020 05:59
 Operator : SY/MD
 Sample : VIBLK51
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	182467	179568	12.61%	1.643%
2	1.576	144	151	164	rVB	132481	154065	10.82%	1.410%
3	2.122	311	321	334	rBV	289262	418725	29.41%	3.832%
4	2.335	384	387	391	rBV4	1123	1154	0.08%	0.011%
5	2.428	414	416	420	rVB5	1519	860	0.06%	0.008%
6	2.495	434	437	439	rBV4	1139	806	0.06%	0.007%
7	2.528	439	447	458	rVB7	5490	10338	0.73%	0.095%
8	2.672	490	492	495	rBV3	1123	808	0.06%	0.007%
9	2.766	517	521	522	rBV5	863	665	0.05%	0.006%
10	2.794	526	530	532	rBV5	926	761	0.05%	0.007%
11	2.997	590	593	595	rBV3	1020	659	0.05%	0.006%
12	3.042	604	607	610	rBV4	1292	867	0.06%	0.008%
13	3.116	628	630	634	rVB3	1422	775	0.05%	0.007%
14	3.290	682	684	686	rBV3	1249	746	0.05%	0.007%
15	3.508	748	752	757	rBV7	1811	1979	0.14%	0.018%
16	3.540	760	762	765	rBV4	1226	797	0.06%	0.007%
17	3.756	823	829	831	rBV6	1366	1580	0.11%	0.014%
18	3.791	838	840	842	rBV3	1265	646	0.05%	0.006%
19	3.830	848	852	853	rBV3	1008	733	0.05%	0.007%
20	3.839	853	855	857	rVB3	1776	761	0.05%	0.007%
21	3.894	862	872	900	rBV	112727	302243	21.23%	2.766%
22	4.187	960	963	966	rVB4	1652	872	0.06%	0.008%
23	4.376	1007	1022	1046	rVB	229425	552707	38.82%	5.058%
24	4.489	1054	1057	1058	rBV3	1525	912	0.06%	0.008%
25	4.589	1083	1088	1090	rBV4	1008	655	0.05%	0.006%
26	4.701	1120	1123	1124	rBV3	976	639	0.04%	0.006%
27	4.711	1124	1126	1129	rVV4	1837	825	0.06%	0.008%
28	4.765	1141	1143	1147	rVB3	1805	1152	0.08%	0.011%
29	4.791	1147	1151	1154	rBV4	1354	1277	0.09%	0.012%
30	4.962	1201	1204	1211	rBV9	1608	1056	0.07%	0.010%
31	5.071	1221	1238	1267	rVV2	559872	1423635	100.00%	13.027%
32	5.454	1355	1357	1360	rVB4	1934	845	0.06%	0.008%
33	5.470	1360	1362	1364	rBV2	1142	639	0.04%	0.006%
34	5.521	1375	1378	1384	rVB6	1117	875	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016492.D
 Acq On : 04 Jun 2020 05:59
 Operator : SY/MD
 Sample : VIBLK51
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	5.547	1384	1386	1389	rBV3	1326	651	0.05%	0.006%
36	5.576	1393	1395	1400	rBV5	826	705	0.05%	0.006%
37	5.640	1400	1415	1441	rBV	460316	921239	64.71%	8.430%
38	5.939	1496	1508	1520	rBV	6548	15771	1.11%	0.144%
39	6.093	1544	1556	1587	rVB	316664	642645	45.14%	5.881%
40	6.351	1634	1636	1638	rBV3	1248	662	0.05%	0.006%
41	6.376	1642	1644	1649	rBV6	1351	1071	0.08%	0.010%
42	6.511	1684	1686	1688	rBV2	1486	826	0.06%	0.008%
43	7.007	1829	1840	1858	rBV	168689	303779	21.34%	2.780%
44	7.164	1886	1889	1891	rBV4	1296	757	0.05%	0.007%
45	7.280	1923	1925	1928	rBV3	1256	1019	0.07%	0.009%
46	7.338	1931	1943	1961	rVV	648457	1114033	78.25%	10.194%
47	7.643	2028	2038	2053	rBV	116645	199770	14.03%	1.828%
48	7.907	2118	2120	2123	rVB4	1763	933	0.07%	0.009%
49	8.106	2172	2182	2207	rBV	427917	707111	49.67%	6.471%
50	8.682	2357	2361	2365	rVB6	1158	977	0.07%	0.009%
51	8.704	2365	2368	2371	rBV4	1383	1050	0.07%	0.010%
52	8.875	2409	2421	2440	rBV	684906	1107117	77.77%	10.131%
53	9.096	2488	2490	2495	rVB6	1808	763	0.05%	0.007%
54	9.270	2542	2544	2547	rVB4	1520	656	0.05%	0.006%
55	9.302	2551	2554	2555	rBV3	1171	665	0.05%	0.006%
56	9.444	2595	2598	2601	rBV5	1576	861	0.06%	0.008%
57	9.486	2607	2611	2613	rBV4	1363	813	0.06%	0.007%
58	9.566	2632	2636	2637	rBV3	1603	997	0.07%	0.009%
59	9.662	2664	2666	2670	rVB4	1331	801	0.06%	0.007%
60	9.762	2693	2697	2700	rBV6	1372	954	0.07%	0.009%
61	9.778	2700	2702	2704	rBV2	1309	767	0.05%	0.007%
62	10.096	2799	2801	2805	rBV4	1102	830	0.06%	0.008%
63	10.164	2816	2822	2824	rBV7	1555	1347	0.09%	0.012%
64	10.238	2834	2845	2860	rBV	433093	662890	46.56%	6.066%
65	10.360	2878	2883	2884	rBV5	1163	991	0.07%	0.009%
66	10.431	2903	2905	2909	rBV4	920	830	0.06%	0.008%
67	10.466	2914	2916	2917	rBV2	1467	702	0.05%	0.006%
68	10.630	2965	2967	2969	rBV3	1387	872	0.06%	0.008%
69	10.717	2990	2994	2995	rBV4	1270	932	0.07%	0.009%
70	10.897	3047	3050	3054	rVB5	1435	918	0.06%	0.008%
71	11.061	3098	3101	3105	rVB5	1153	986	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016492.D
 Acq On : 04 Jun 2020 05:59
 Operator : SY/MD
 Sample : VIBLK51
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.084	3105	3108	3109	rBV3	1163	674	0.05%	0.006%
73	11.119	3115	3119	3122	rBV4	1259	925	0.06%	0.008%
74	11.177	3133	3137	3141	rBV6	1896	1867	0.13%	0.017%
75	11.270	3154	3166	3184	rBV	703237	1067169	74.96%	9.765%
76	11.453	3217	3223	3226	rBV5	2049	2128	0.15%	0.019%
77	11.530	3245	3247	3250	rBV3	1324	659	0.05%	0.006%
78	11.582	3261	3263	3267	rVB3	1176	732	0.05%	0.007%
79	11.646	3272	3283	3302	rVV	698057	1067463	74.98%	9.768%
80	11.884	3354	3357	3362	rVB6	1295	1042	0.07%	0.010%
81	11.910	3362	3365	3369	rBV5	1235	1211	0.09%	0.011%
82	11.929	3369	3371	3374	rBV4	1211	679	0.05%	0.006%
83	12.051	3407	3409	3413	rVB4	1255	752	0.05%	0.007%
84	12.209	3454	3458	3460	rBV3	1095	884	0.06%	0.008%
85	12.286	3478	3482	3483	rVB4	1335	767	0.05%	0.007%
86	12.373	3506	3509	3514	rBV6	1558	1533	0.11%	0.014%
87	12.402	3514	3518	3522	rVB6	1755	1542	0.11%	0.014%
88	12.614	3582	3584	3587	rBV4	1097	655	0.05%	0.006%
89	12.926	3677	3681	3685	rBV7	965	720	0.05%	0.007%
90	13.009	3700	3707	3708	rBV6	1428	1267	0.09%	0.012%
91	13.067	3721	3725	3729	rVB5	1728	1407	0.10%	0.013%
92	13.193	3762	3764	3766	rVB3	1583	703	0.05%	0.006%
93	13.524	3865	3867	3869	rBV2	2522	1621	0.11%	0.015%
94	13.662	3908	3910	3913	rBV4	797	698	0.05%	0.006%
95	13.775	3943	3945	3952	rVB6	1644	1375	0.10%	0.013%
96	14.154	4058	4063	4066	rBV6	1091	1002	0.07%	0.009%
97	14.305	4108	4110	4115	rBV4	1802	1155	0.08%	0.011%
98	14.579	4193	4195	4200	rBV5	1557	1127	0.08%	0.010%
99	14.810	4265	4267	4270	rVB3	1744	764	0.05%	0.007%
100	15.119	4361	4363	4369	rBV6	1307	1171	0.08%	0.011%


Sum of corrected areas: 10928008

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016492.D
Acq On : 04 Jun 2020 05:59
Operator : SY/MD
Sample : VIBLK51
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK51

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

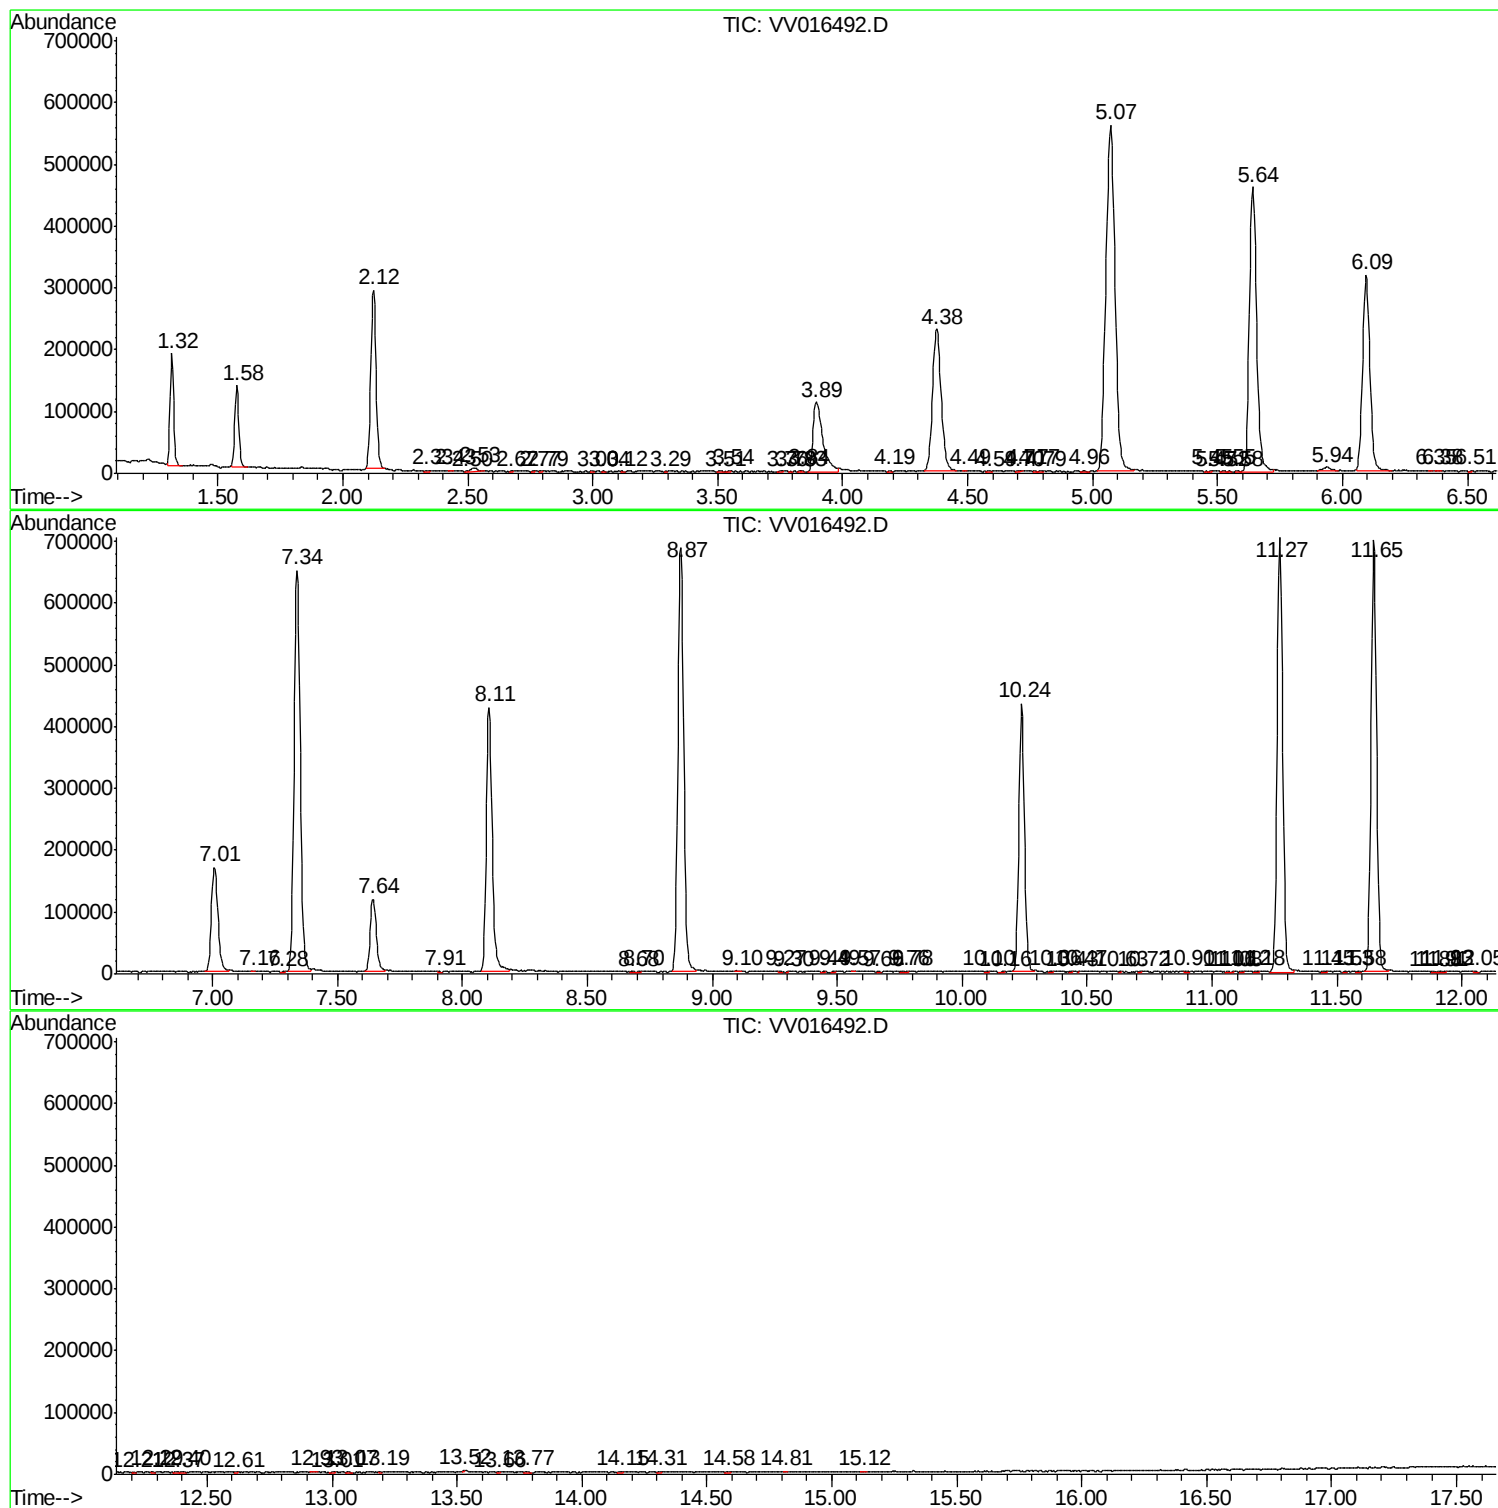

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016492.D
Acq On : 04 Jun 2020 05:59
Operator : SY/MD
Sample : VIBLK51
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK51

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016492.D
Acq On : 04 Jun 2020 05:59
Operator : SY/MD
Sample : VIBLK51
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK51

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc