

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016493.D
 Acq On : 04 Jun 2020 06:23
 Operator : SY/MD
 Sample : L2861-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	85	rVB	174873	180638	12.68%	1.668%
2	1.576	144	151	163	rVB	151179	169324	11.88%	1.563%
3	2.123	311	321	342	rVB	272869	404358	28.38%	3.734%
4	2.354	390	393	394	rBV3	983	721	0.05%	0.007%
5	2.766	514	521	523	rBV8	2099	2170	0.15%	0.020%
6	2.894	558	561	563	rBV4	1372	857	0.06%	0.008%
7	2.971	581	585	589	rBV4	1569	1693	0.12%	0.016%
8	3.026	599	602	603	rVB3	1102	498	0.03%	0.005%
9	3.097	622	624	625	rBV2	855	345	0.02%	0.003%
10	3.142	636	638	641	rBV3	1356	748	0.05%	0.007%
11	3.229	662	665	666	rBV3	1498	823	0.06%	0.008%
12	3.270	674	678	679	rBV4	1249	777	0.05%	0.007%
13	3.312	690	691	694	rVB3	810	305	0.02%	0.003%
14	3.328	694	696	699	rBV3	682	461	0.03%	0.004%
15	3.344	699	701	703	rBV3	1152	753	0.05%	0.007%
16	3.399	716	718	721	rVB5	659	275	0.02%	0.003%
17	3.412	721	722	725	rVB3	1338	494	0.03%	0.005%
18	3.428	725	727	730	rBV3	1171	790	0.06%	0.007%
19	3.444	730	732	735	rVB3	1194	696	0.05%	0.006%
20	3.460	735	737	739	rBV2	658	299	0.02%	0.003%
21	3.473	739	741	742	rBV2	815	282	0.02%	0.003%
22	3.486	743	745	750	rBV4	904	576	0.04%	0.005%
23	3.608	781	783	786	rBV4	1305	543	0.04%	0.005%
24	3.637	790	792	794	rBV2	580	274	0.02%	0.003%
25	3.679	803	805	808	rBV4	800	547	0.04%	0.005%
26	3.798	841	842	843	rBV	1006	314	0.02%	0.003%
27	3.852	856	859	861	rBV4	973	596	0.04%	0.006%
28	3.894	862	872	902	rBV	120806	316094	22.18%	2.919%
29	4.377	1007	1022	1046	rBV	232866	559141	39.24%	5.163%
30	4.569	1078	1082	1084	rBV4	1858	1610	0.11%	0.015%
31	4.701	1120	1123	1126	rBV5	1517	1070	0.08%	0.010%
32	4.894	1181	1183	1184	rBV2	1191	390	0.03%	0.004%
33	4.978	1205	1209	1213	rBV6	1330	1322	0.09%	0.012%
34	5.071	1216	1238	1258	rBV2	551328	1424855	100.00%	13.156%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016493.D
 Acq On : 04 Jun 2020 06:23
 Operator : SY/MD
 Sample : L2861-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	5.348	1321	1324	1326	rBV2	1385	834	0.06%	0.008%
36	5.640	1403	1415	1440	rBV	437971	862064	60.50%	7.960%
37	5.987	1520	1523	1525	rBV4	1940	1329	0.09%	0.012%
38	6.093	1544	1556	1583	rVB	326835	655619	46.01%	6.053%
39	6.290	1615	1617	1621	rVB3	1224	707	0.05%	0.007%
40	6.380	1642	1645	1646	rBV3	1364	701	0.05%	0.006%
41	6.428	1657	1660	1661	rBV3	1672	919	0.06%	0.008%
42	6.563	1700	1702	1707	rVB3	1091	774	0.05%	0.007%
43	6.618	1712	1719	1720	rBV7	1963	1851	0.13%	0.017%
44	6.749	1759	1760	1762	rBV	810	416	0.03%	0.004%
45	6.923	1812	1814	1816	rVB3	1235	600	0.04%	0.006%
46	7.007	1829	1840	1855	rBV	168293	300251	21.07%	2.772%
47	7.338	1931	1943	1965	rBV	663468	1140366	80.03%	10.529%
48	7.585	2017	2020	2023	rBV4	1539	1127	0.08%	0.010%
49	7.643	2027	2038	2057	rVV	122017	205954	14.45%	1.902%
50	8.048	2162	2164	2165	rBV2	781	308	0.02%	0.003%
51	8.106	2172	2182	2203	rBV	427140	697445	48.95%	6.440%
52	8.576	2325	2328	2331	rBV5	1526	1088	0.08%	0.010%
53	8.788	2392	2394	2396	rBV3	1300	763	0.05%	0.007%
54	8.875	2408	2421	2439	rBV	665831	1073296	75.33%	9.910%
55	9.280	2545	2547	2551	rBV5	944	555	0.04%	0.005%
56	9.380	2575	2578	2579	rBV3	1607	849	0.06%	0.008%
57	9.470	2605	2606	2609	rVB3	908	376	0.03%	0.003%
58	9.489	2609	2612	2614	rVB2	1368	649	0.05%	0.006%
59	9.508	2614	2618	2621	rBV4	1689	1255	0.09%	0.012%
60	9.531	2621	2625	2629	rBV5	1226	1274	0.09%	0.012%
61	9.688	2670	2674	2680	rBV8	1796	1875	0.13%	0.017%
62	9.785	2700	2704	2705	rBV3	1339	1007	0.07%	0.009%
63	9.971	2760	2762	2765	rBV4	993	882	0.06%	0.008%
64	10.103	2800	2803	2804	rBV3	1502	713	0.05%	0.007%
65	10.238	2834	2845	2861	rBV	448923	691605	48.54%	6.386%
66	10.441	2906	2908	2910	rVV3	1154	534	0.04%	0.005%
67	10.495	2924	2925	2927	rBV2	1032	466	0.03%	0.004%
68	10.617	2960	2963	2964	rBV2	1539	752	0.05%	0.007%
69	10.775	3008	3012	3016	rBV5	1271	1349	0.09%	0.012%
70	10.801	3016	3020	3022	rBV4	1303	825	0.06%	0.008%
71	10.920	3055	3057	3061	rBV4	1202	782	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016493.D
 Acq On : 04 Jun 2020 06:23
 Operator : SY/MD
 Sample : L2861-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.019	3086	3088	3089	rBV3	873	289	0.02%	0.003%
73	11.068	3100	3103	3105	rBV3	1360	887	0.06%	0.008%
74	11.180	3132	3138	3141	rBV6	2416	2737	0.19%	0.025%
75	11.270	3154	3166	3182	rBV	659657	1011862	71.02%	9.343%
76	11.646	3271	3283	3298	rBV	696851	1069440	75.06%	9.874%
77	11.932	3371	3372	3373	rBV	1016	278	0.02%	0.003%
78	11.942	3373	3375	3377	rVV2	1257	558	0.04%	0.005%
79	12.029	3399	3402	3403	rBV3	1165	628	0.04%	0.006%
80	12.132	3431	3434	3435	rBV3	977	570	0.04%	0.005%
81	12.174	3444	3447	3448	rBV3	1383	777	0.05%	0.007%
82	12.209	3456	3458	3460	rBV4	1121	564	0.04%	0.005%
83	12.341	3496	3499	3500	rBV2	1461	636	0.04%	0.006%
84	12.399	3516	3517	3521	rBV2	1304	802	0.06%	0.007%
85	12.505	3548	3550	3551	rBV2	1427	369	0.03%	0.003%
86	12.694	3606	3609	3613	rBV3	1407	1143	0.08%	0.011%
87	12.746	3622	3625	3627	rVB4	1546	910	0.06%	0.008%
88	12.765	3627	3631	3634	rBV6	1459	1173	0.08%	0.011%
89	12.781	3634	3636	3637	rBV2	892	405	0.03%	0.004%
90	12.936	3682	3684	3688	rBV4	1292	821	0.06%	0.008%
91	13.000	3701	3704	3706	rBV3	1214	618	0.04%	0.006%
92	13.096	3732	3734	3736	rBV3	599	318	0.02%	0.003%
93	13.440	3838	3841	3843	rVB3	1149	701	0.05%	0.006%
94	13.457	3843	3846	3850	rBV3	1945	1515	0.11%	0.014%
95	13.659	3906	3909	3910	rBV3	1008	488	0.03%	0.005%
96	13.714	3924	3926	3927	rBV2	852	322	0.02%	0.003%
97	13.775	3942	3945	3947	rBV3	1433	743	0.05%	0.007%
98	14.129	4051	4055	4059	rBV6	1679	1879	0.13%	0.017%
99	14.190	4072	4074	4077	rVB3	1573	729	0.05%	0.007%
100	14.408	4138	4142	4145	rBV5	1733	1460	0.10%	0.013%


Sum of corrected areas: 10830421

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016493.D
Acq On : 04 Jun 2020 06:23
Operator : SY/MD
Sample : L2861-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D79

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

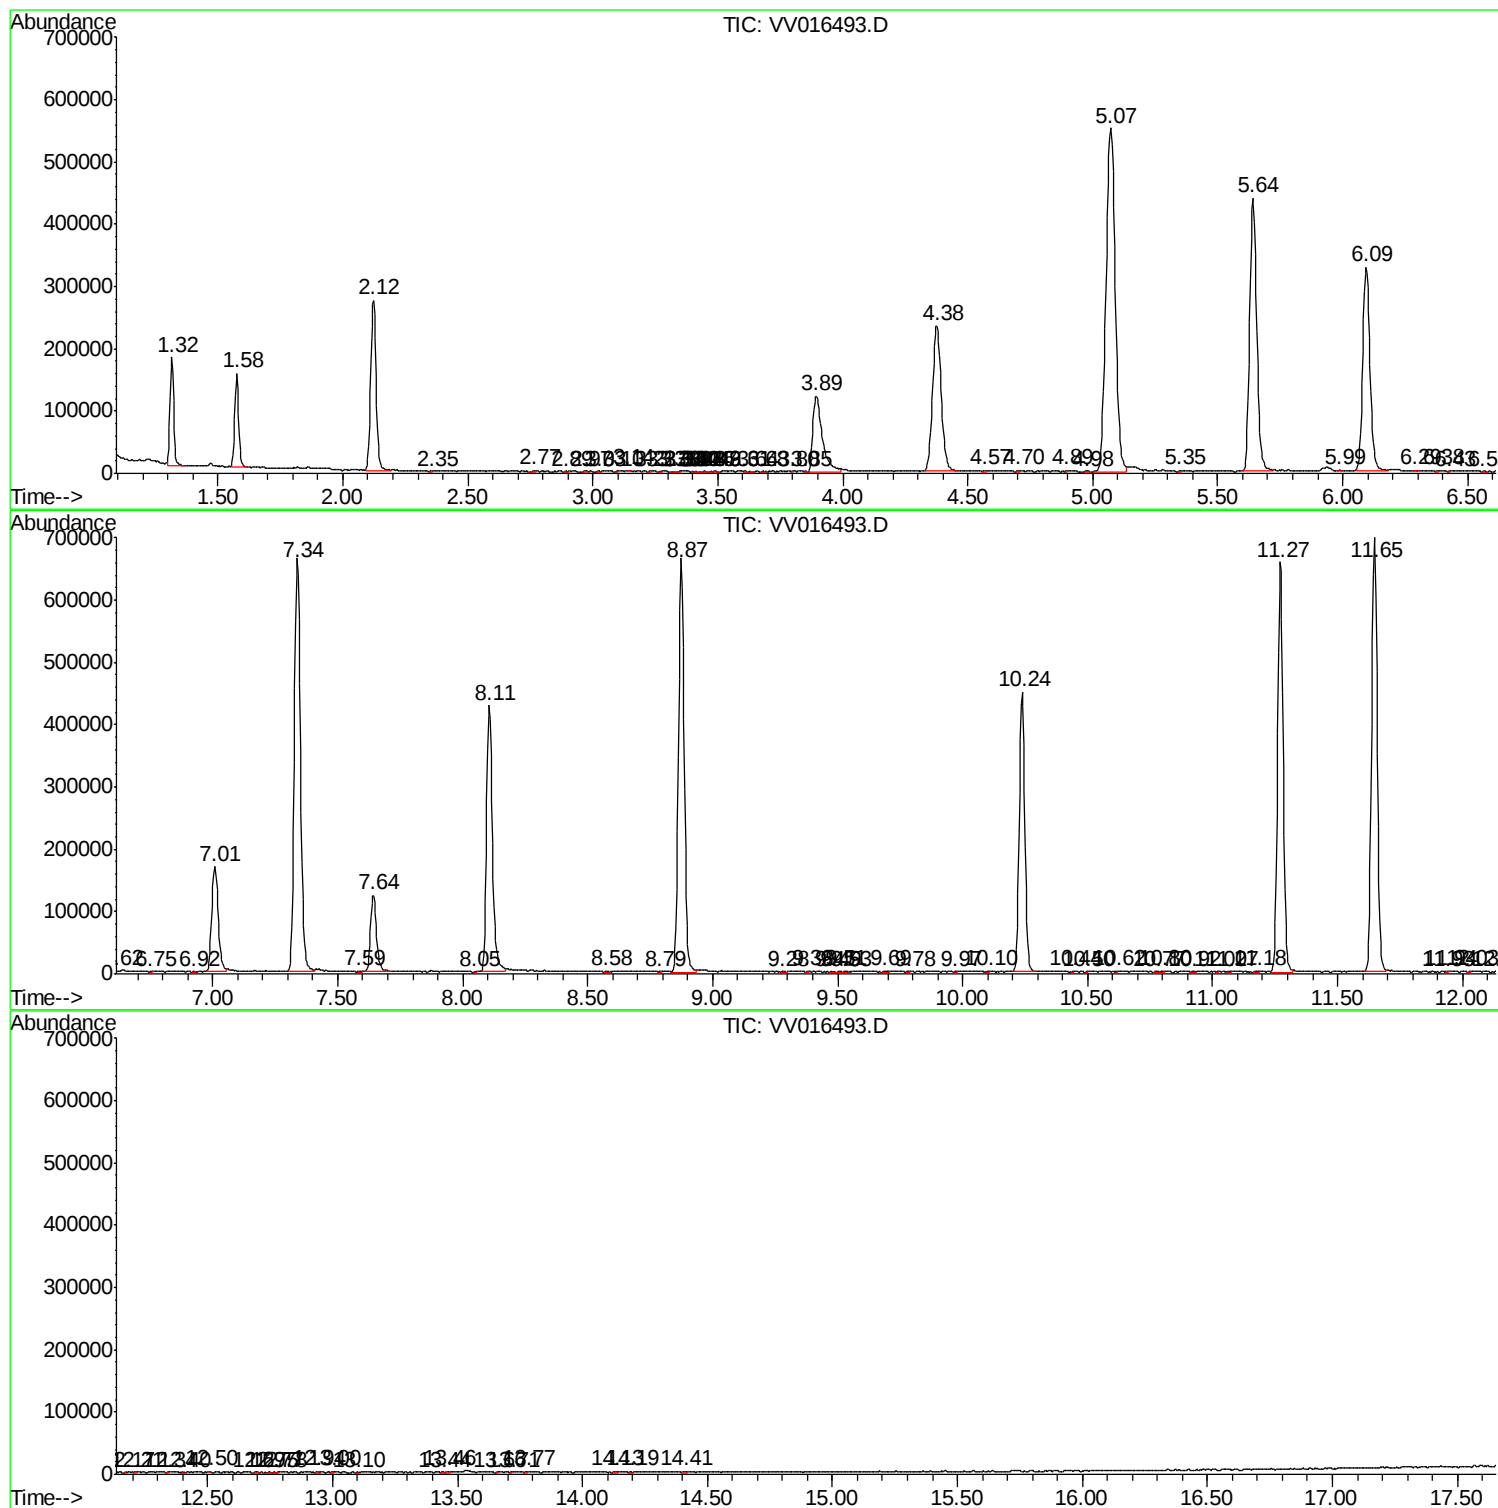

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016493.D
Acq On : 04 Jun 2020 06:23
Operator : SY/MD
Sample : L2861-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D79

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016493.D
Acq On : 04 Jun 2020 06:23
Operator : SY/MD
Sample : L2861-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D79

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc