


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV060320\
 Data File : VV016427.D
 Acq On : 02 Jun 2020 14:00
 Operator : SY/MD
 Sample : BFB78
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB78

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis
 Last Update : Wed Jun 03 01:20:33 2020

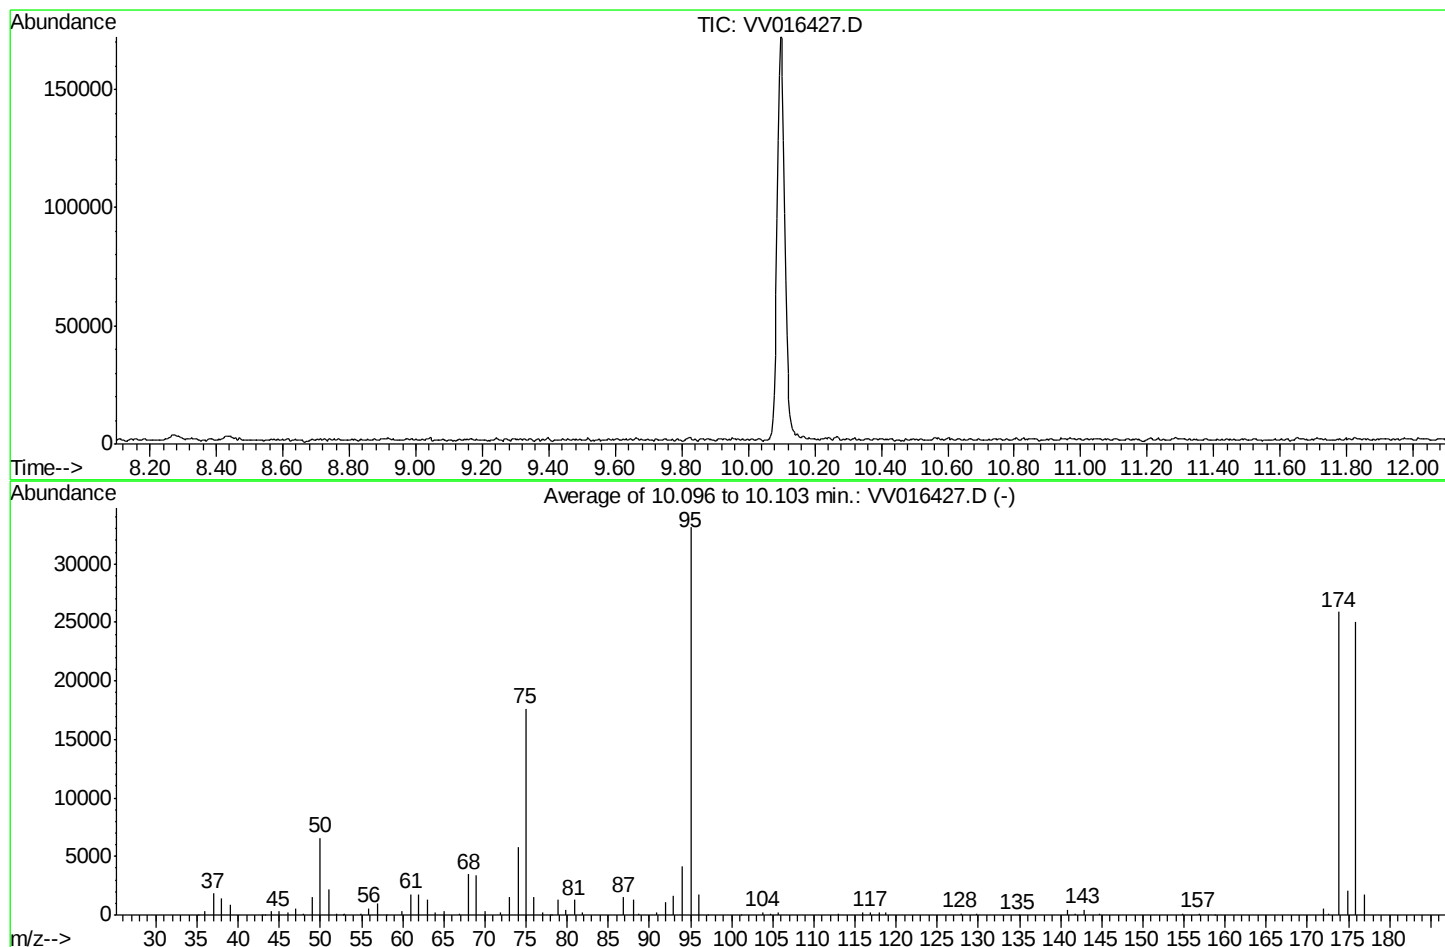

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	6595	PASS
75	95	30	80	53.3	17662	PASS
95	95	100	100	100.0	33125	PASS
96	95	5	9	5.2	1739	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.1	25885	PASS
175	174	5	9	8.0	2075	PASS
176	174	95	101	96.9	25077	PASS
177	176	5	9	6.8	1703	PASS

m/z	Abundance
35.90	503.0
37.00	1871.0
38.00	1550.0
39.00	845.0
39.90	372.0
41.20	132.0
42.90	117.0
44.00	739.0
44.80	320.0
46.20	166.0
47.00	501.0
47.90	316.0
49.00	1544.0
50.00	7046.0
51.00	2161.0
51.90	122.0
52.70	116.0
53.00	128.0
54.90	172.0
55.90	533.0
57.00	1020.0
59.90	344.0
61.00	1854.0
62.00	1765.0
63.00	1421.0
64.00	251.0
65.00	361.0
66.90	120.0
68.00	3685.0
69.00	3538.0
70.00	310.0
71.80	289.0
73.00	1705.0
74.00	5933.0
75.00	18688.0
76.00	1612.0
76.90	241.0
77.90	138.0
78.90	1308.0
79.80	412.0
80.90	1332.0
81.80	225.0
86.90	1560.0
88.00	1366.0
88.80	113.0
90.90	191.0
91.90	1036.0
93.00	1880.0
94.00	4259.0
95.00	34208.0
96.00	1814.0
101.10	103.0
103.90	270.0
104.80	111.0
105.70	199.0
116.00	196.0
116.90	269.0
118.00	199.0
118.70	262.0
127.80	174.0
129.80	107.0
140.80	462.0
141.70	117.0
142.80	486.0
154.80	123.0
156.70	113.0
172.00	443.0
172.60	193.0
173.90	26448.0
174.90	2148.0
175.90	25784.0
176.90	1756.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.90	507.0
37.00	1846.0
38.00	1583.0
39.00	862.0
39.90	399.0
41.20	134.0
43.90	732.0
44.90	301.0
46.00	142.0
46.10	143.0
46.90	558.0
47.90	264.0
49.00	1598.0
50.00	6814.0
51.00	2261.0
52.00	130.0
53.00	120.0
54.90	172.0
55.90	592.0
57.00	975.0
59.90	344.0
61.00	1829.0
62.00	1764.0
63.00	1387.0
64.00	213.0
65.00	361.0
67.10	124.0
68.00	3549.0
69.00	3494.0
70.00	302.0
71.90	282.0
73.00	1628.0
74.00	6097.0
75.00	18208.0
76.00	1574.0
77.00	231.0
78.90	1308.0
79.90	415.0
80.80	1349.0
81.90	236.0
86.90	1531.0
88.00	1427.0
88.70	158.0
90.90	222.0
91.90	1069.0
93.00	1627.0
94.00	4247.0
95.00	34392.0
96.00	1770.0
103.90	271.0
104.70	119.0
105.70	208.0
113.00	109.0
116.00	196.0
116.90	267.0
117.90	189.0
118.80	245.0
127.90	151.0
129.80	115.0
140.80	423.0
141.70	117.0
142.90	465.0
144.70	105.0
154.80	100.0
156.80	119.0
158.70	112.0
172.00	538.0
173.90	26528.0
174.90	2154.0
175.90	25976.0
176.90	1761.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.20	106.0
36.00	473.0
37.00	1734.0
38.00	1492.0
39.00	820.0
39.90	409.0
41.30	122.0
43.30	104.0
44.00	685.0
45.00	271.0
45.90	130.0
46.90	552.0
47.90	218.0
49.00	1523.0
50.00	5927.0
51.00	2022.0
52.00	151.0
52.90	113.0
54.80	141.0
55.90	535.0
57.00	893.0
58.00	110.0
59.90	349.0
61.00	1587.0
62.00	1643.0
63.00	1216.0
63.80	197.0
65.00	300.0
66.80	117.0
67.20	110.0
68.00	3120.0
69.00	3092.0
70.00	231.0
71.90	235.0
72.90	1418.0
74.00	5532.0
75.00	16090.0
76.00	1347.0
77.10	182.0
78.10	143.0
78.90	1230.0
79.90	392.0
80.80	1190.0
81.80	249.0
86.90	1358.0
88.00	1303.0
88.70	135.0
90.90	230.0
91.90	1033.0
92.90	1354.0
94.00	3941.0
95.00	30776.0
96.00	1633.0
97.10	104.0
103.80	253.0
104.70	106.0
105.70	204.0
113.00	106.0
115.90	193.0
116.90	253.0
117.90	151.0
118.90	232.0
127.90	142.0
129.90	126.0
134.90	103.0
140.80	368.0
142.90	448.0
144.70	105.0
156.90	136.0
172.00	530.0
173.90	24680.0
175.00	1925.0
175.90	23472.0
176.90	1593.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
36.00	137.0
37.90	129.0
39.90	419.0
41.30	170.0
44.00	432.0
45.80	117.0
48.10	101.0
56.20	111.0
67.10	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78