


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016449.D
 Acq On : 03 Jun 2020 09:44
 Operator : SY/MD
 Sample : BFB79
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB79

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis
 Last Update : Thu Jun 04 05:34:42 2020

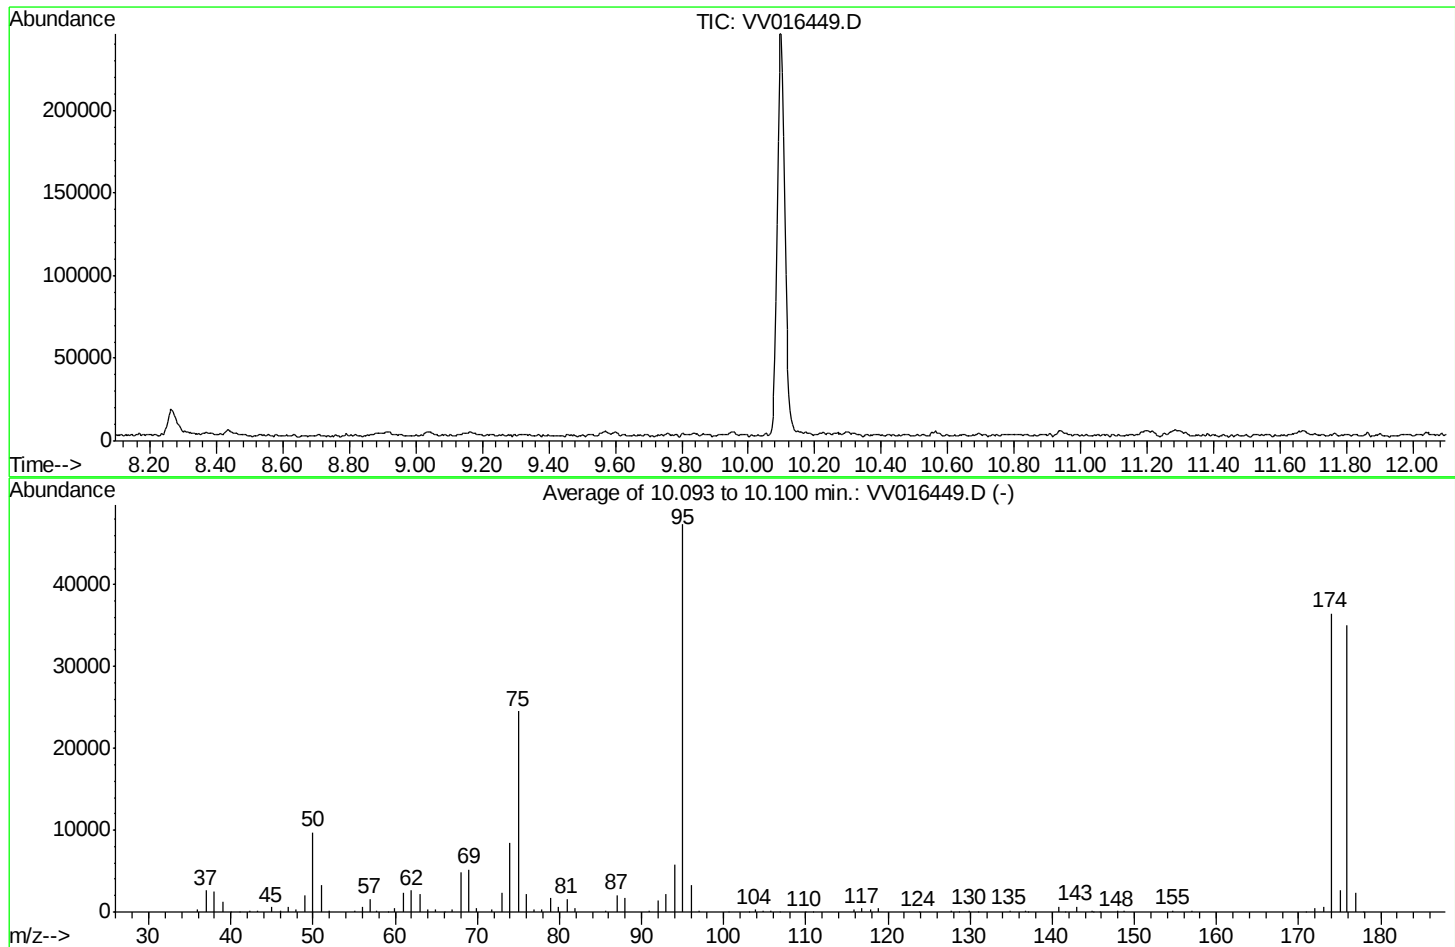

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	9730	PASS
75	95	30	80	51.8	24557	PASS
95	95	100	100	100.0	47378	PASS
96	95	5	9	6.8	3220	PASS
173	174	0.00	2	1.8	645	PASS
174	95	50	120	77.0	36488	PASS
175	174	5	9	7.5	2738	PASS
176	174	95	101	95.9	35002	PASS
177	176	5	9	6.7	2357	PASS

m/z	Abundance
36.00	544.0
37.00	2583.0
38.00	2461.0
39.00	1087.0
39.90	422.0
41.10	121.0
41.90	114.0
42.40	118.0
43.20	167.0
43.90	699.0
44.90	554.0
46.00	165.0
47.00	654.0
47.90	380.0
49.00	2017.0
50.00	9539.0
51.00	3112.0
52.00	215.0
55.10	195.0
56.00	708.0
57.00	1465.0
57.80	104.0
59.90	536.0
61.00	2315.0
61.90	2517.0
63.00	2007.0
63.90	247.0
64.90	317.0
66.00	102.0
66.90	252.0
68.00	4815.0
69.00	5114.0
69.90	474.0
71.80	311.0
73.00	2066.0
74.00	7921.0
75.00	22928.0
76.00	1996.0
76.90	384.0
77.80	282.0
78.90	1593.0
79.90	550.0
80.90	1530.0
81.90	474.0
85.60	184.0
87.00	2173.0
87.90	1709.0
90.80	162.0
92.00	1405.0
93.00	2043.0
94.00	5461.0
95.00	44336.0
96.00	2965.0
97.00	230.0
100.60	125.0
103.10	117.0
103.90	292.0
104.80	156.0
105.70	210.0
115.90	240.0
116.80	442.0
117.90	285.0
118.90	421.0
123.80	105.0
127.80	199.0
129.90	237.0
134.80	206.0
136.80	146.0
140.80	536.0
141.60	121.0
142.90	646.0
144.80	161.0
145.80	104.0
147.90	125.0
148.80	174.0
154.70	147.0
156.90	112.0
171.90	442.0
173.00	659.0
173.90	33256.0
175.00	2532.0
175.90	31600.0
177.00	2136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
36.00	537.0
37.00	2720.0
38.00	2549.0
39.00	1242.0
39.90	441.0
41.10	145.0
41.80	113.0
42.30	141.0
43.20	198.0
43.90	710.0
44.90	579.0
46.00	163.0
47.00	674.0
48.00	374.0
49.00	2270.0
50.00	10195.0
51.00	3362.0
51.90	211.0
55.10	211.0
56.00	668.0
57.00	1714.0
57.80	122.0
59.90	653.0
61.00	2418.0
62.00	2687.0
63.00	2237.0
64.00	326.0
64.90	303.0
66.80	272.0
68.00	5048.0
69.00	5348.0
69.90	460.0
71.80	342.0
73.00	2424.0
74.00	8704.0
75.00	25472.0
76.00	2179.0
76.90	390.0
77.80	324.0
78.90	1788.0
79.90	574.0
80.90	1688.0
81.90	509.0
85.60	146.0
87.00	2183.0
87.90	1786.0
90.80	161.0
92.00	1518.0
93.00	2334.0
94.00	6017.0
95.00	48960.0
96.00	3317.0
97.00	206.0
103.10	101.0
103.90	258.0
104.70	173.0
105.80	230.0
106.80	105.0
109.90	119.0
115.90	273.0
116.80	453.0
117.90	312.0
118.80	475.0
127.70	232.0
129.90	251.0
134.80	192.0
136.70	156.0
140.80	622.0
141.60	122.0
142.90	738.0
144.80	138.0
147.90	157.0
148.80	116.0
154.70	187.0
157.00	150.0
172.00	499.0
173.00	653.0
173.90	37656.0
175.00	2808.0
175.90	36184.0
177.00	2392.0
177.90	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
36.00	462.0
37.00	2667.0
38.00	2500.0
39.00	1356.0
39.90	507.0
41.10	193.0
41.70	125.0
42.30	161.0
43.20	172.0
44.00	708.0
44.90	566.0
46.00	162.0
47.00	702.0
48.00	374.0
49.00	2236.0
50.00	9456.0
51.00	3299.0
51.90	241.0
54.90	208.0
56.10	632.0
56.90	1758.0
57.80	143.0
59.20	134.0
60.00	689.0
61.00	2264.0
62.00	2610.0
63.00	2256.0
64.00	386.0
64.80	286.0
66.00	103.0
66.80	226.0
68.00	4806.0
69.00	5132.0
69.90	404.0
71.80	317.0
73.00	2523.0
74.00	8644.0
75.00	25272.0
76.00	2279.0
76.90	332.0
77.80	330.0
78.90	1781.0
79.90	545.0
80.90	1646.0
81.90	480.0
85.50	121.0
86.90	1928.0
87.90	1775.0
90.90	204.0
91.90	1550.0
93.00	2388.0
94.00	5935.0
95.00	48840.0
96.00	3378.0
97.00	190.0
103.70	229.0
104.70	214.0
105.90	248.0
106.80	125.0
110.80	107.0
115.90	290.0
116.80	456.0
117.80	330.0
118.80	434.0
127.80	197.0
128.70	130.0
129.90	213.0
130.90	127.0
134.90	151.0
136.70	135.0
137.10	136.0
140.90	647.0
142.90	720.0
145.00	115.0
147.90	140.0
154.70	178.0
157.10	152.0
170.80	105.0
172.00	425.0
173.00	625.0
173.90	38552.0
175.00	2874.0
175.90	37224.0
176.90	2544.0
177.80	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.80	134.0
36.60	113.0
37.70	141.0
38.30	215.0
39.30	228.0
40.00	392.0
41.00	135.0
41.90	188.0
42.60	142.0
42.80	137.0
44.00	732.0
45.20	105.0
45.70	125.0
48.00	135.0
49.00	131.0
49.70	111.0
50.50	156.0
52.20	112.0
54.50	152.0
55.30	108.0
60.00	154.0
62.60	107.0
70.50	113.0
76.80	108.0
85.00	161.0
115.60	129.0
126.40	103.0
157.90	129.0
166.20	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79