
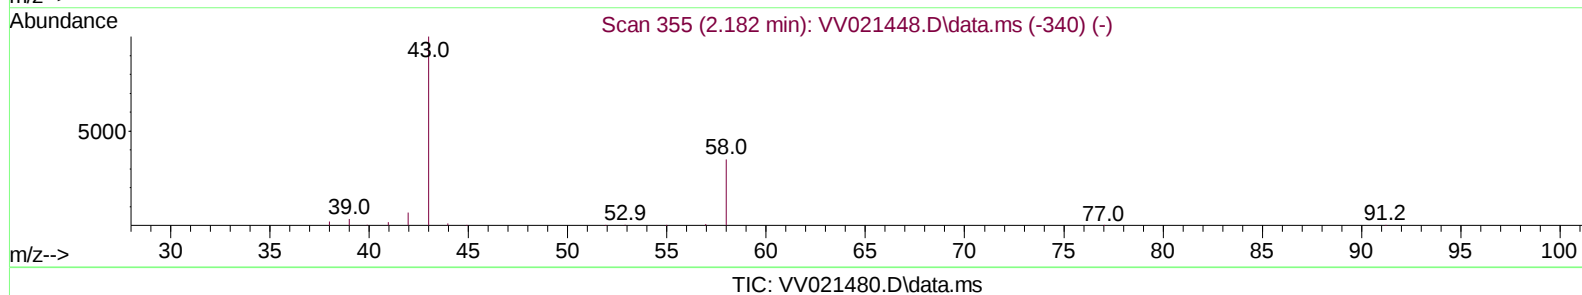
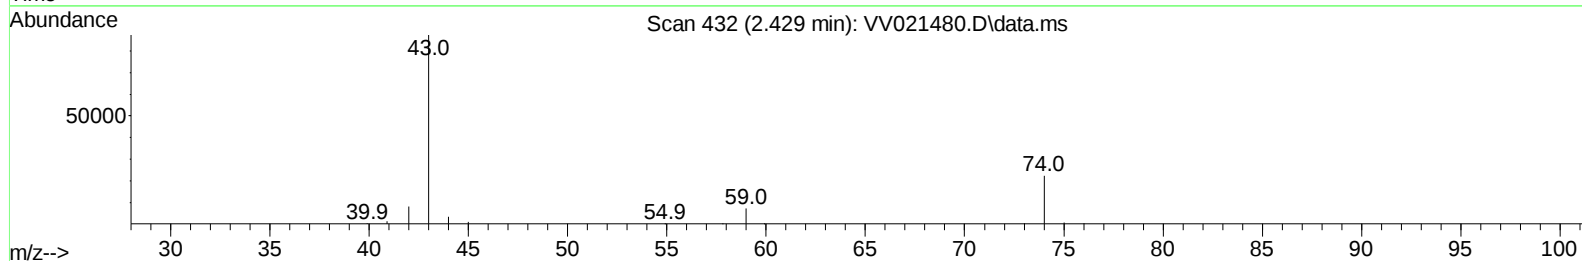


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021480.D
 Acq On : 03 Jun 2021 10:37
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jun 04 03:03:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 29 00:49:04 2021
 Response via : Initial Calibration

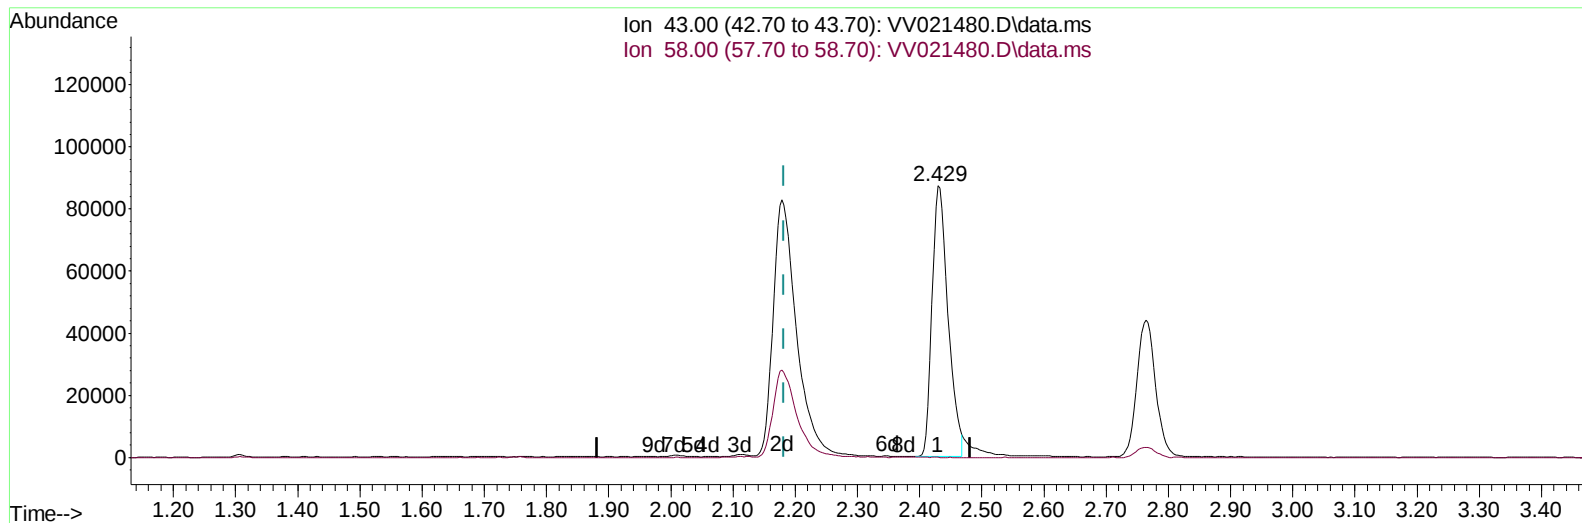

(13) Acetone (T)

2.429min (+ 0.248) 76.97 ug/L

response 156591

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	0.10	0.07
0.00	0.00	0.00
0.00	0.00	0.00