

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021481.D
 Acq On : 03 Jun 2021 11:21
 Operator : SY/MD
 Sample : VV0603MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 04 03:07:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 04 03:06:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	495296	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	471818	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	268804	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	138424	42.449	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	84.900%	
7) Chloroethane-d5	1.564	69	111318	45.890	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	91.780%	
11) 1,1-Dichloroethene-d2	2.101	63	188548	33.838	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	67.680%	
21) 2-Butanone-d5	3.883	46	212786	90.998	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	91.000%	
24) Chloroform-d	4.343	84	301410	46.432	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.860%	
26) 1,2-Dichloroethane-d4	5.027	65	180814	48.360	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.720%	
32) Benzene-d6	5.043	84	619942	46.968	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.940%	
36) 1,2-Dichloropropane-d6	6.066	67	194218	47.648	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	95.300%	
41) Toluene-d8	7.313	98	590276	46.940	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	93.880%	
43) trans-1,3-Dichloroprop...	7.619	79	100292	45.976	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.960%	
47) 2-Hexanone-d5	8.085	63	162279	86.702	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	86.700%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	262745	46.436	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	92.880%	
66) 1,2-Dichlorobenzene-d4	11.625	152	267350	47.846	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.700%	
Target Compounds						
					Qvalue	
39) cis-1,3-Dichloropropene	6.985	75	6086	1.051	ug/L #	64
44) trans-1,3-Dichloropropene	7.619	75	4159	0.759	ug/L #	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021481.D
Acq On : 03 Jun 2021 11:21
Operator : SY/MD
Sample : VV0603MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jun 04 03:07:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 04 03:06:56 2021
Response via : Initial Calibration

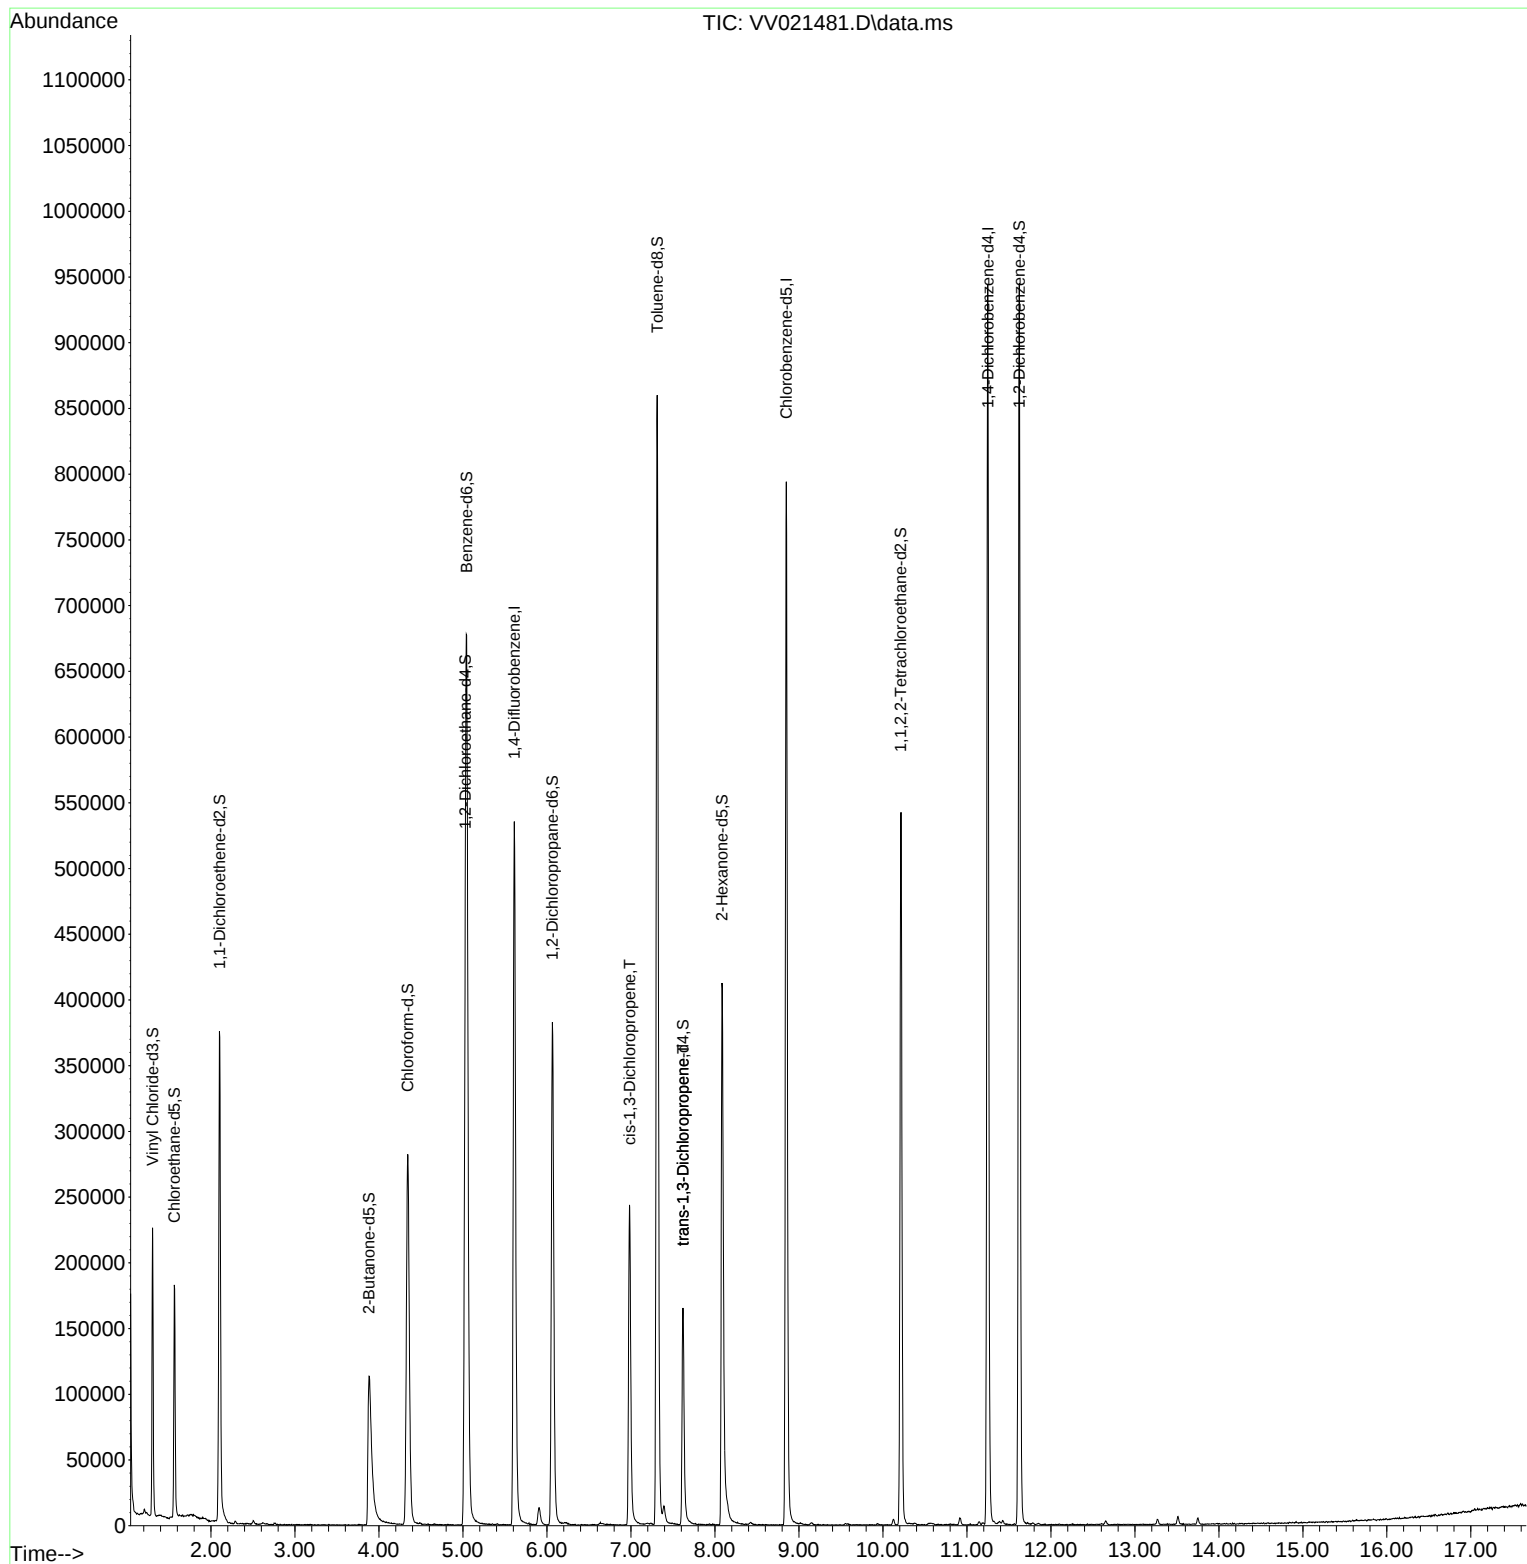




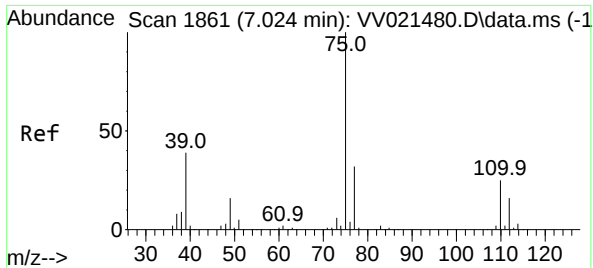


#39

cis-1,3-Dichloropropene
Concen: 1.051 ug/L
RT: 6.985 min Scan# 1849
Delta R.T. -0.039 min
Lab File: VV021481.D
Acq: 03 Jun 2021 11:21

Instrument :
MSVOA_V
ClientSampled :

Tgt Ion: 75 Resp: 6086
Ion Ratio Lower Upper
75 100
77 51.2 22.0 41.0#

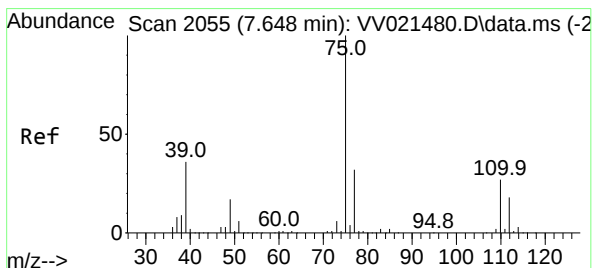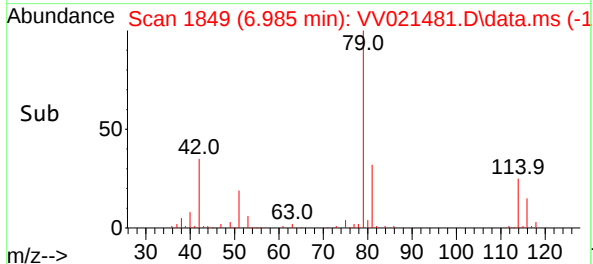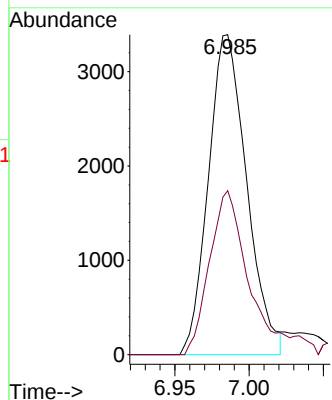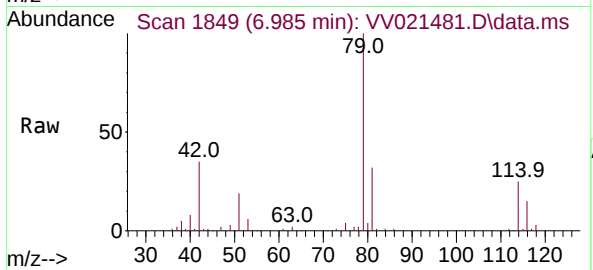

#44

trans-1,3-Dichloropropene
Concen: 0.759 ug/L
RT: 7.619 min Scan# 2046
Delta R.T. -0.029 min
Lab File: VV021481.D
Acq: 03 Jun 2021 11:21

Tgt Ion: 75 Resp: 4159
Ion Ratio Lower Upper
75 100
77 45.0 22.9 42.5#

