

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021482.D
 Acq On : 03 Jun 2021 11:44
 Operator : SY/MD
 Sample : VV0603WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 04 03:07:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 04 03:06:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	486662	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	458166	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	258216	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	133859	41.777	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.560%
7) Chloroethane-d5	1.568	69	106859	44.833	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.660%
11) 1,1-Dichloroethene-d2	2.108	63	182576	33.347	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.700%
21) 2-Butanone-d5	3.886	46	227959	99.216	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.220%
24) Chloroform-d	4.352	84	299730	46.992	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.980%
26) 1,2-Dichloroethane-d4	5.034	65	181126	49.302	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.600%
32) Benzene-d6	5.053	84	614601	47.951	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.900%
36) 1,2-Dichloropropane-d6	6.072	67	192115	48.536	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.080%
41) Toluene-d8	7.317	98	580511	47.539	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.080%
43) trans-1,3-Dichloroprop...	7.625	79	99820	47.124	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.240%
47) 2-Hexanone-d5	8.088	63	171079	94.127	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.130%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	268153	48.804	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	263644	49.117	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.240%
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.622	75	4316	0.812	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021482.D
Acq On : 03 Jun 2021 11:44
Operator : SY/MD
Sample : VV0603WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jun 04 03:07:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 04 03:06:56 2021
Response via : Initial Calibration

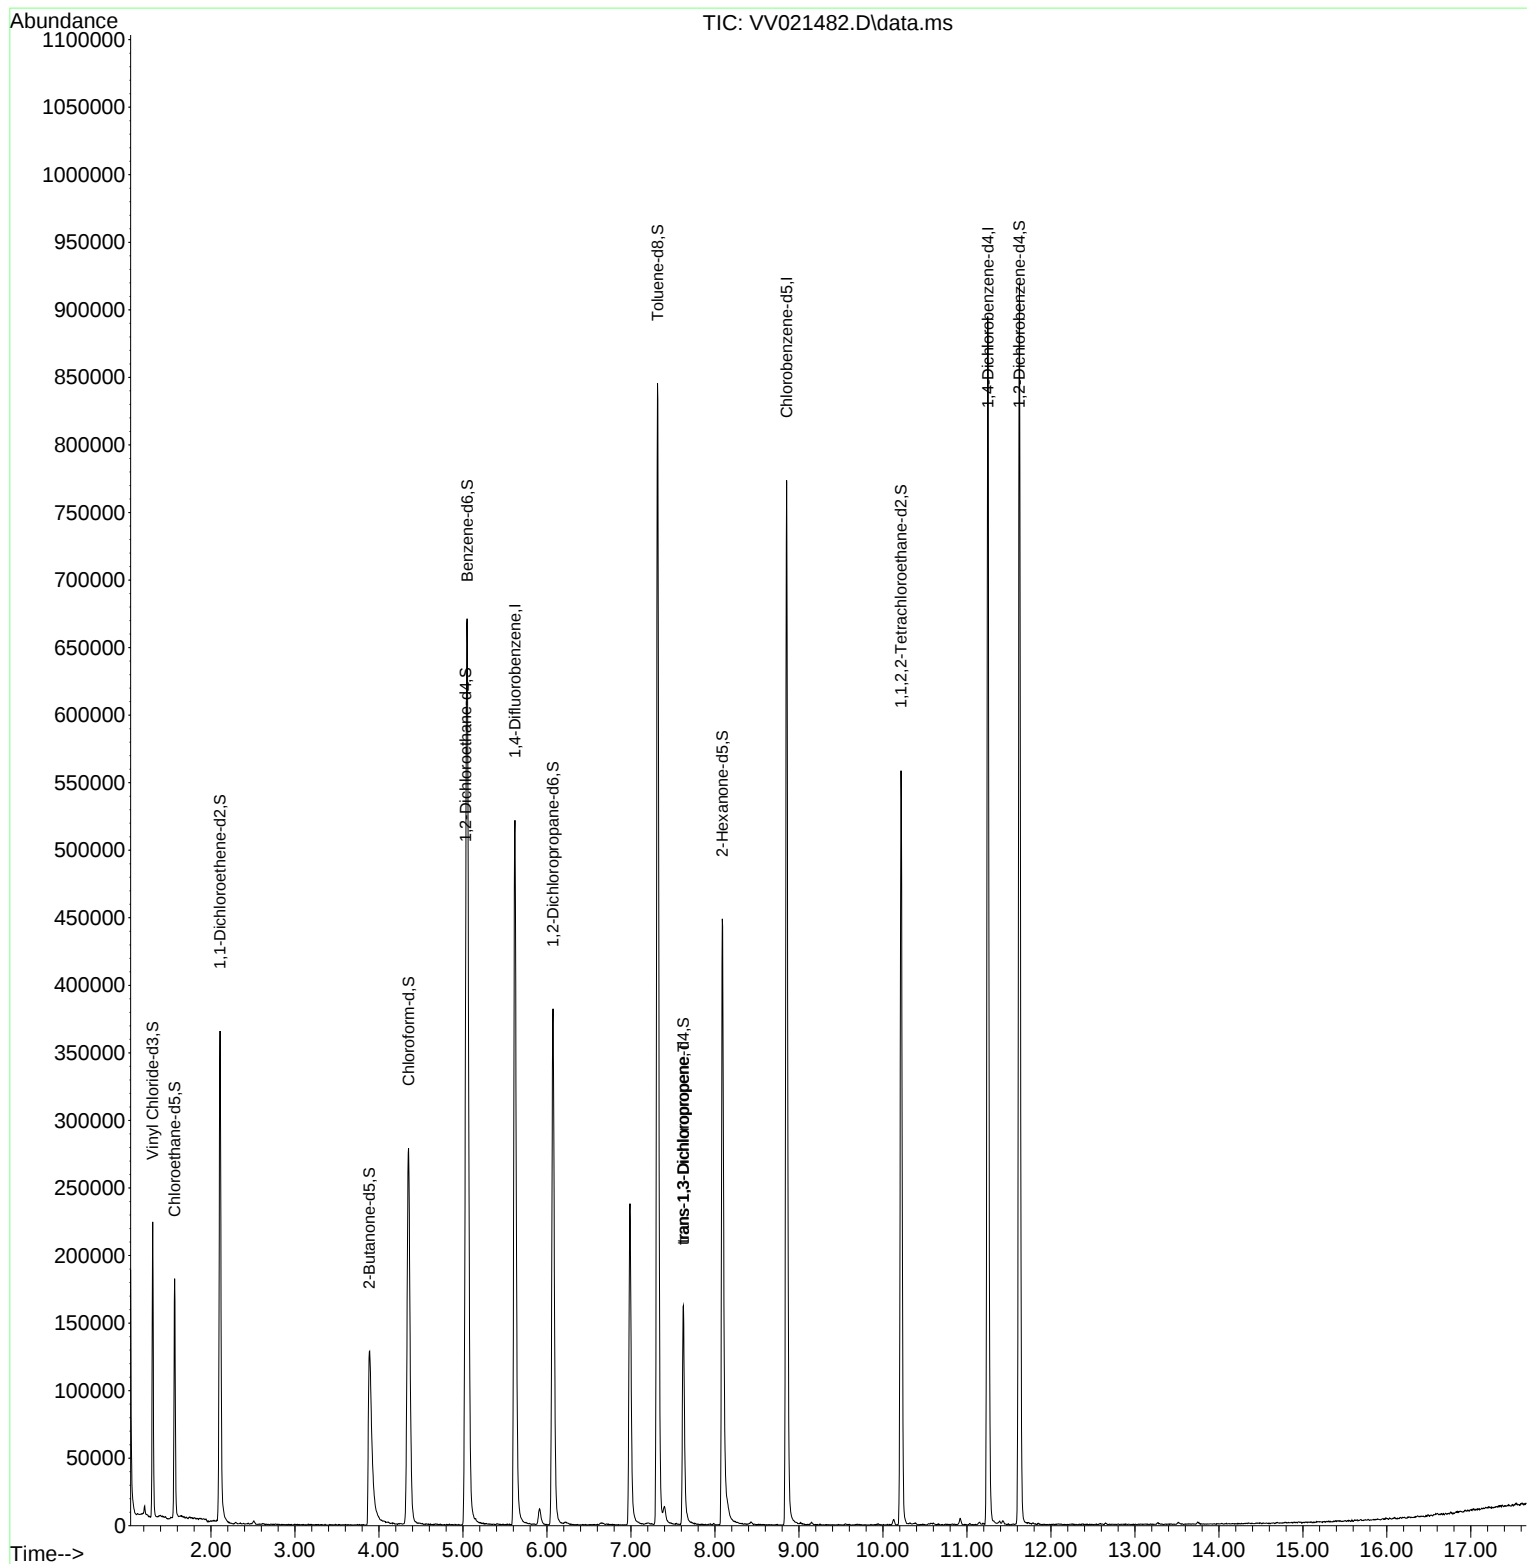

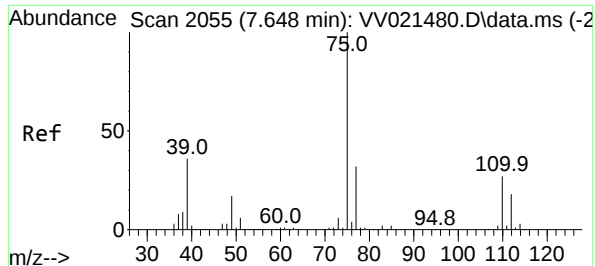

#44
 trans-1,3-Dichloropropene
 Concen: 0.812 ug/L
 RT: 7.622 min Scan# 2047
 Delta R.T. -0.026 min
 Lab File: VV021482.D
 Acq: 03 Jun 2021 11:44

Instrument :
 MSVOA_V
 ClientSampleId :

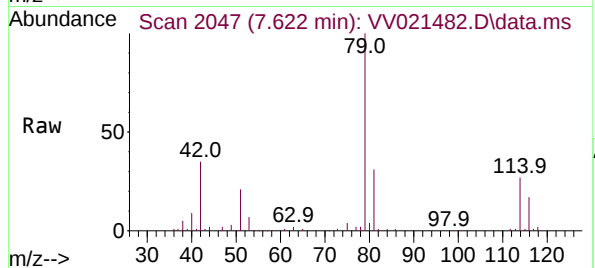

Tgt Ion: 75 Resp: 4316
 Ion Ratio Lower Upper
 75 100
 77 35.7 22.9 42.5

