

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021484.D
 Acq On : 03 Jun 2021 14:00
 Operator : SY/MD
 Sample : M2605-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 04 03:07:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 04 03:06:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	498101	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	466230	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	260509	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	129753	39.566	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	79.140%		
7) Chloroethane-d5	1.568	69	106193	43.530	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.060%		
11) 1,1-Dichloroethene-d2	2.108	63	176234	31.450	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.900%		
21) 2-Butanone-d5	3.892	46	236226	100.453	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	100.450%		
24) Chloroform-d	4.352	84	289229	44.305	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.600%		
26) 1,2-Dichloroethane-d4	5.034	65	176597	46.966	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.940%		
32) Benzene-d6	5.053	84	586498	44.967	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.940%		
36) 1,2-Dichloropropane-d6	6.072	67	184616	45.835	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.660%		
41) Toluene-d8	7.317	98	560984	45.145	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.300%		
43) trans-1,3-Dichloroprop...	7.625	79	95490	44.300	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.600%		
47) 2-Hexanone-d5	8.088	63	174946	94.590	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	94.590%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	263899	47.199	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.400%		
66) 1,2-Dichlorobenzene-d4	11.625	152	251706	46.481	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.960%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.989	75	5526	0.966	ug/L #	62
61) 1,2,3-Trichloropropane	11.249	75	24633	6.018	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021484.D
Acq On : 03 Jun 2021 14:00
Operator : SY/MD
Sample : M2605-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jun 04 03:07:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 04 03:06:56 2021
Response via : Initial Calibration




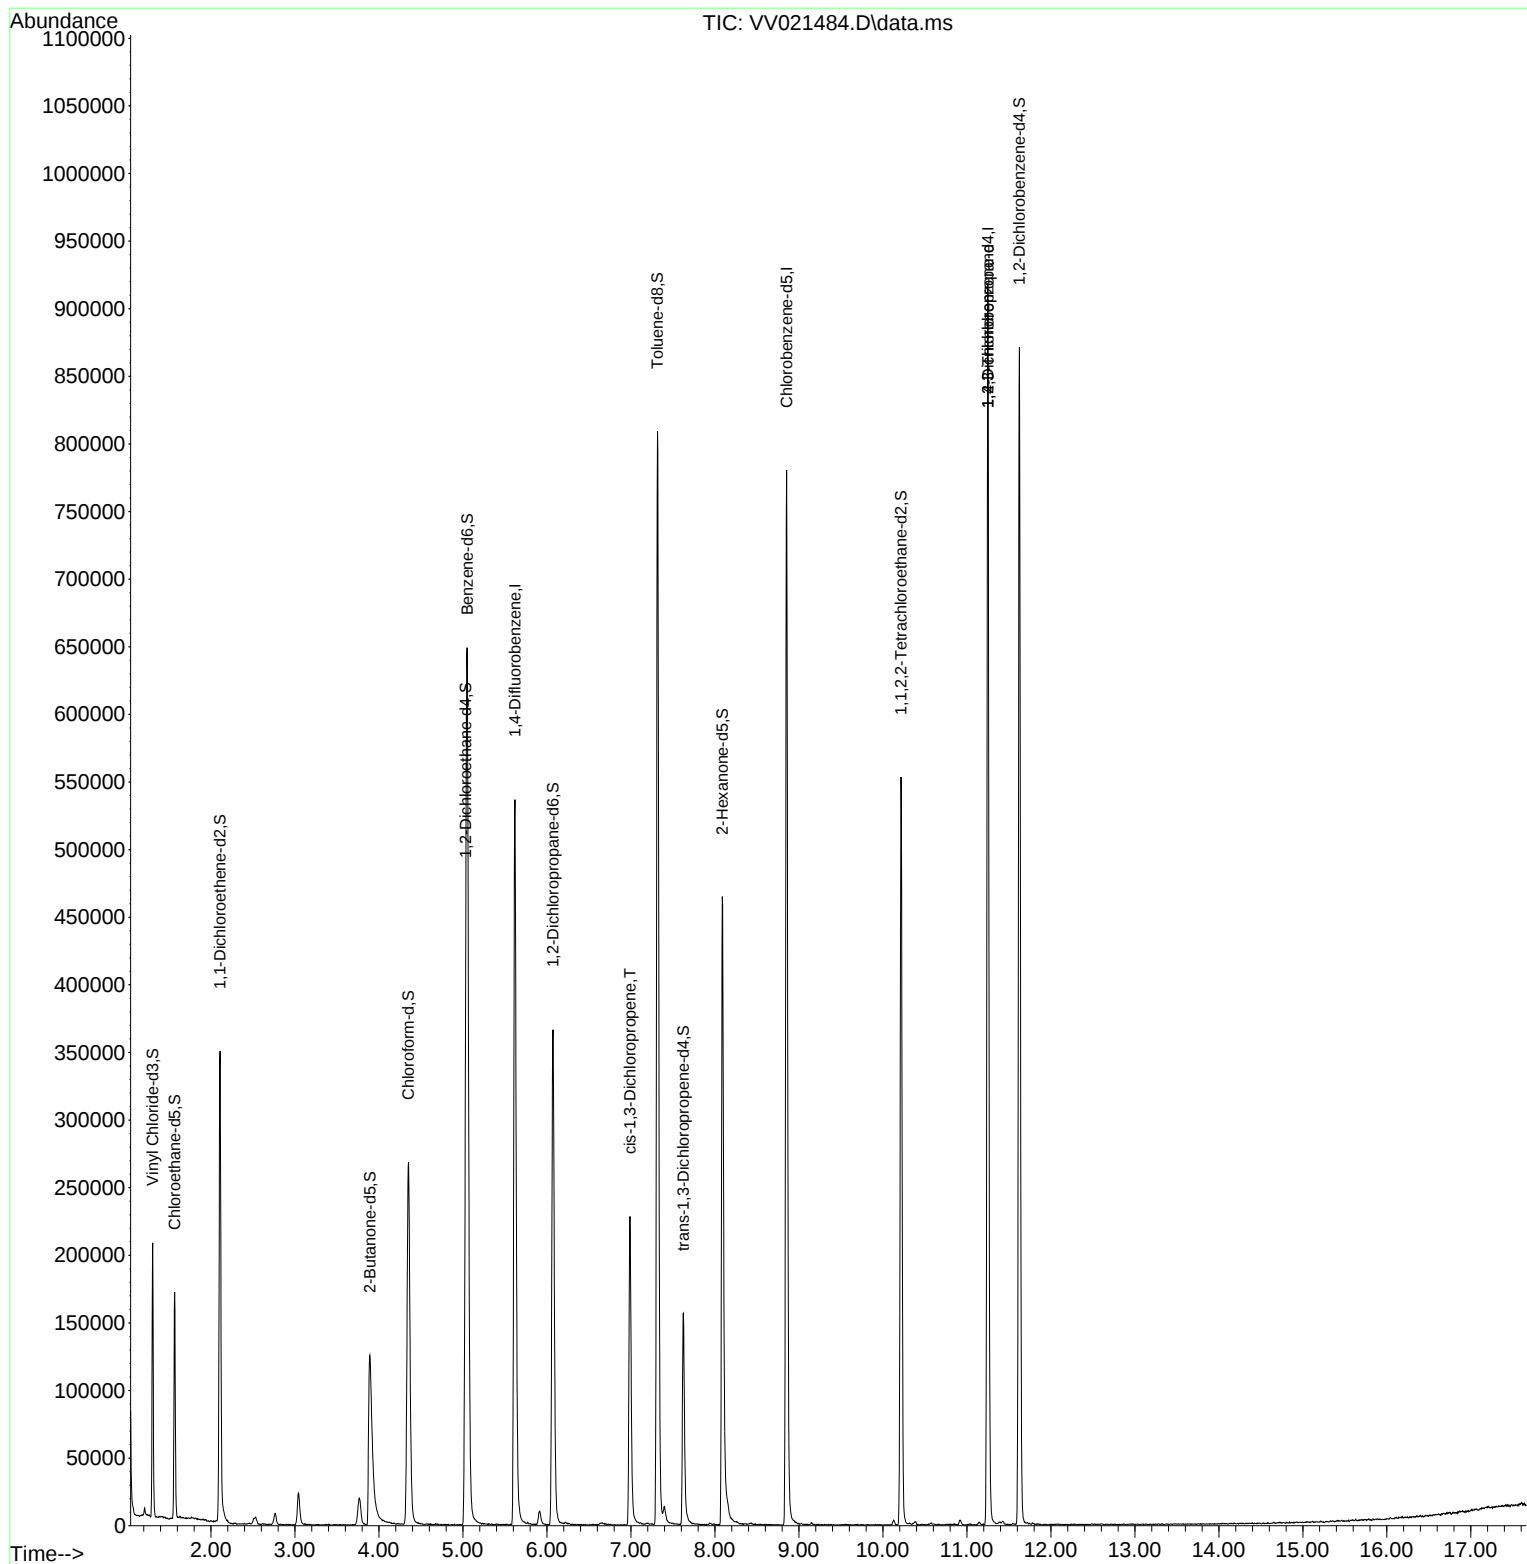


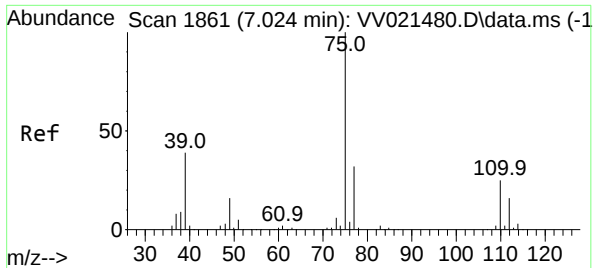

#39
 cis-1,3-Dichloropropene
 Concen: 0.966 ug/L
 RT: 6.989 min Scan# 1850
 Delta R.T. -0.035 min
 Lab File: VV021484.D
 Acq: 03 Jun 2021 14:00

Instrument :
 MSVOA_V
 ClientSampled :

Tgt Ion: 75 Resp: 5526
 Ion Ratio Lower Upper
 75 100
 77 52.6 22.0 41.0#

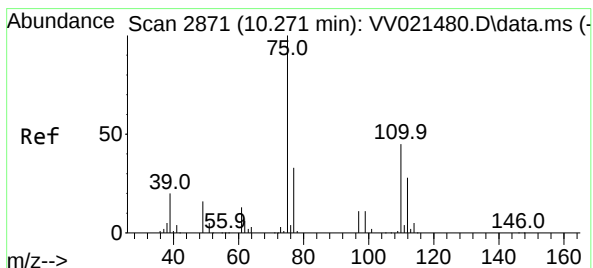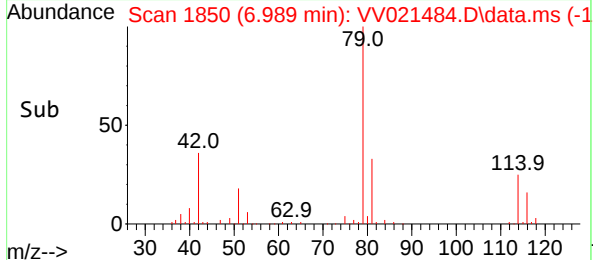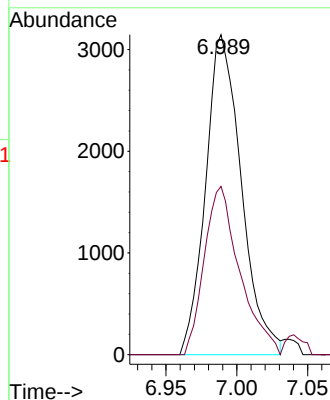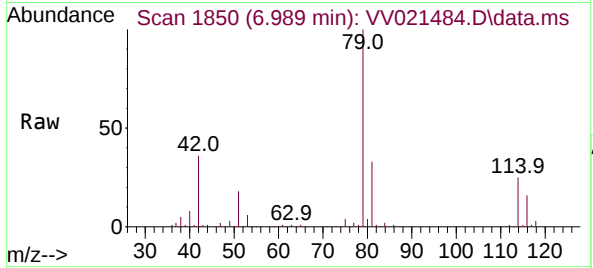

#61
 1,2,3-Trichloropropane
 Concen: 6.018 ug/L
 RT: 11.249 min Scan# 3175
 Delta R.T. 0.978 min
 Lab File: VV021484.D
 Acq: 03 Jun 2021 14:00

Tgt Ion: 75 Resp: 24633
 Ion Ratio Lower Upper
 75 100
 77 32.5 25.9 38.9
 110 2.9 34.8 52.2#

