

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021483.D
 Acq On : 03 Jun 2021 13:36
 Operator : SY/MD
 Sample : M2596-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG5W4

Quant Time: Jun 04 03:07:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 04 03:06:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	493209	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	455848	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	261246	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	129863	39.992	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.980%
7) Chloroethane-d5	1.568	69	108160	44.777	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.560%
11) 1,1-Dichloroethene-d2	2.108	63	178225	32.120	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.240%
21) 2-Butanone-d5	3.895	46	208757	89.652	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.650%
24) Chloroform-d	4.352	84	287373	44.457	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.920%
26) 1,2-Dichloroethane-d4	5.037	65	174913	46.979	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.960%
32) Benzene-d6	5.053	84	588593	46.155	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.320%
36) 1,2-Dichloropropane-d6	6.072	67	185045	46.988	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.980%
41) Toluene-d8	7.317	98	562618	46.308	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.620%
43) trans-1,3-Dichloroprop...	7.625	79	96820	45.940	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.880%
47) 2-Hexanone-d5	8.091	63	150036	82.969	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.970%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	245909	44.984	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.960%
66) 1,2-Dichlorobenzene-d4	11.625	152	256388	47.212	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.420%
Target Compounds						
13) Acetone	2.185	43	12784	6.381	ug/L	Qvalue # 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021483.D
Acq On : 03 Jun 2021 13:36
Operator : SY/MD
Sample : M2596-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG5W4

Quant Time: Jun 04 03:07:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 04 03:06:56 2021
Response via : Initial Calibration

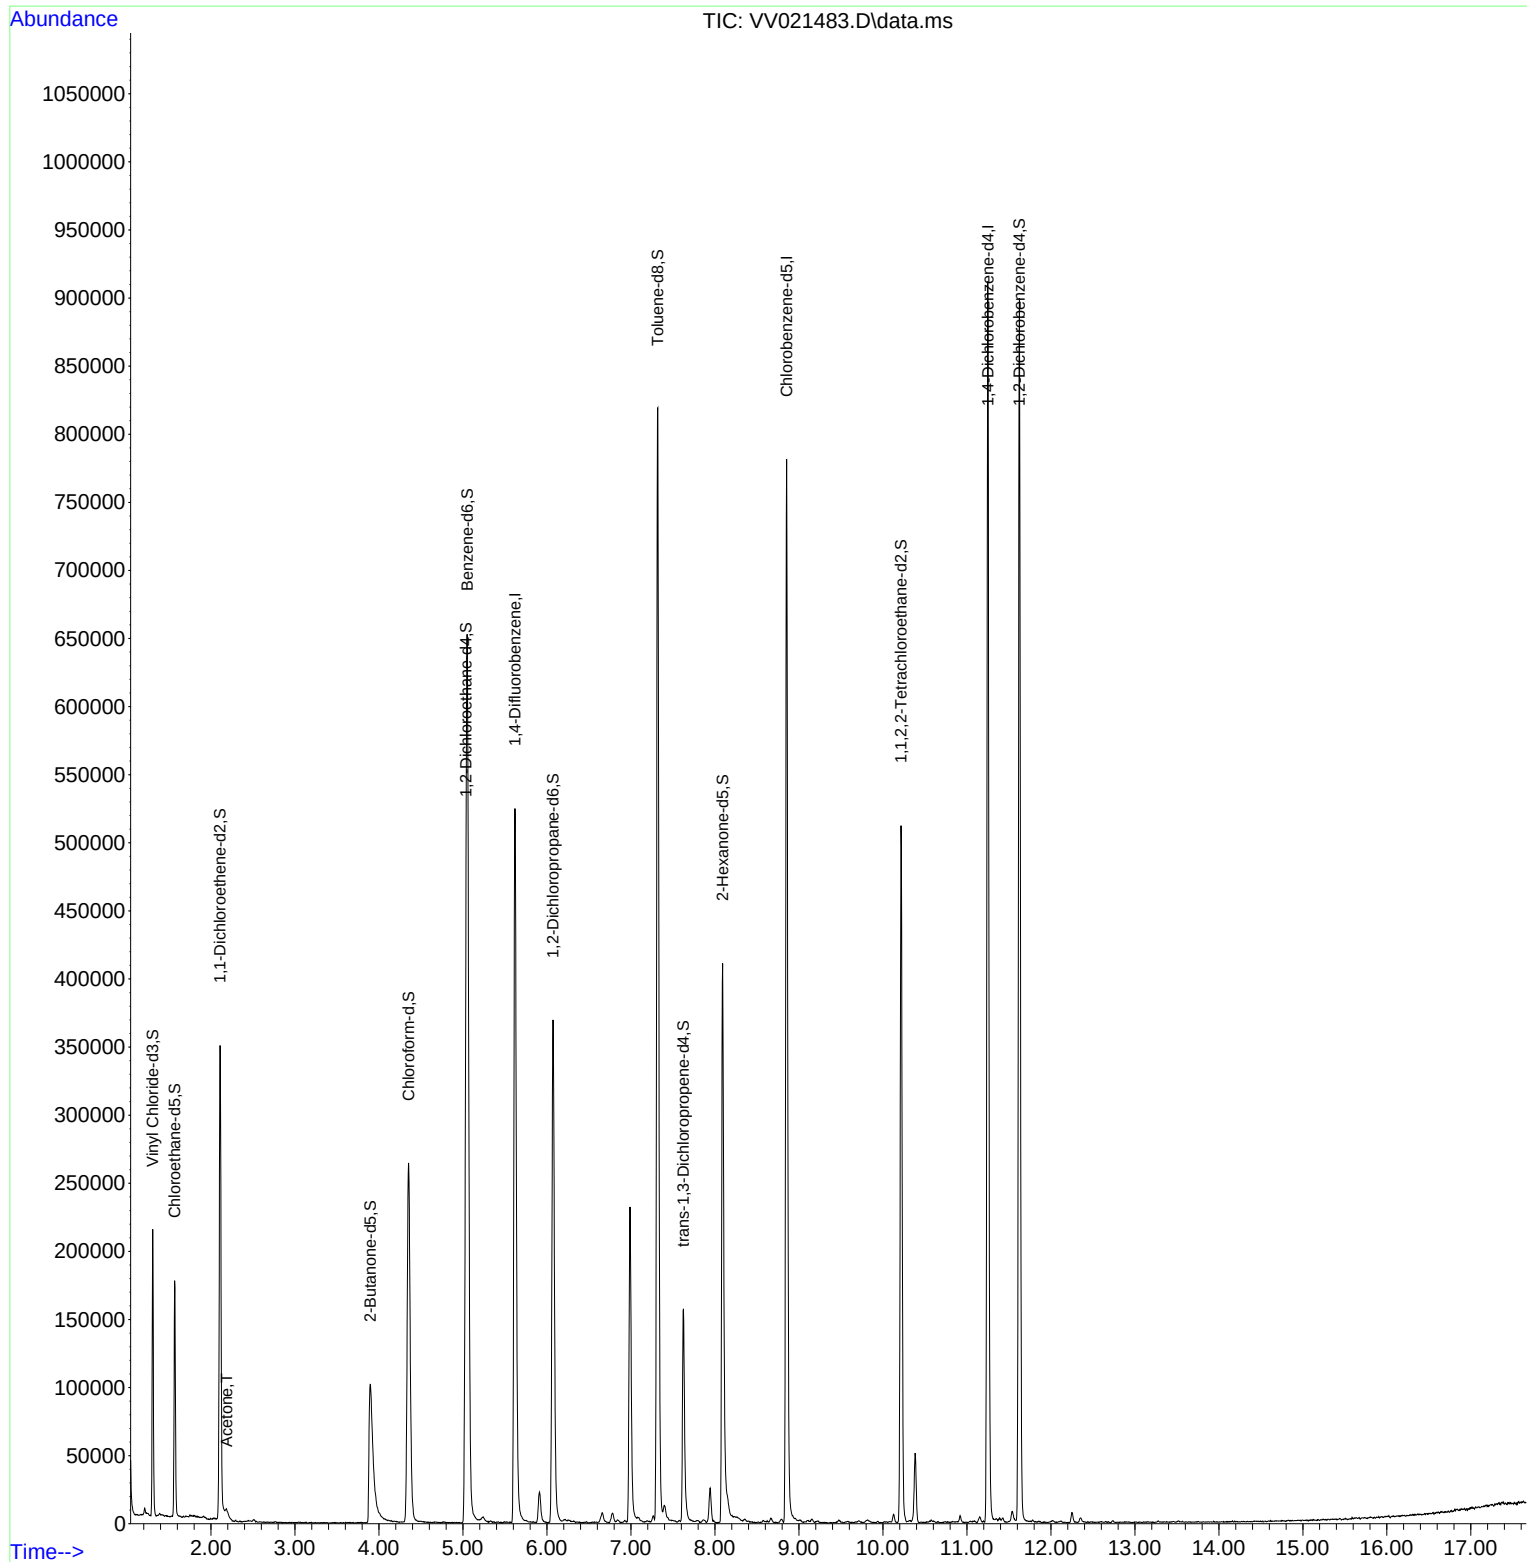

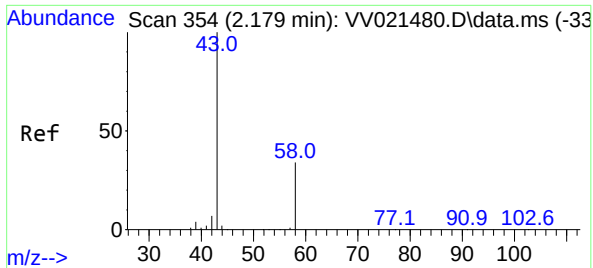

#13
 Acetone
 Concen: 6.381 ug/L
 RT: 2.185 min Scan# 356
 Delta R.T. 0.006 min
 Lab File: VV021483.D
 Acq: 03 Jun 2021 13:36

Instrument :
 MSVOA_V
 ClientSampleId :
 BG5W4

Tgt Ion: 43 Resp: 12784
 Ion Ratio Lower Upper
 43 100
 58 29.9 0.0 0.2#

