

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV060321\  
 Data File : VV021485.D  
 Acq On : 03 Jun 2021 14:23  
 Operator : SY/MD  
 Sample : M2605-01  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BG7H2

Quant Time: Jun 04 03:07:53 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM052721WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Fri Jun 04 03:06:56 2021  
 Response via : Initial Calibration


| Compound                      | R.T.    | QIon  | Response | Conc     | Units | Dev(Min)    |
|-------------------------------|---------|-------|----------|----------|-------|-------------|
| -----                         |         |       |          |          |       |             |
| Internal Standards            |         |       |          |          |       |             |
| 1) 1,4-Difluorobenzene        | 5.619   | 114   | 485418   | 50.000   | ug/L  | 0.00        |
| 28) Chlorobenzene-d5          | 8.854   | 117   | 457379   | 50.000   | ug/L  | 0.00        |
| 58) 1,4-Dichlorobenzene-d4    | 11.249  | 152   | 254955   | 50.000   | ug/L  | 0.00        |
| System Monitoring Compounds   |         |       |          |          |       |             |
| 4) Vinyl Chloride-d3          | 1.304   | 65    | 124202   | 38.862   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 60 - 135 | Recovery | =     | 77.720%     |
| 7) Chloroethane-d5            | 1.568   | 69    | 104986   | 44.160   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 70 - 130 | Recovery | =     | 88.320%     |
| 11) 1,1-Dichloroethene-d2     | 2.108   | 63    | 171001   | 31.313   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 60 - 125 | Recovery | =     | 62.620%     |
| 21) 2-Butanone-d5             | 3.889   | 46    | 216104   | 94.297   | ug/L  | 0.00        |
| Spiked Amount                 | 100.000 | Range | 40 - 130 | Recovery | =     | 94.300%     |
| 24) Chloroform-d              | 4.352   | 84    | 276658   | 43.486   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =     | 86.980%     |
| 26) 1,2-Dichloroethane-d4     | 5.034   | 65    | 170884   | 46.634   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =     | 93.260%     |
| 32) Benzene-d6                | 5.053   | 84    | 573125   | 44.792   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =     | 89.580%     |
| 36) 1,2-Dichloropropane-d6    | 6.072   | 67    | 181508   | 45.935   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 70 - 120 | Recovery | =     | 91.880%     |
| 41) Toluene-d8                | 7.317   | 98    | 539780   | 44.279   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 80 - 120 | Recovery | =     | 88.560%     |
| 43) trans-1,3-Dichloroprop... | 7.625   | 79    | 92018    | 43.515   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 60 - 125 | Recovery | =     | 87.040%     |
| 47) 2-Hexanone-d5             | 8.088   | 63    | 165355   | 91.135   | ug/L  | 0.00        |
| Spiked Amount                 | 100.000 | Range | 45 - 130 | Recovery | =     | 91.130%     |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217  | 84    | 245273   | 44.717   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 65 - 120 | Recovery | =     | 89.440%     |
| 66) 1,2-Dichlorobenzene-d4    | 11.625  | 152   | 247306   | 46.663   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 80 - 120 | Recovery | =     | 93.320%     |
| Target Compounds              |         |       |          |          |       |             |
| 13) Acetone                   | 2.188   | 43    | 11701    | 5.934    | ug/L  | Qvalue # 84 |
| -----                         |         |       |          |          |       |             |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV060321\  
Data File : VV021485.D  
Acq On : 03 Jun 2021 14:23  
Operator : SY/MD  
Sample : M2605-01  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BG7H2

Quant Time: Jun 04 03:07:53 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM052721WMA.M  
Quant Title : VOC Analysis  
QLast Update : Fri Jun 04 03:06:56 2021  
Response via : Initial Calibration

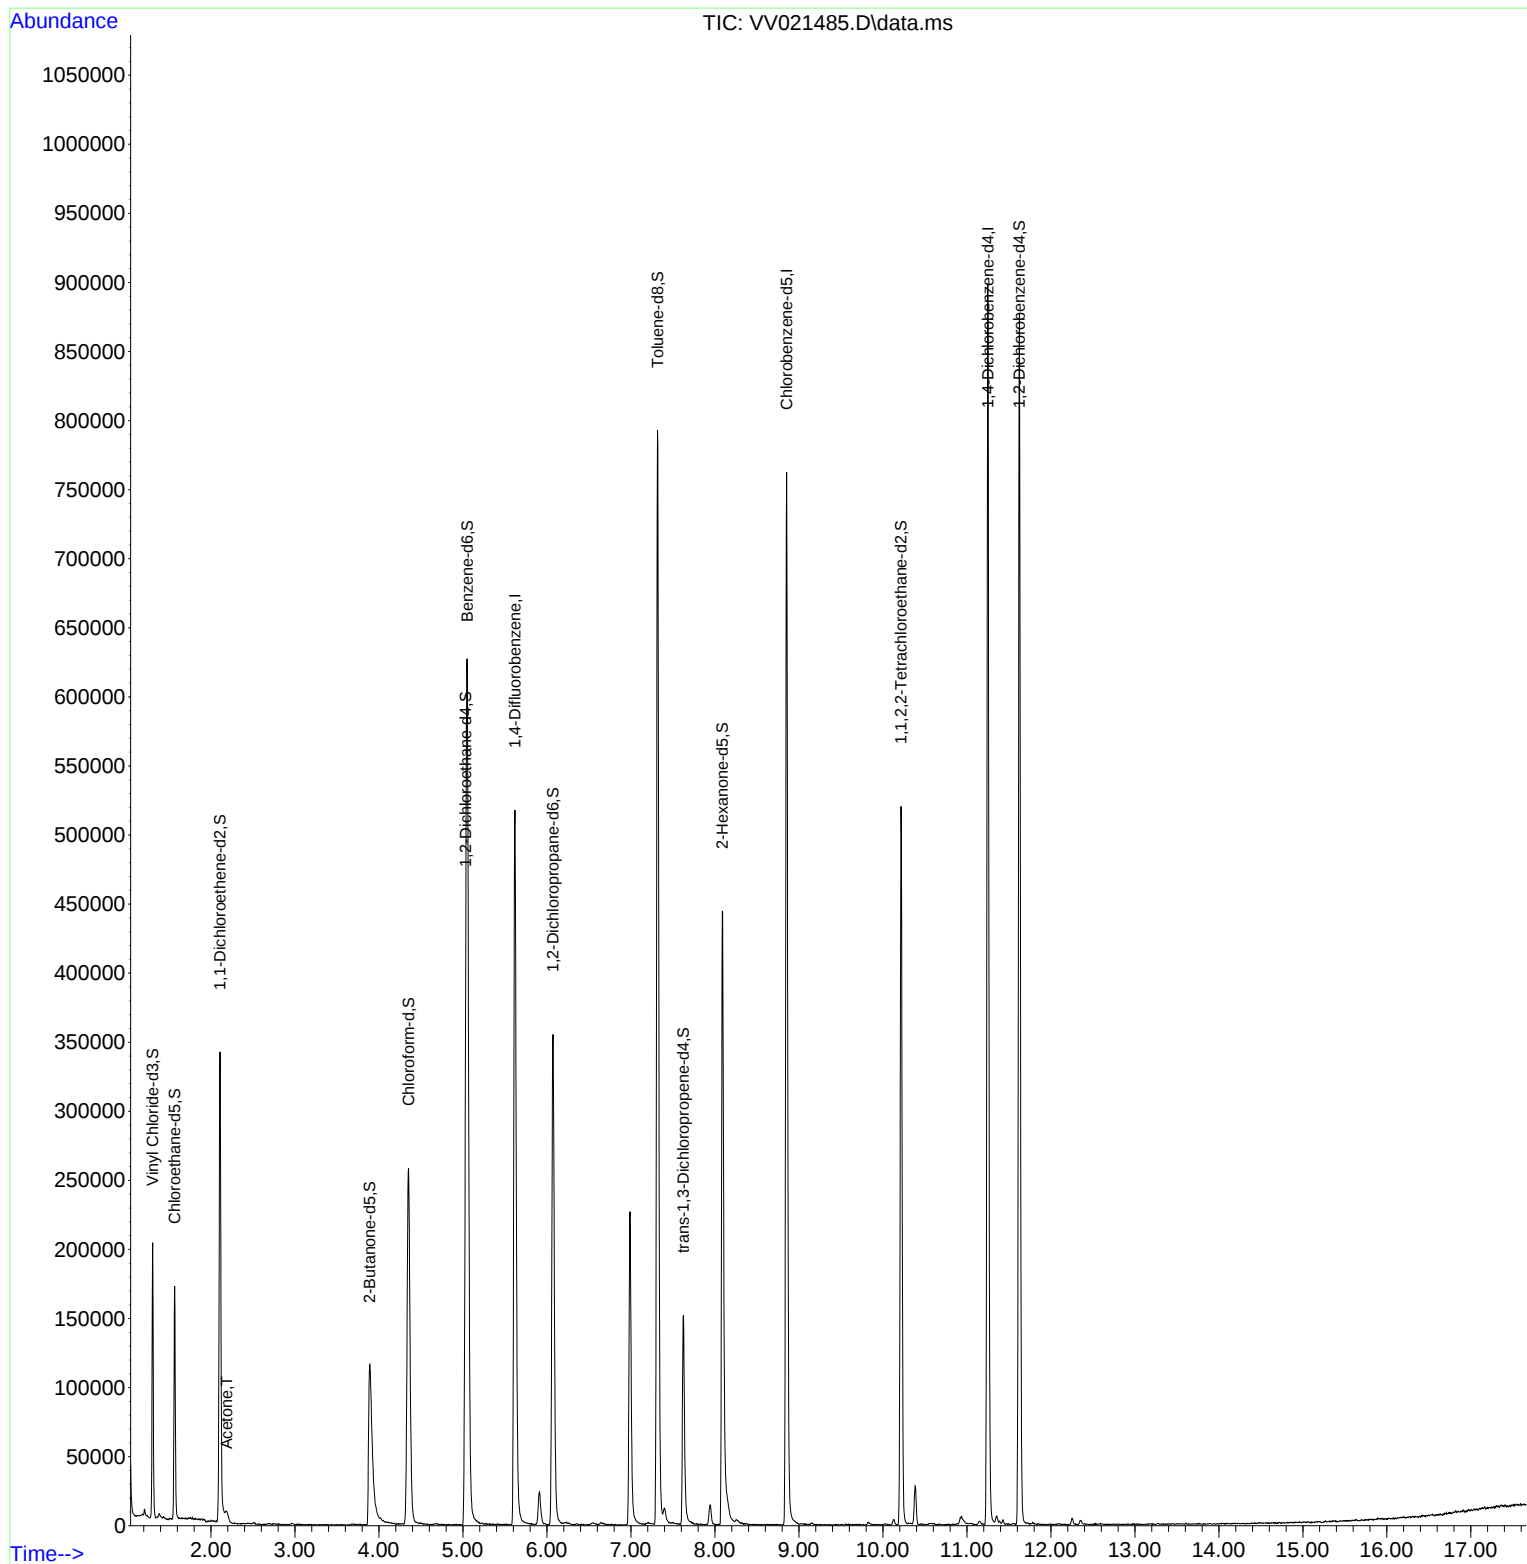

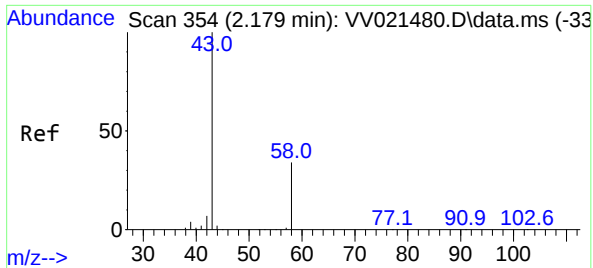

#13  
 Acetone  
 Concen: 5.934 ug/L  
 RT: 2.188 min Scan# 357  
 Delta R.T. 0.010 min  
 Lab File: VV021485.D  
 Acq: 03 Jun 2021 14:23

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BG7H2

Tgt Ion: 43 Resp: 11701  
 Ion Ratio Lower Upper  
 43 100  
 58 37.3 0.0 0.2#

