

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021486.D
 Acq On : 03 Jun 2021 14:47
 Operator : SY/MD
 Sample : M2605-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H8

Quant Time: Jun 04 03:07:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 04 03:06:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	493061	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	455131	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	257051	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	126605	39.000	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	78.000%		
7) Chloroethane-d5	1.568	69	105031	43.494	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.980%		
11) 1,1-Dichloroethene-d2	2.108	63	173638	31.303	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.600%		
21) 2-Butanone-d5	3.892	46	226548	97.322	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.320%		
24) Chloroform-d	4.352	84	278874	43.155	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.320%		
26) 1,2-Dichloroethane-d4	5.034	65	170977	45.936	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.880%		
32) Benzene-d6	5.053	84	576586	45.285	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.580%		
36) 1,2-Dichloropropane-d6	6.072	67	181900	46.262	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.520%		
41) Toluene-d8	7.317	98	549275	45.281	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.560%		
43) trans-1,3-Dichloroprop...	7.625	79	92483	43.951	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.900%		
47) 2-Hexanone-d5	8.088	63	162808	90.174	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	90.170%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	243477	44.609	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.220%		
66) 1,2-Dichlorobenzene-d4	11.625	152	245527	45.950	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.900%		
Target Compounds					Qvalue	
13) Acetone	2.185	43	12662	6.322	ug/L #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021486.D
Acq On : 03 Jun 2021 14:47
Operator : SY/MD
Sample : M2605-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H8

Quant Time: Jun 04 03:07:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 04 03:06:56 2021
Response via : Initial Calibration

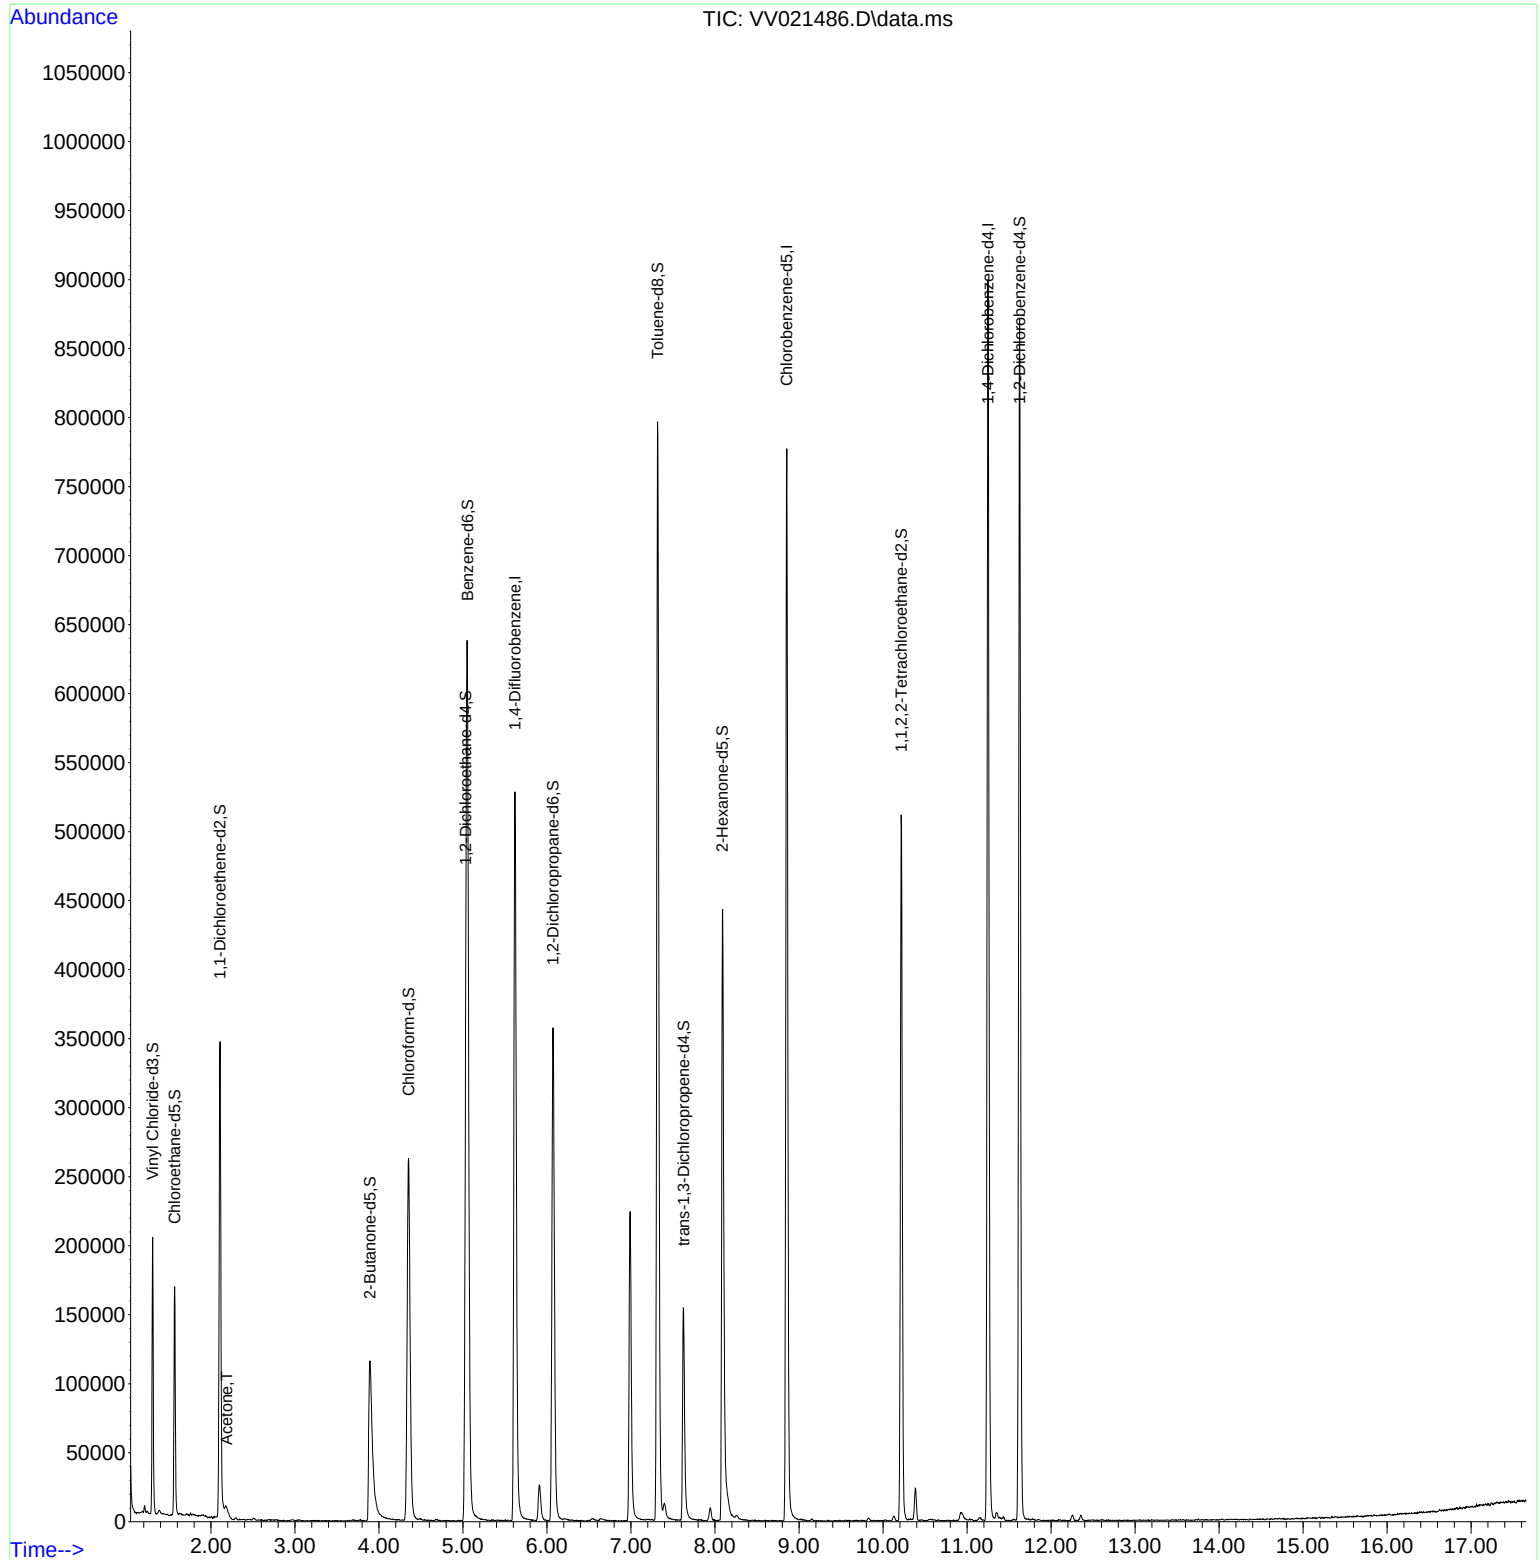

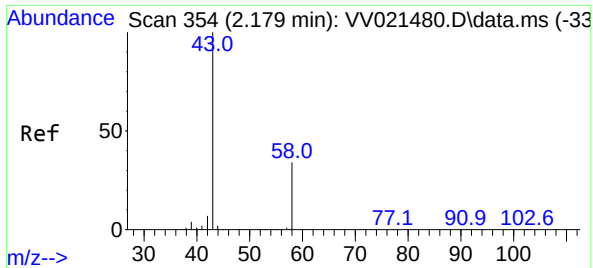

#13
 Acetone
 Concen: 6.322 ug/L
 RT: 2.185 min Scan# 356
 Delta R.T. 0.006 min
 Lab File: VV021486.D
 Acq: 03 Jun 2021 14:47

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H8

Tgt Ion:	43	Resp:	12662
Ion	Ratio	Lower	Upper
43	100		
58	12.2	0.0	0.2#

