

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021482.D
 Acq On : 03 Jun 2021 11:44
 Operator : SY/MD
 Sample : VV0603WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK184

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

Signal : TIC: VV021482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	218306	215732	12.48%	1.578%
2	1.568	157	164	179	rVB	176112	193218	11.18%	1.414%
3	2.108	322	332	361	rVB	363506	547886	31.69%	4.009%
4	2.654	499	502	503	rBV	381	227	0.01%	0.002%
5	2.712	516	520	523	rBV4	555	516	0.03%	0.004%
6	2.802	547	548	549	rBV4	381	137	0.01%	0.001%
7	2.844	559	561	564	rBV2	346	169	0.01%	0.001%
8	2.924	584	586	590	rVB3	400	227	0.01%	0.002%
9	2.953	594	595	599	rBV	318	140	0.01%	0.001%
10	3.031	617	619	622	rVB2	428	227	0.01%	0.002%
11	3.143	651	654	656	rBV	291	183	0.01%	0.001%
12	3.159	657	659	663	rVV3	523	379	0.02%	0.003%
13	3.214	674	676	679	rVB2	268	175	0.01%	0.001%
14	3.243	680	685	687	rBV	294	230	0.01%	0.002%
15	3.256	687	689	691	rVB2	268	126	0.01%	0.001%
16	3.301	700	703	704	rBV	363	217	0.01%	0.002%
17	3.358	720	721	731	rVB2	425	255	0.01%	0.002%
18	3.416	733	739	743	rBV2	456	386	0.02%	0.003%
19	3.432	743	744	746	rBV	261	139	0.01%	0.001%
20	3.481	756	759	761	rBV2	441	220	0.01%	0.002%
21	3.526	770	773	778	rVB2	367	358	0.02%	0.003%
22	3.632	802	806	811	rBV3	353	375	0.02%	0.003%
23	3.696	824	826	829	rBV	225	165	0.01%	0.001%
24	3.715	829	832	836	rVV2	350	290	0.02%	0.002%
25	3.744	836	841	843	rVV2	421	348	0.02%	0.003%
26	3.770	847	849	852	rVV	473	203	0.01%	0.001%
27	3.815	859	863	865	rBV3	285	196	0.01%	0.001%
28	3.889	873	886	927	rBV	128714	401654	23.24%	2.939%
29	4.236	990	994	997	rBV5	751	713	0.04%	0.005%
30	4.352	1013	1030	1055	rBV	277987	681077	39.40%	4.983%
31	4.593	1102	1105	1106	rBV3	455	174	0.01%	0.001%
32	4.654	1122	1124	1125	rBV	369	123	0.01%	0.001%
33	4.670	1125	1129	1130	rBV2	576	370	0.02%	0.003%
34	4.805	1168	1171	1174	rBV2	463	310	0.02%	0.002%
35	4.905	1200	1202	1204	rVB2	398	145	0.01%	0.001%
36	4.918	1204	1206	1208	rVV	311	173	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021482.D
 Acq On : 03 Jun 2021 11:44
 Operator : SY/MD
 Sample : VV0603WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK184

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	4.934	1208	1211	1213	rVV	261	137	0.01%	0.001%
38	4.950	1213	1216	1220	rVB	540	369	0.02%	0.003%
39	5.050	1230	1247	1276	rBV2	670469	1728648	100.00%	12.648%
40	5.407	1353	1358	1361	rBV4	735	853	0.05%	0.006%
41	5.526	1392	1395	1396	rBV	377	203	0.01%	0.001%
42	5.555	1402	1404	1407	rVB2	420	155	0.01%	0.001%
43	5.619	1411	1424	1462	rBV	521621	1056487	61.12%	7.730%
44	5.911	1506	1515	1532	rVB4	11340	24097	1.39%	0.176%
45	5.989	1537	1539	1541	rBV	323	140	0.01%	0.001%
46	6.072	1551	1565	1596	rBV	381894	773736	44.76%	5.661%
47	6.362	1652	1655	1657	rBV3	382	191	0.01%	0.001%
48	6.394	1663	1665	1669	rBV2	199	163	0.01%	0.001%
49	6.522	1702	1705	1707	rBV	195	133	0.01%	0.001%
50	6.645	1734	1743	1746	rBV5	1507	2375	0.14%	0.017%
51	6.792	1786	1789	1792	rBV3	359	220	0.01%	0.002%
52	6.809	1792	1794	1797	rVB2	370	205	0.01%	0.001%
53	6.831	1798	1801	1804	rVB2	427	267	0.02%	0.002%
54	6.850	1804	1807	1808	rBV	368	125	0.01%	0.001%
55	6.931	1827	1832	1835	rBV3	360	305	0.02%	0.002%
56	6.989	1835	1850	1874	rBV	237855	437971	25.34%	3.205%
57	7.317	1939	1952	1970	rBV	844585	1472331	85.17%	10.773%
58	7.625	2037	2048	2074	rBV	161984	287878	16.65%	2.106%
59	7.982	2155	2159	2167	rBV4	1059	1183	0.07%	0.009%
60	8.088	2182	2192	2227	rBV	448588	829934	48.01%	6.072%
61	8.503	2317	2321	2324	rBV2	313	244	0.01%	0.002%
62	8.522	2324	2327	2331	rBV3	596	488	0.03%	0.004%
63	8.677	2373	2375	2379	rVB2	297	155	0.01%	0.001%
64	8.712	2383	2386	2388	rBV	294	159	0.01%	0.001%
65	8.731	2389	2392	2394	rBV2	312	196	0.01%	0.001%
66	8.780	2403	2407	2411	rBV2	148	149	0.01%	0.001%
67	8.853	2418	2430	2455	rBV	773125	1258954	72.83%	9.211%
68	9.255	2550	2555	2559	rBV2	624	494	0.03%	0.004%
69	9.320	2571	2575	2577	rBV2	357	221	0.01%	0.002%
70	9.333	2577	2579	2583	rVV2	232	170	0.01%	0.001%
71	9.474	2619	2623	2627	rBV4	379	341	0.02%	0.002%
72	9.554	2642	2648	2653	rBV5	861	1187	0.07%	0.009%
73	9.779	2714	2718	2722	rBV3	239	218	0.01%	0.002%
74	9.898	2752	2755	2758	rBV2	285	234	0.01%	0.002%
75	9.927	2760	2764	2765	rBV	385	257	0.01%	0.002%
76	10.005	2786	2788	2791	rBB2	316	180	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021482.D
 Acq On : 03 Jun 2021 11:44
 Operator : SY/MD
 Sample : VV0603WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK184

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	10.037	2795	2798	2801	rBV2	237	169	0.01%	0.001%
78	10.050	2801	2802	2807	rVB2	306	130	0.01%	0.001%
79	10.130	2818	2827	2836	rVB3	4118	6548	0.38%	0.048%
80	10.217	2842	2854	2876	rBV	558260	883587	51.11%	6.465%
81	10.429	2918	2920	2922	rBV	332	156	0.01%	0.001%
82	10.451	2924	2927	2928	rBV	326	181	0.01%	0.001%
83	10.548	2951	2957	2960	rBV4	767	858	0.05%	0.006%
84	10.657	2986	2991	2993	rBV3	722	571	0.03%	0.004%
85	10.689	2999	3001	3004	rBV	249	200	0.01%	0.001%
86	10.773	3024	3027	3031	rBV3	521	390	0.02%	0.003%
87	10.976	3088	3090	3092	rBV	310	141	0.01%	0.001%
88	11.017	3098	3103	3105	rBV2	410	343	0.02%	0.003%
89	11.033	3105	3108	3115	rVB4	980	994	0.06%	0.007%
90	11.101	3125	3129	3131	rBV3	508	330	0.02%	0.002%
91	11.152	3135	3145	3152	rBV6	1845	3288	0.19%	0.024%
92	11.249	3164	3175	3197	rBV	894122	1383251	80.02%	10.121%
93	11.541	3263	3266	3268	rBV2	434	298	0.02%	0.002%
94	11.625	3280	3292	3318	rBV	918132	1451548	83.97%	10.621%
95	11.850	3357	3362	3367	rBV5	1045	1082	0.06%	0.008%
96	12.152	3452	3456	3457	rBV	330	234	0.01%	0.002%
97	12.368	3520	3523	3524	rBV	691	342	0.02%	0.003%
98	12.574	3585	3587	3590	rBV2	550	390	0.02%	0.003%
99	12.651	3606	3611	3620	rBV4	1238	1618	0.09%	0.012%
100	13.274	3799	3805	3808	rBV6	1204	1381	0.08%	0.010%




Sum of corrected areas: 13667246

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021482.D
Acq On : 03 Jun 2021 11:44
Operator : SY/MD
Sample : VV0603WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK184

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

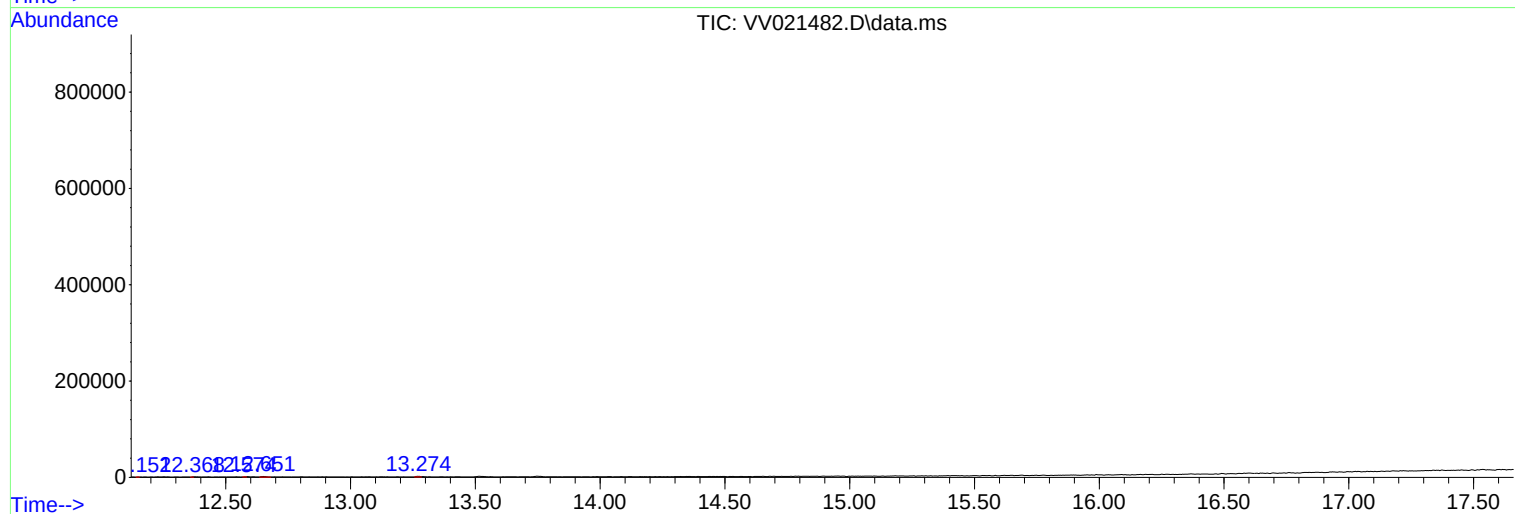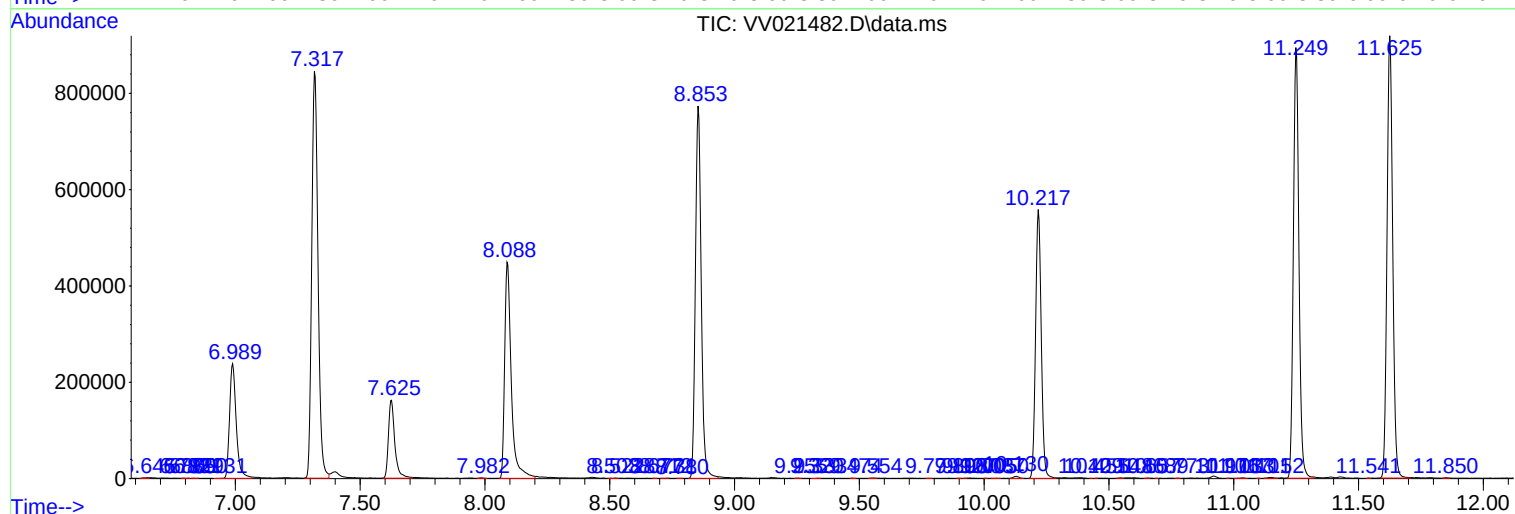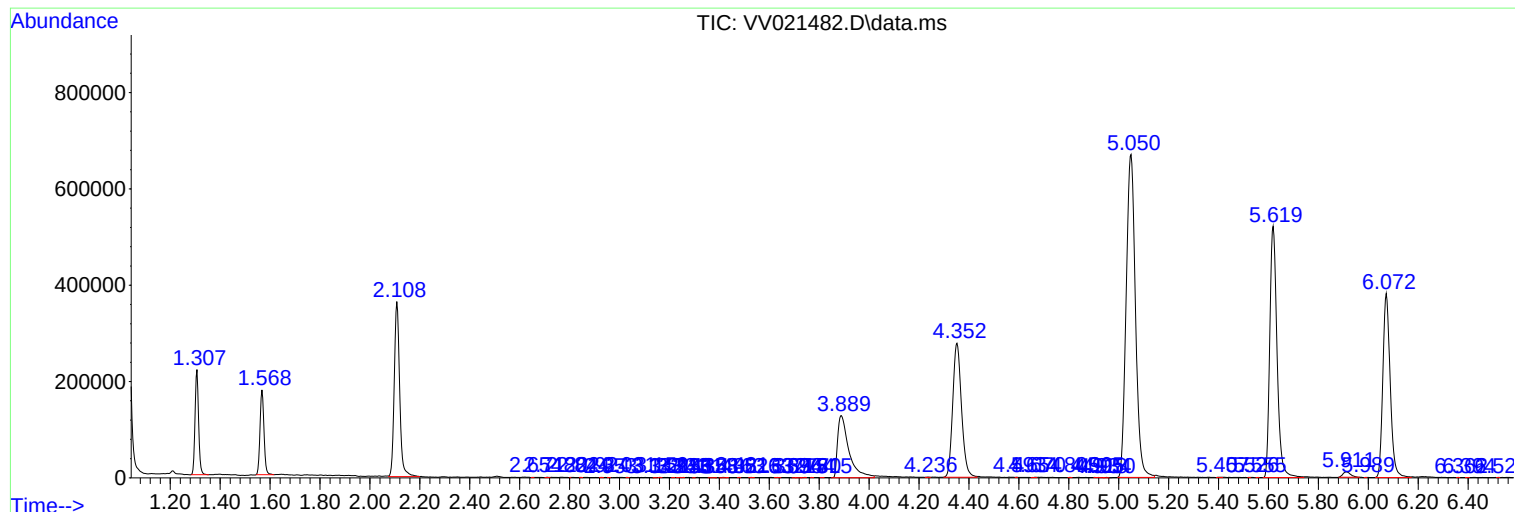

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021482.D
Acq On : 03 Jun 2021 11:44
Operator : SY/MD
Sample : VV0603WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK184

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021482.D
Acq On : 03 Jun 2021 11:44
Operator : SY/MD
Sample : VV0603WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK184

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
