

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021483.D
 Acq On : 03 Jun 2021 13:36
 Operator : SY/MD
 Sample : M2596-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG5W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	210549	209273	12.51%	1.558%
2	1.568	157	164	179	rVB	172983	192956	11.54%	1.436%
3	2.108	323	332	350	rBV	346139	513079	30.68%	3.819%
4	2.703	515	517	521	rBV3	427	308	0.02%	0.002%
5	2.738	526	528	531	rBV2	377	141	0.01%	0.001%
6	2.857	564	565	566	rBV2	281	96	0.01%	0.001%
7	2.966	596	599	602	rBV3	359	312	0.02%	0.002%
8	3.172	659	663	665	rBV2	335	273	0.02%	0.002%
9	3.243	680	685	690	rBV2	429	359	0.02%	0.003%
10	3.352	714	719	720	rBV2	429	335	0.02%	0.002%
11	3.378	724	727	733	rVB3	282	317	0.02%	0.002%
12	3.426	741	742	743	rVB3	121	23	0.00%	0.000%
13	3.442	743	747	752	rBV3	407	523	0.03%	0.004%
14	3.481	757	759	761	rBV3	252	114	0.01%	0.001%
15	3.500	761	765	769	rVB2	307	261	0.02%	0.002%
16	3.523	769	772	774	rBV2	212	128	0.01%	0.001%
17	3.545	775	779	785	rVB3	424	414	0.02%	0.003%
18	3.574	785	788	794	rBV2	447	376	0.02%	0.003%
19	3.606	794	798	799	rBV	417	218	0.01%	0.002%
20	3.654	811	813	815	rVB	335	107	0.01%	0.001%
21	3.703	827	828	830	rVB2	48	17	0.00%	0.000%
22	3.712	830	831	832	rBV	113	24	0.00%	0.000%
23	3.722	832	834	837	rBV2	217	196	0.01%	0.001%
24	3.764	843	847	850	rBV	374	272	0.02%	0.002%
25	3.895	878	888	938	rBV2	101157	360716	21.57%	2.685%
26	4.352	1015	1030	1057	rBV	263027	652836	39.03%	4.860%
27	4.809	1170	1172	1175	rBV3	348	292	0.02%	0.002%
28	4.879	1193	1194	1197	rBV2	222	90	0.01%	0.001%
29	4.899	1197	1200	1202	rVB3	425	251	0.02%	0.002%
30	4.985	1223	1227	1229	rBV2	250	175	0.01%	0.001%
31	5.050	1229	1247	1285	rBV3	652450	1672588	100.00%	12.450%
32	5.452	1369	1372	1376	rVB3	686	408	0.02%	0.003%
33	5.490	1376	1384	1387	rBV2	991	1043	0.06%	0.008%
34	5.619	1412	1424	1462	rBV	524323	1063387	63.58%	7.916%
35	5.911	1503	1515	1537	rBV4	22324	48028	2.87%	0.358%
36	6.021	1547	1549	1550	rBV4	365	138	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021483.D
 Acq On : 03 Jun 2021 13:36
 Operator : SY/MD
 Sample : M2596-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG5W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.072	1552	1565	1595	rVV	369010	750470	44.87%	5.586%
38	6.426	1673	1675	1677	rVB	248	93	0.01%	0.001%
39	6.442	1678	1680	1681	rBV	387	139	0.01%	0.001%
40	6.500	1695	1698	1700	rBV	243	171	0.01%	0.001%
41	6.538	1707	1710	1714	rBV3	488	428	0.03%	0.003%
42	6.780	1773	1785	1796	rBV4	7176	15477	0.93%	0.115%
43	6.879	1815	1816	1820	rBV2	408	222	0.01%	0.002%
44	6.989	1839	1850	1876	rBV	231124	422266	25.25%	3.143%
45	7.320	1941	1953	1971	rBV	816350	1419497	84.87%	10.566%
46	7.625	2038	2048	2070	rBV	155916	274556	16.42%	2.044%
47	7.944	2139	2147	2158	rVB2	24477	41011	2.45%	0.305%
48	8.024	2170	2172	2175	rVB2	405	231	0.01%	0.002%
49	8.040	2175	2177	2179	rBV	491	276	0.02%	0.002%
50	8.091	2182	2193	2227	rBV	410357	760601	45.47%	5.662%
51	8.506	2316	2322	2323	rBV3	457	389	0.02%	0.003%
52	8.574	2340	2343	2351	rVB5	1063	1055	0.06%	0.008%
53	8.725	2387	2390	2393	rBV2	486	280	0.02%	0.002%
54	8.763	2400	2402	2403	rBV	462	216	0.01%	0.002%
55	8.792	2403	2411	2418	rVB4	2289	3935	0.24%	0.029%
56	8.853	2419	2430	2451	rBV	780392	1262817	75.50%	9.400%
57	9.194	2533	2536	2537	rBV2	698	324	0.02%	0.002%
58	9.288	2563	2565	2569	rVB2	522	311	0.02%	0.002%
59	9.310	2569	2572	2573	rBV2	518	305	0.02%	0.002%
60	9.358	2585	2587	2588	rBV2	201	74	0.00%	0.001%
61	9.374	2588	2592	2597	rVB3	363	366	0.02%	0.003%
62	9.397	2597	2599	2600	rBV3	244	127	0.01%	0.001%
63	9.558	2641	2649	2650	rBV3	866	961	0.06%	0.007%
64	9.632	2668	2672	2676	rBV3	559	520	0.03%	0.004%
65	9.651	2676	2678	2680	rBV2	268	128	0.01%	0.001%
66	9.937	2762	2767	2774	rVB4	1133	1466	0.09%	0.011%
67	9.976	2775	2779	2781	rBV2	300	256	0.02%	0.002%
68	10.217	2841	2854	2874	rBV	511781	810431	48.45%	6.033%
69	10.384	2898	2906	2921	rVB	51118	86832	5.19%	0.646%
70	10.516	2944	2947	2948	rBV2	730	430	0.03%	0.003%
71	10.725	3010	3012	3013	rBV2	509	209	0.01%	0.002%
72	10.770	3023	3026	3027	rBV	549	303	0.02%	0.002%
73	10.918	3066	3072	3084	rVB3	4851	6933	0.41%	0.052%
74	10.982	3089	3092	3095	rBV2	605	478	0.03%	0.004%
75	11.152	3134	3145	3155	rBV6	4498	8973	0.54%	0.067%
76	11.249	3163	3175	3196	rBV	911093	1409509	84.27%	10.492%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021483.D
 Acq On : 03 Jun 2021 13:36
 Operator : SY/MD
 Sample : M2596-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG5W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

77	11.625	3280	3292	3313	rBV	897215	1410570	84.33%	10.500%
78	11.905	3375	3379	3380	rBV2	305	223	0.01%	0.002%
79	12.204	3469	3472	3476	rBV2	327	223	0.01%	0.002%
80	12.223	3476	3478	3479	rBV	325	114	0.01%	0.001%
81	12.252	3479	3487	3496	rVV2	7204	11584	0.69%	0.086%
82	12.355	3511	3519	3527	rBV5	3091	5204	0.31%	0.039%
83	12.525	3571	3572	3574	rBV5	319	137	0.01%	0.001%
84	12.676	3617	3619	3620	rBV	333	116	0.01%	0.001%
85	12.741	3632	3639	3644	rBV6	1245	1595	0.10%	0.012%
86	12.979	3710	3713	3716	rBV2	362	323	0.02%	0.002%
87	12.995	3716	3718	3720	rBV2	389	186	0.01%	0.001%
88	13.053	3732	3736	3739	rBV3	459	432	0.03%	0.003%
89	13.143	3761	3764	3765	rBV	416	248	0.01%	0.002%




Sum of corrected areas: 13434095

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021483.D
Acq On : 03 Jun 2021 13:36
Operator : SY/MD
Sample : M2596-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG5W4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

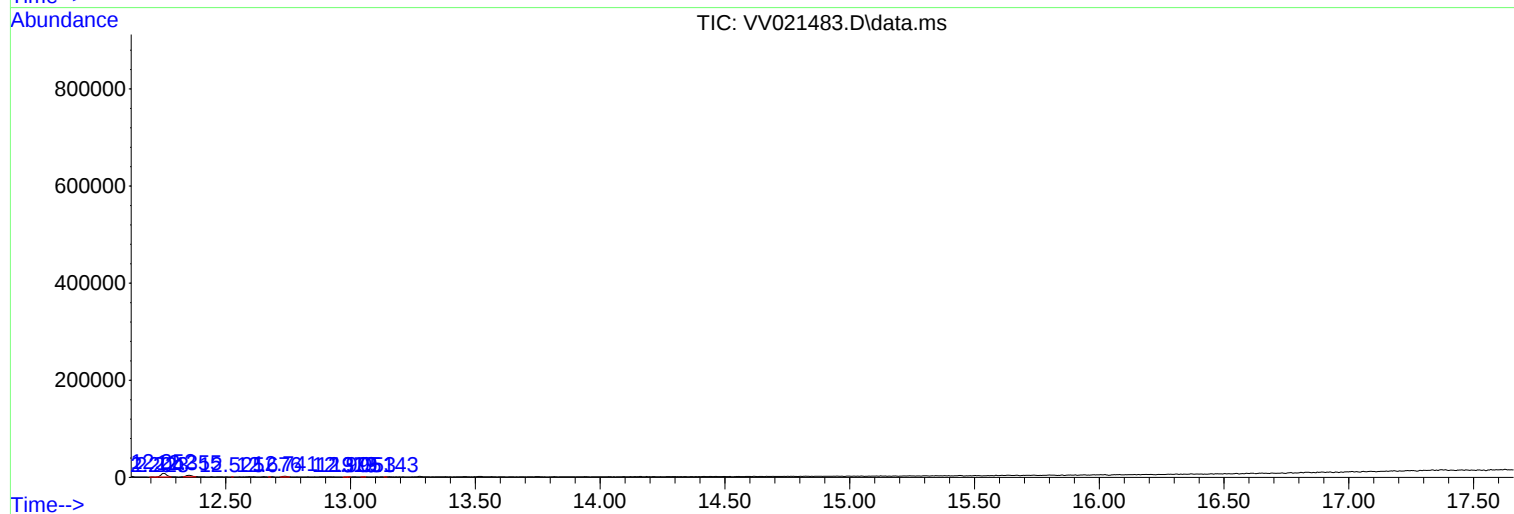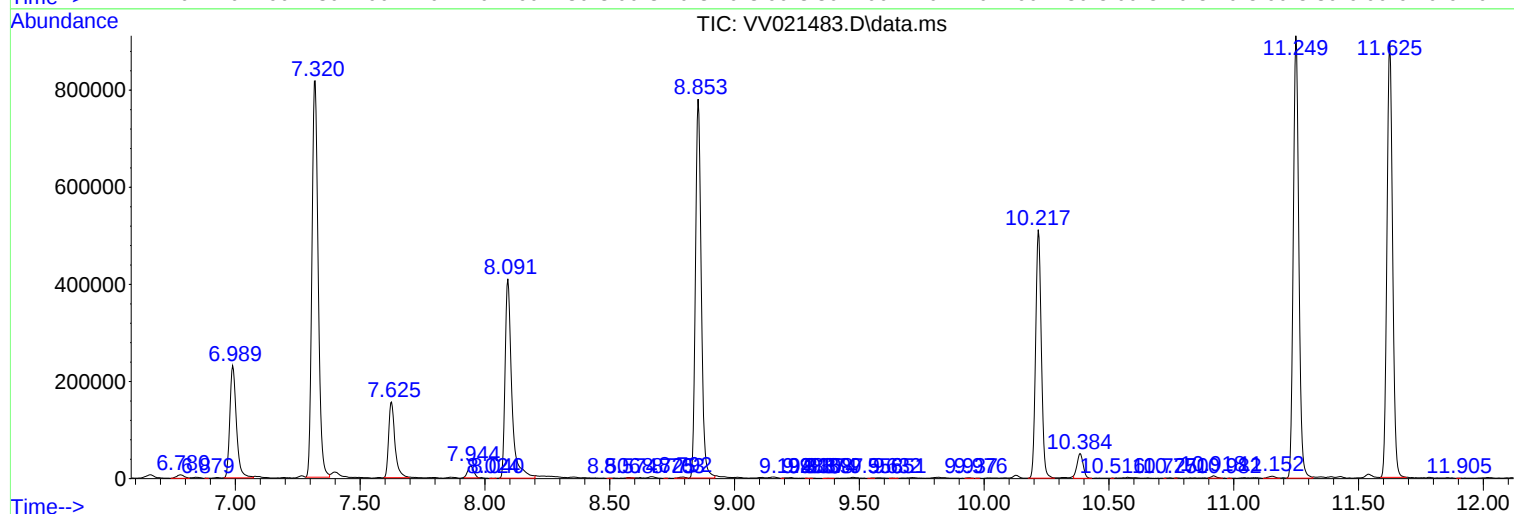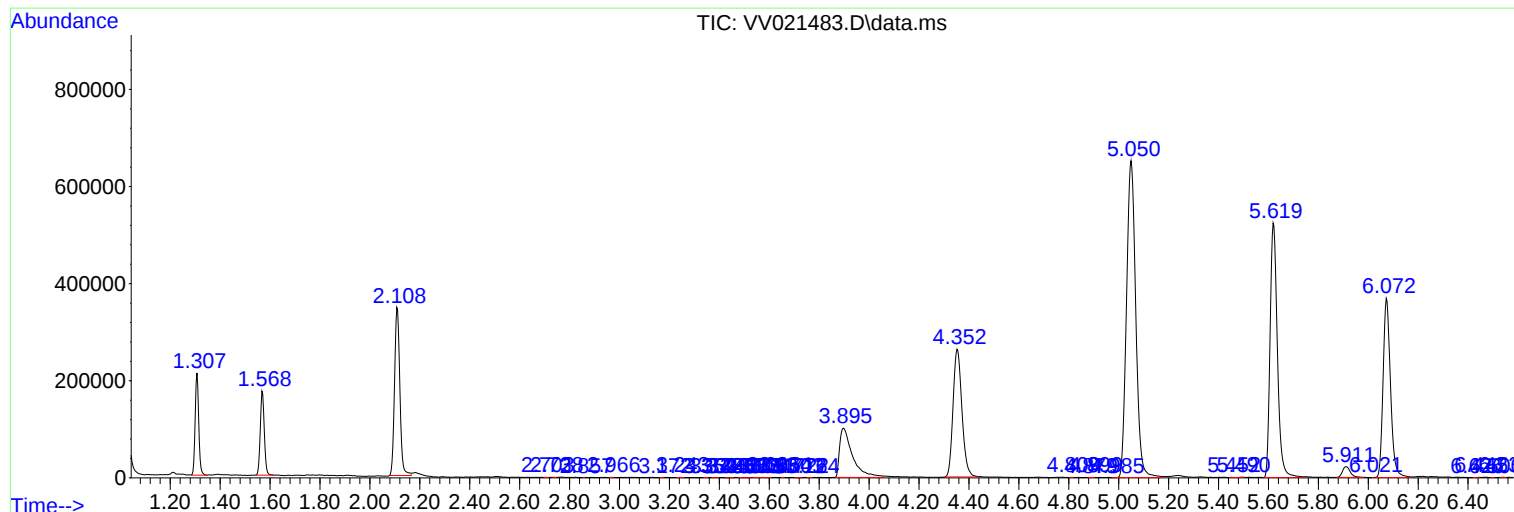

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021483.D
Acq On : 03 Jun 2021 13:36
Operator : SY/MD
Sample : M2596-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG5W4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021483.D
Acq On : 03 Jun 2021 13:36
Operator : SY/MD
Sample : M2596-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG5W4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
