

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021484.D
 Acq On : 03 Jun 2021 14:00
 Operator : SY/MD
 Sample : M2605-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7J9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	202919	205276	12.37%	1.515%
2	1.568	157	164	174	rVB	166632	185565	11.18%	1.369%
3	2.108	323	332	359	rVB	347437	517918	31.21%	3.822%
4	2.764	522	536	550	rBV2	8498	17496	1.05%	0.129%
5	2.864	565	567	571	rBV2	345	252	0.02%	0.002%
6	2.896	575	577	582	rVV3	385	217	0.01%	0.002%
7	3.044	609	623	641	rBV3	23659	50295	3.03%	0.371%
8	3.156	653	658	661	rBV3	364	418	0.03%	0.003%
9	3.253	686	688	693	rVB2	310	263	0.02%	0.002%
10	3.275	693	695	696	rBV	300	136	0.01%	0.001%
11	3.285	696	698	699	rVB	449	165	0.01%	0.001%
12	3.320	705	709	714	rVB3	213	155	0.01%	0.001%
13	3.571	784	787	794	rVB2	328	344	0.02%	0.003%
14	3.603	794	797	800	rVB2	388	223	0.01%	0.002%
15	3.632	800	806	809	rBV2	283	250	0.02%	0.002%
16	3.693	822	825	826	rBV	271	171	0.01%	0.001%
17	3.767	831	848	864	rBV4	19807	51651	3.11%	0.381%
18	3.892	876	887	932	rBV	125189	411226	24.78%	3.035%
19	4.352	1012	1030	1064	rBV	267897	662198	39.90%	4.887%
20	4.606	1107	1109	1111	rBV	383	159	0.01%	0.001%
21	4.677	1127	1131	1136	rBV4	765	686	0.04%	0.005%
22	4.732	1146	1148	1151	rBV	243	136	0.01%	0.001%
23	4.863	1183	1189	1190	rBV	354	245	0.01%	0.002%
24	4.899	1194	1200	1202	rBV2	518	348	0.02%	0.003%
25	4.963	1218	1220	1225	rVB3	423	374	0.02%	0.003%
26	5.050	1229	1247	1276	rBV2	648854	1659599	100.00%	12.247%
27	5.516	1388	1392	1393	rBV3	326	200	0.01%	0.001%
28	5.564	1405	1407	1410	rBV2	522	246	0.01%	0.002%
29	5.619	1411	1424	1453	rBV	536112	1072286	64.61%	7.913%
30	5.912	1505	1515	1530	rBV3	9808	21043	1.27%	0.155%
31	6.072	1551	1565	1591	rBV	366164	743811	44.82%	5.489%
32	6.304	1631	1637	1642	rVB3	502	628	0.04%	0.005%
33	6.330	1642	1645	1646	rBV	377	188	0.01%	0.001%
34	6.362	1651	1655	1658	rBV2	569	380	0.02%	0.003%
35	6.381	1658	1661	1663	rBV	386	161	0.01%	0.001%
36	6.439	1676	1679	1681	rBV	360	245	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021484.D
 Acq On : 03 Jun 2021 14:00
 Operator : SY/MD
 Sample : M2605-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7J9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.461	1684	1686	1690	rVB	342	164	0.01%	0.001%
38	6.510	1697	1701	1703	rVB3	281	164	0.01%	0.001%
39	6.526	1703	1706	1708	rBV2	209	179	0.01%	0.001%
40	6.584	1721	1724	1726	rVB	386	210	0.01%	0.002%
41	6.606	1726	1731	1733	rBV2	411	334	0.02%	0.002%
42	6.645	1733	1743	1744	rBV3	1255	1787	0.11%	0.013%
43	6.728	1767	1769	1773	rVB3	426	264	0.02%	0.002%
44	6.886	1813	1818	1820	rBV3	236	198	0.01%	0.001%
45	6.921	1828	1829	1834	rVB3	313	148	0.01%	0.001%
46	6.989	1838	1850	1875	rBV	228264	420191	25.32%	3.101%
47	7.317	1941	1952	1971	rBV	808119	1414756	85.25%	10.440%
48	7.625	2037	2048	2080	rBV	156277	281348	16.95%	2.076%
49	7.818	2106	2108	2111	rBV3	388	187	0.01%	0.001%
50	7.867	2118	2123	2125	rBV3	418	378	0.02%	0.003%
51	7.902	2132	2134	2135	rBV3	394	134	0.01%	0.001%
52	7.921	2137	2140	2141	rBV	433	219	0.01%	0.002%
53	7.940	2142	2146	2148	rBV3	943	772	0.05%	0.006%
54	8.047	2175	2179	2181	rBV4	423	263	0.02%	0.002%
55	8.088	2181	2192	2223	rBV	464653	844091	50.86%	6.229%
56	8.596	2348	2350	2355	rBV3	395	276	0.02%	0.002%
57	8.619	2355	2357	2361	rVB2	422	275	0.02%	0.002%
58	8.641	2361	2364	2366	rBV	419	258	0.02%	0.002%
59	8.770	2402	2404	2411	rVB3	290	200	0.01%	0.001%
60	8.854	2411	2430	2456	rBV	780045	1283273	77.32%	9.470%
61	9.207	2538	2540	2543	rBV2	508	261	0.02%	0.002%
62	9.230	2543	2547	2548	rBV2	254	200	0.01%	0.001%
63	9.249	2551	2553	2556	rBV2	209	145	0.01%	0.001%
64	9.310	2564	2572	2576	rBV3	382	485	0.03%	0.004%
65	9.413	2602	2604	2607	rVB2	313	142	0.01%	0.001%
66	9.587	2656	2658	2662	rVB2	418	230	0.01%	0.002%
67	9.606	2662	2664	2667	rBV	289	158	0.01%	0.001%
68	9.674	2682	2685	2689	rBV2	398	347	0.02%	0.003%
69	9.738	2702	2705	2709	rVB2	404	329	0.02%	0.002%
70	9.757	2709	2711	2712	rBV2	387	158	0.01%	0.001%
71	9.815	2726	2729	2732	rVB2	455	267	0.02%	0.002%
72	9.866	2742	2745	2748	rBV2	225	185	0.01%	0.001%
73	9.915	2755	2760	2763	rBV4	356	342	0.02%	0.003%
74	9.963	2772	2775	2777	rVB2	274	126	0.01%	0.001%
75	10.014	2786	2791	2794	rBV3	241	208	0.01%	0.002%
76	10.040	2795	2799	2802	rBV3	241	175	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021484.D
 Acq On : 03 Jun 2021 14:00
 Operator : SY/MD
 Sample : M2605-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7J9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

77	10.072	2807	2809	2813	rBV2	261	168	0.01%	0.001%
78	10.127	2819	2826	2835	rVB4	3459	5173	0.31%	0.038%
79	10.217	2842	2854	2876	rBV	552904	871873	52.54%	6.434%
80	10.355	2895	2897	2900	rBV2	638	477	0.03%	0.004%
81	10.661	2988	2992	2994	rBV3	477	362	0.02%	0.003%
82	10.792	3031	3033	3035	rBV3	334	171	0.01%	0.001%
83	10.805	3035	3037	3040	rVV3	349	209	0.01%	0.002%
84	10.892	3061	3064	3065	rBV2	397	190	0.01%	0.001%
85	10.918	3065	3072	3083	rVB6	3459	5979	0.36%	0.044%
86	11.027	3105	3106	3107	rBV6	460	175	0.01%	0.001%
87	11.143	3135	3142	3151	rBV5	1954	3333	0.20%	0.025%
88	11.191	3155	3157	3158	rBV5	372	174	0.01%	0.001%
89	11.249	3163	3175	3210	rVV	917640	1411770	85.07%	10.418%
90	11.625	3280	3292	3311	rBV	870459	1388703	83.68%	10.248%
91	11.879	3369	3371	3375	rVB3	499	237	0.01%	0.002%
92	11.931	3381	3387	3388	rBV3	454	467	0.03%	0.003%
93	12.156	3455	3457	3458	rBV	271	128	0.01%	0.001%
94	12.243	3481	3484	3485	rBV2	447	246	0.01%	0.002%
95	12.342	3512	3515	3519	rBV	406	456	0.03%	0.003%
96	12.484	3555	3559	3565	rBV3	815	998	0.06%	0.007%
97	12.516	3567	3569	3570	rBV	544	232	0.01%	0.002%
98	12.648	3608	3610	3613	rBV3	430	288	0.02%	0.002%
99	12.712	3628	3630	3635	rBV3	397	306	0.02%	0.002%
100	12.815	3660	3662	3664	rBV	324	157	0.01%	0.001%




Sum of corrected areas: 13551053

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021484.D
Acq On : 03 Jun 2021 14:00
Operator : SY/MD
Sample : M2605-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7J9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

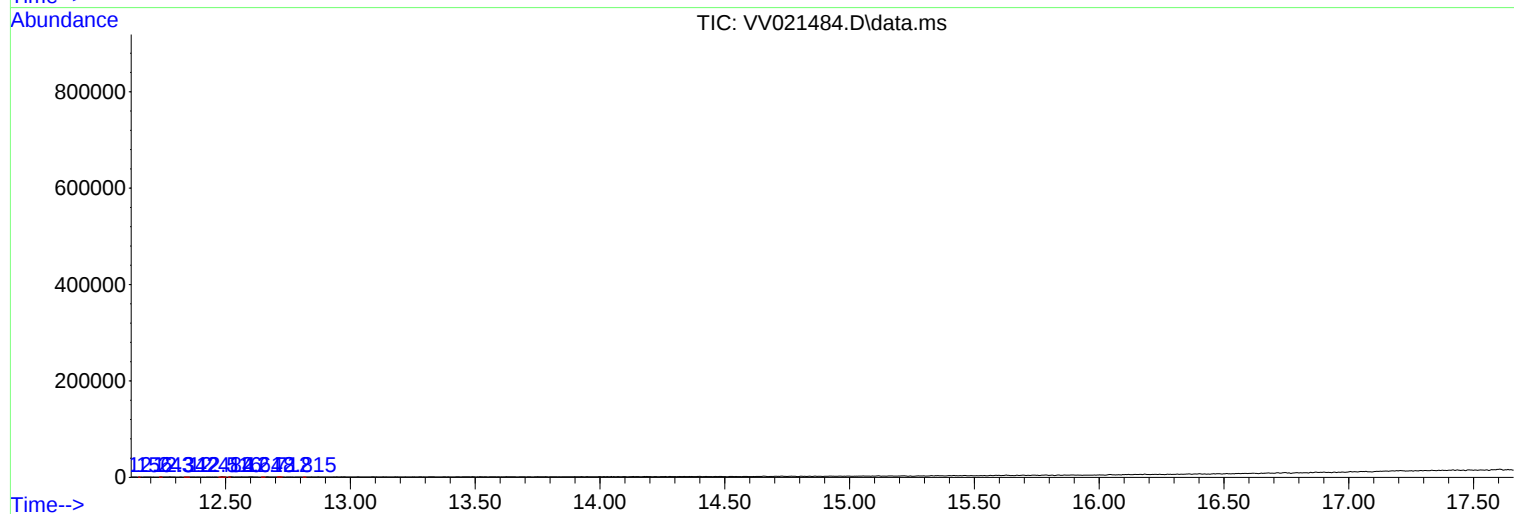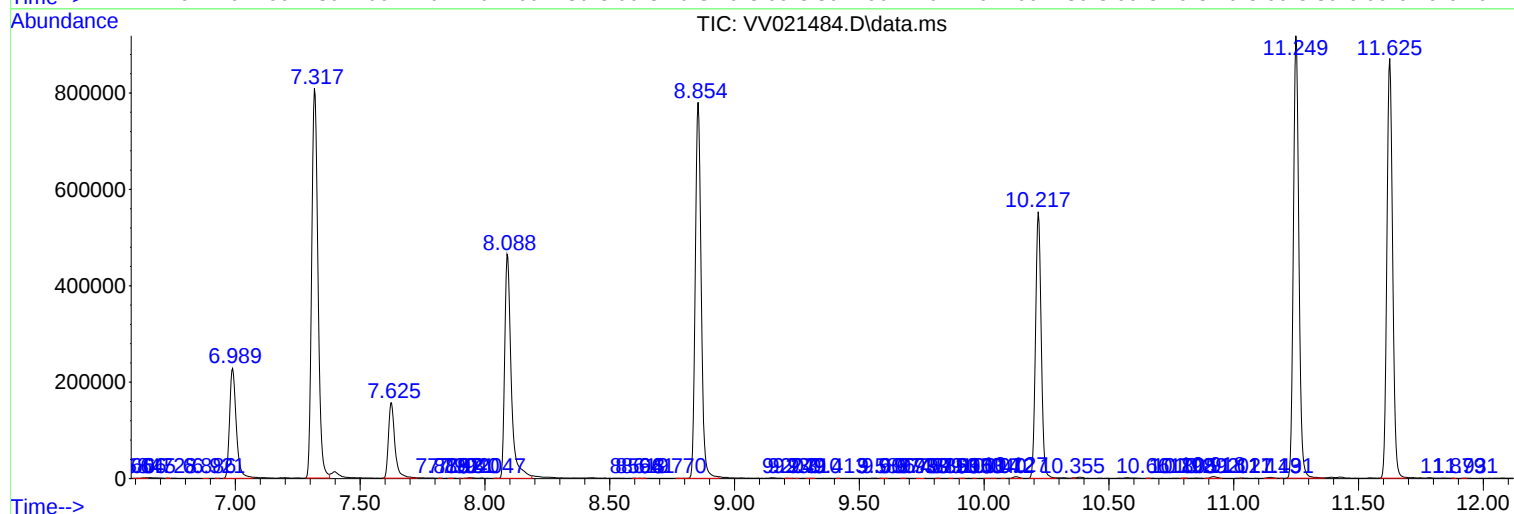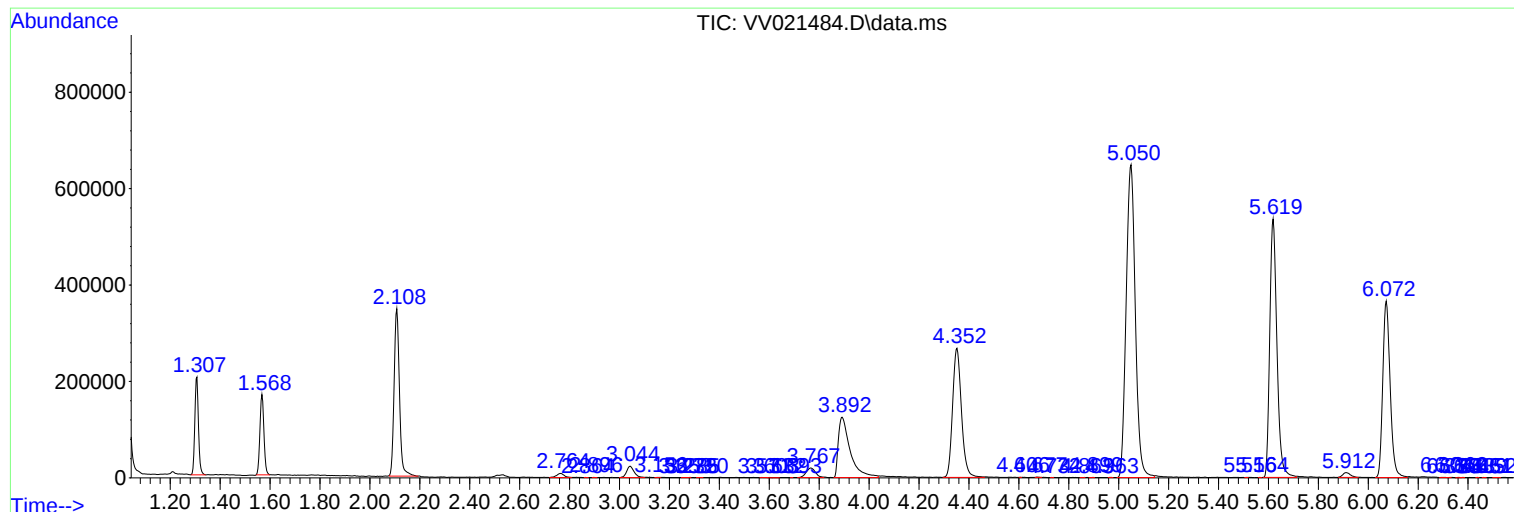

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021484.D
Acq On : 03 Jun 2021 14:00
Operator : SY/MD
Sample : M2605-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7J9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021484.D
Acq On : 03 Jun 2021 14:00
Operator : SY/MD
Sample : M2605-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7J9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
