

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021485.D
 Acq On : 03 Jun 2021 14:23
 Operator : SY/MD
 Sample : M2605-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	199320	200976	12.42%	1.531%
2	1.568	157	164	179	rVB	168124	186175	11.50%	1.418%
3	2.108	322	332	349	rBV	338864	497250	30.72%	3.787%
4	2.841	558	560	561	rBV	307	111	0.01%	0.001%
5	2.873	568	570	574	rVB3	394	300	0.02%	0.002%
6	2.905	578	580	583	rBV2	284	116	0.01%	0.001%
7	3.021	613	616	619	rBV3	362	227	0.01%	0.002%
8	3.037	619	621	623	rBV2	469	230	0.01%	0.002%
9	3.153	656	657	660	rBV	299	197	0.01%	0.002%
10	3.294	698	701	704	rBV2	282	167	0.01%	0.001%
11	3.420	737	740	743	rBV2	185	156	0.01%	0.001%
12	3.471	752	756	759	rBV2	274	257	0.02%	0.002%
13	3.539	775	777	778	rBV2	262	108	0.01%	0.001%
14	3.645	807	810	812	rVB2	203	107	0.01%	0.001%
15	3.664	813	816	817	rBV2	437	188	0.01%	0.001%
16	3.773	842	850	851	rBV4	536	531	0.03%	0.004%
17	3.825	862	866	868	rBV2	263	177	0.01%	0.001%
18	3.892	875	887	923	rBV	116061	369698	22.84%	2.815%
19	4.352	1013	1030	1057	rBV	257452	636040	39.29%	4.844%
20	4.645	1118	1121	1124	rBV3	520	310	0.02%	0.002%
21	4.722	1143	1145	1148	rBV2	197	140	0.01%	0.001%
22	4.770	1157	1160	1162	rBV2	364	210	0.01%	0.002%
23	4.870	1189	1191	1193	rVB	379	157	0.01%	0.001%
24	4.889	1193	1197	1198	rBV	317	223	0.01%	0.002%
25	4.918	1203	1206	1208	rBV3	435	204	0.01%	0.002%
26	4.944	1213	1214	1217	rBV2	152	90	0.01%	0.001%
27	4.963	1217	1220	1222	rVB2	416	273	0.02%	0.002%
28	4.976	1222	1224	1229	rBV3	350	286	0.02%	0.002%
29	5.050	1229	1247	1280	rBV2	627019	1618714	100.00%	12.327%
30	5.474	1376	1379	1381	rBV	273	202	0.01%	0.002%
31	5.487	1381	1383	1384	rVB	349	87	0.01%	0.001%
32	5.539	1397	1399	1404	rBV3	418	286	0.02%	0.002%
33	5.619	1411	1424	1453	rBV	517250	1047448	64.71%	7.977%
34	5.912	1502	1515	1531	rBV3	23474	50109	3.10%	0.382%
35	6.072	1551	1565	1594	rBV	354911	722562	44.64%	5.503%
36	6.314	1638	1640	1643	rBV3	403	281	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021485.D
 Acq On : 03 Jun 2021 14:23
 Operator : SY/MD
 Sample : M2605-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.352	1649	1652	1660	rVB6	675	855	0.05%	0.007%
38	6.407	1666	1669	1671	rBV3	496	254	0.02%	0.002%
39	6.487	1691	1694	1696	rVB	454	289	0.02%	0.002%
40	6.500	1696	1698	1700	rBV2	542	339	0.02%	0.003%
41	6.735	1768	1771	1773	rBV2	348	208	0.01%	0.002%
42	6.770	1777	1782	1787	rVB4	638	694	0.04%	0.005%
43	6.796	1787	1790	1792	rBV2	355	232	0.01%	0.002%
44	6.857	1807	1809	1811	rVB	292	120	0.01%	0.001%
45	6.873	1811	1814	1818	rBV2	239	156	0.01%	0.001%
46	6.934	1828	1833	1835	rBV4	266	300	0.02%	0.002%
47	6.989	1839	1850	1882	rVV	226508	409889	25.32%	3.122%
48	7.317	1940	1952	1971	rBV	791937	1373261	84.84%	10.458%
49	7.625	2037	2048	2073	rBV	151514	270307	16.70%	2.059%
50	7.899	2130	2133	2136	rBV4	501	368	0.02%	0.003%
51	7.944	2136	2147	2158	rVV3	14251	26604	1.64%	0.203%
52	8.047	2176	2179	2181	rBV2	605	357	0.02%	0.003%
53	8.088	2183	2192	2237	rVV	443740	823647	50.88%	6.272%
54	8.532	2327	2330	2336	rBV3	312	345	0.02%	0.003%
55	8.593	2344	2349	2350	rBV	275	260	0.02%	0.002%
56	8.648	2363	2366	2370	rBV3	382	264	0.02%	0.002%
57	8.677	2372	2375	2378	rBV3	382	258	0.02%	0.002%
58	8.706	2383	2384	2386	rVB3	319	101	0.01%	0.001%
59	8.722	2386	2389	2391	rBV	392	179	0.01%	0.001%
60	8.738	2392	2394	2398	rBV	352	210	0.01%	0.002%
61	8.854	2418	2430	2460	rBV	761865	1256075	77.60%	9.566%
62	9.130	2513	2516	2517	rBV2	515	306	0.02%	0.002%
63	9.153	2517	2523	2524	rBV3	992	972	0.06%	0.007%
64	9.223	2541	2545	2549	rBV2	414	390	0.02%	0.003%
65	9.249	2550	2553	2557	rVV	413	334	0.02%	0.003%
66	9.272	2557	2560	2564	rVB3	339	230	0.01%	0.002%
67	9.394	2595	2598	2600	rVB	265	153	0.01%	0.001%
68	9.448	2614	2615	2617	rVB2	305	96	0.01%	0.001%
69	9.497	2627	2630	2631	rBV	243	132	0.01%	0.001%
70	9.555	2642	2648	2655	rBV3	768	959	0.06%	0.007%
71	9.593	2658	2660	2665	rVV4	621	460	0.03%	0.004%
72	9.651	2676	2678	2681	rBV	430	338	0.02%	0.003%
73	9.767	2712	2714	2717	rBV	356	190	0.01%	0.001%
74	9.825	2726	2732	2734	rBV4	1739	1849	0.11%	0.014%
75	9.918	2758	2761	2764	rBV2	266	224	0.01%	0.002%
76	9.989	2777	2783	2786	rBV3	294	336	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
 Data File : VV021485.D
 Acq On : 03 Jun 2021 14:23
 Operator : SY/MD
 Sample : M2605-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	10.130	2817	2827	2838	rBV4	3895	6505	0.40%	0.050%
78	10.217	2842	2854	2876	rBV	519937	812735	50.21%	6.189%
79	10.384	2896	2906	2919	rVB	27821	47308	2.92%	0.360%
80	10.551	2954	2958	2960	rBV4	570	499	0.03%	0.004%
81	10.712	3006	3008	3009	rBV2	229	86	0.01%	0.001%
82	10.738	3014	3016	3019	rVB2	252	137	0.01%	0.001%
83	10.773	3024	3027	3029	rBV4	477	400	0.02%	0.003%
84	10.834	3042	3046	3050	rBV3	542	515	0.03%	0.004%
85	10.921	3066	3073	3075	rBV5	4634	5065	0.31%	0.039%
86	11.146	3134	3143	3153	rBV5	2498	5374	0.33%	0.041%
87	11.249	3164	3175	3200	rBV	898375	1375332	84.96%	10.474%
88	11.471	3240	3244	3248	rBV3	684	673	0.04%	0.005%
89	11.625	3279	3292	3315	rBV	876526	1360035	84.02%	10.357%
90	11.837	3356	3358	3359	rBV	274	113	0.01%	0.001%
91	11.850	3359	3362	3367	rVB4	937	862	0.05%	0.007%
92	11.873	3367	3369	3373	rBV2	271	158	0.01%	0.001%
93	11.979	3400	3402	3403	rBV	325	121	0.01%	0.001%
94	12.017	3410	3414	3417	rBV2	484	383	0.02%	0.003%
95	12.175	3460	3463	3464	rBV	451	177	0.01%	0.001%
96	12.252	3482	3487	3499	rVB3	4436	6180	0.38%	0.047%
97	12.464	3552	3553	3557	rBV	358	253	0.02%	0.002%
98	12.513	3565	3568	3570	rBV2	731	397	0.02%	0.003%
99	12.699	3625	3626	3632	rVB3	375	233	0.01%	0.002%
100	13.770	3957	3959	3963	rBV2	696	407	0.03%	0.003%


Sum of corrected areas: 13131082

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021485.D
Acq On : 03 Jun 2021 14:23
Operator : SY/MD
Sample : M2605-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG7H2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

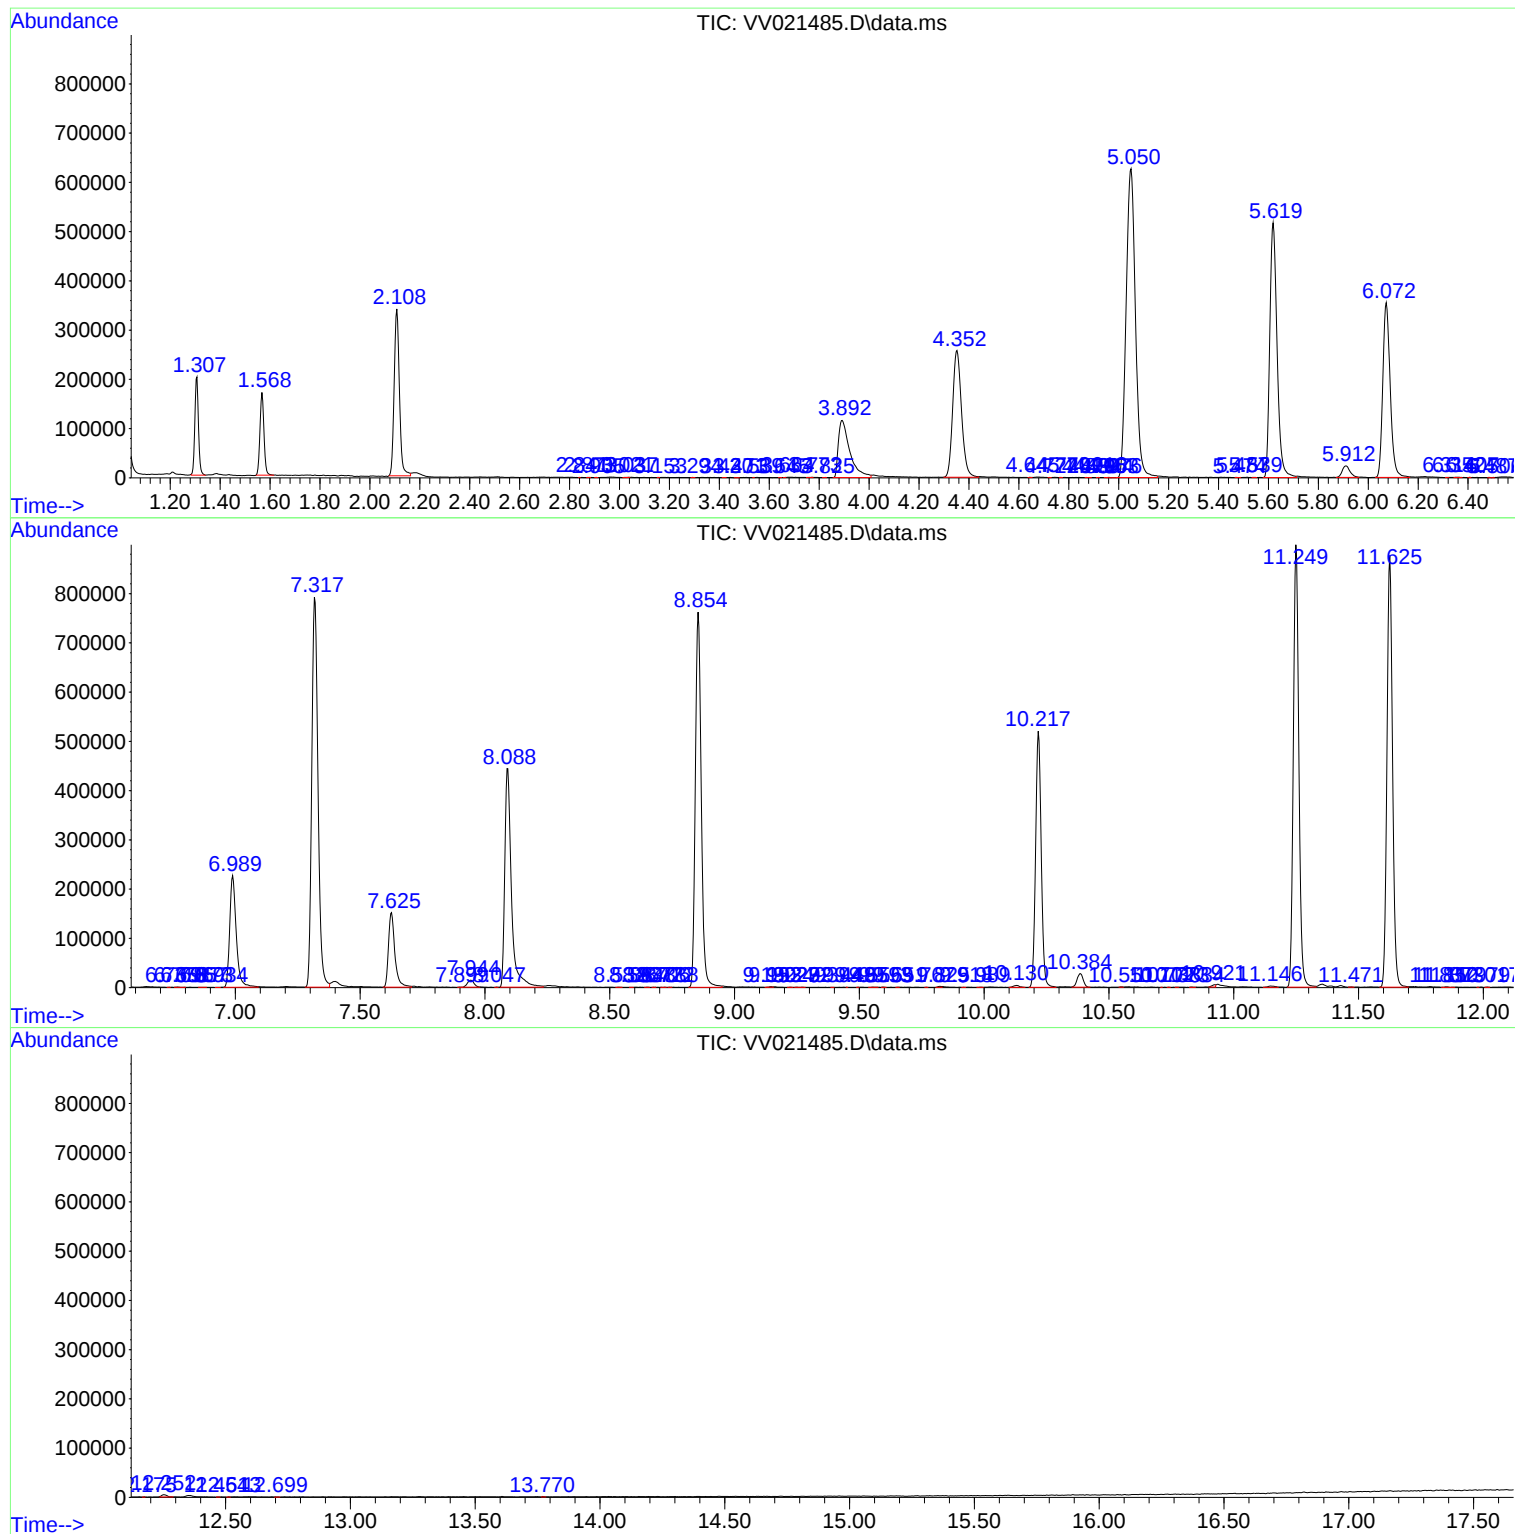

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021485.D
Acq On : 03 Jun 2021 14:23
Operator : SY/MD
Sample : M2605-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060321\
Data File : VV021485.D
Acq On : 03 Jun 2021 14:23
Operator : SY/MD
Sample : M2605-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
