
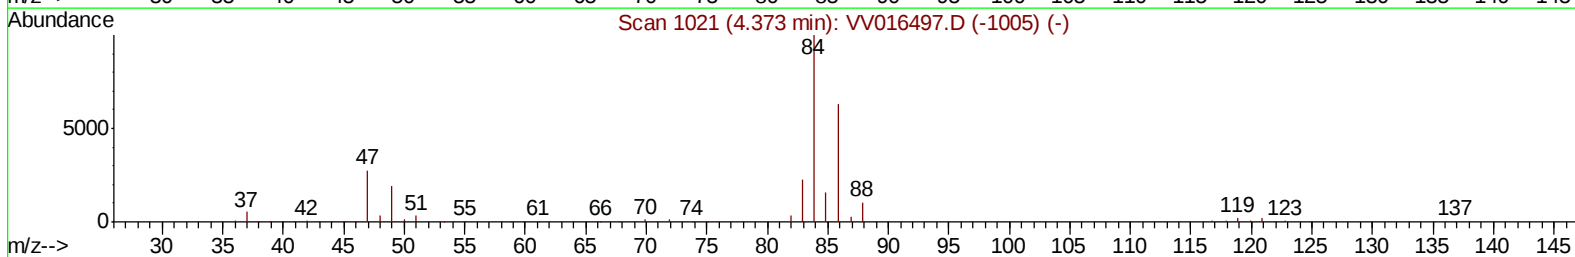
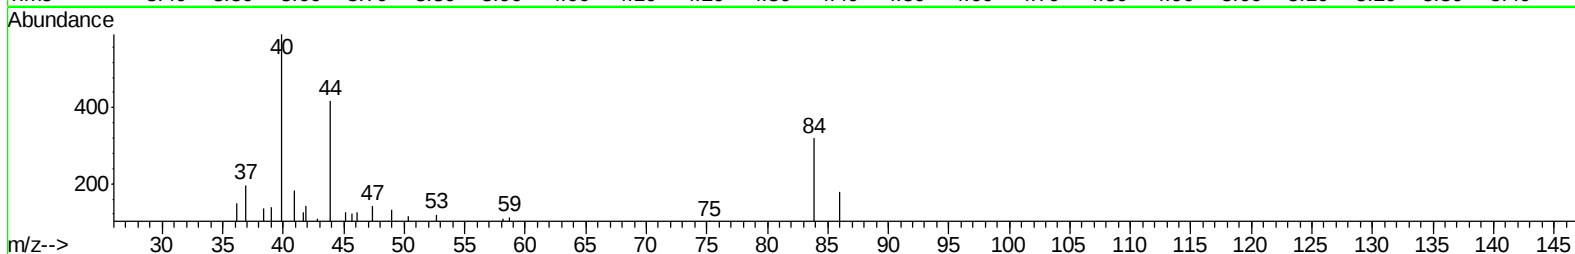


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016502.D
 Acq On : 04 Jun 2020 12:08
 Operator : SY/MD
 Sample : L2869-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Jun 05 01:54:17 2020
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 05 01:52:01 2020
 Response via : Initial Calibration

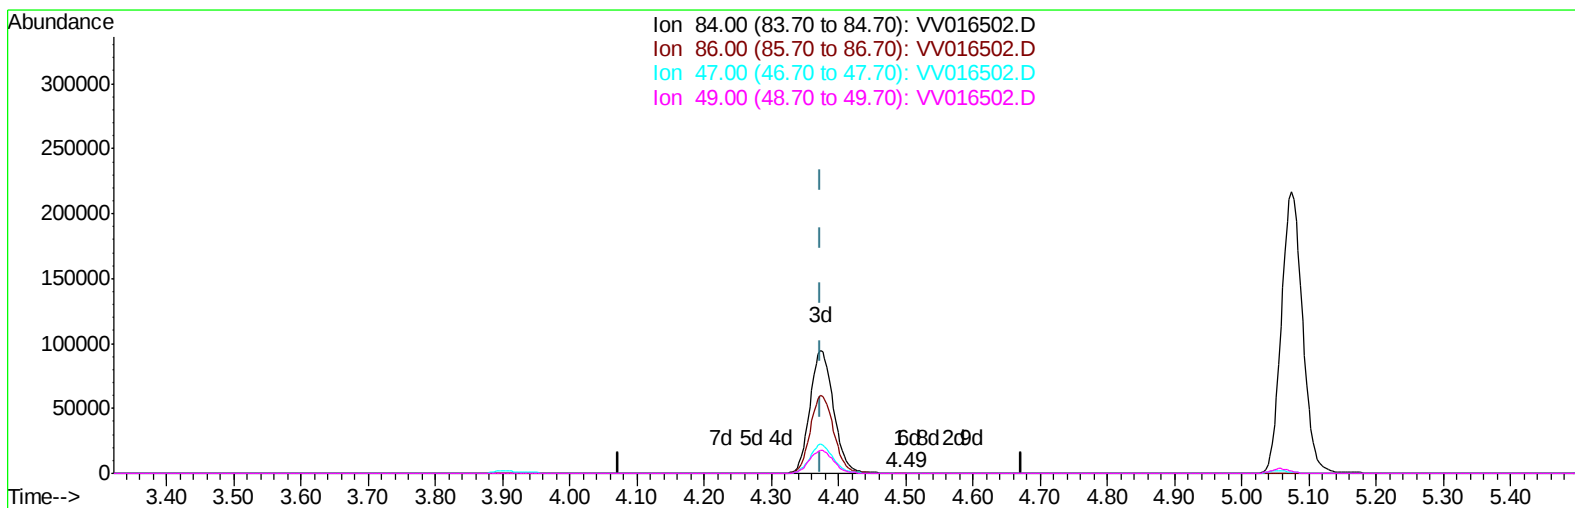

TIC: VV016502.D

(24) Chloroform-d (S)

4.492min (+0.119) 0.05ug/L

response 268

Ion	Exp%	Act%
84.00	100	100
86.00	61.90	70.52
47.00	45.00	45.52
49.00	27.10	23.88