
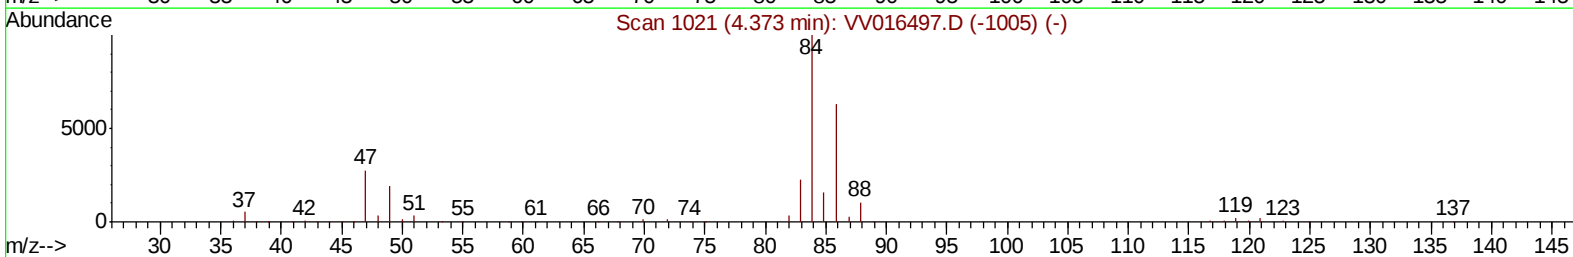
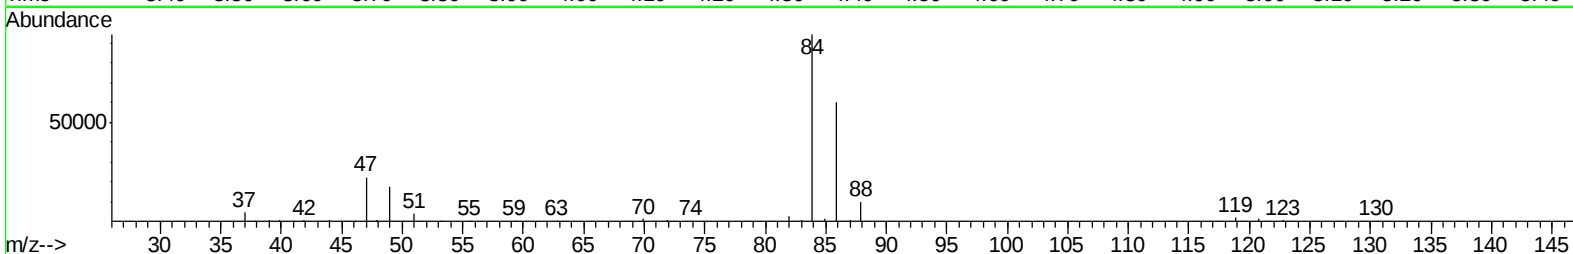


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016502.D
Acq On : 04 Jun 2020 12:08
Operator : SY/MD
Sample : L2869-03DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Jun 05 01:54:17 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 05 01:52:01 2020
Response via : Initial Calibration

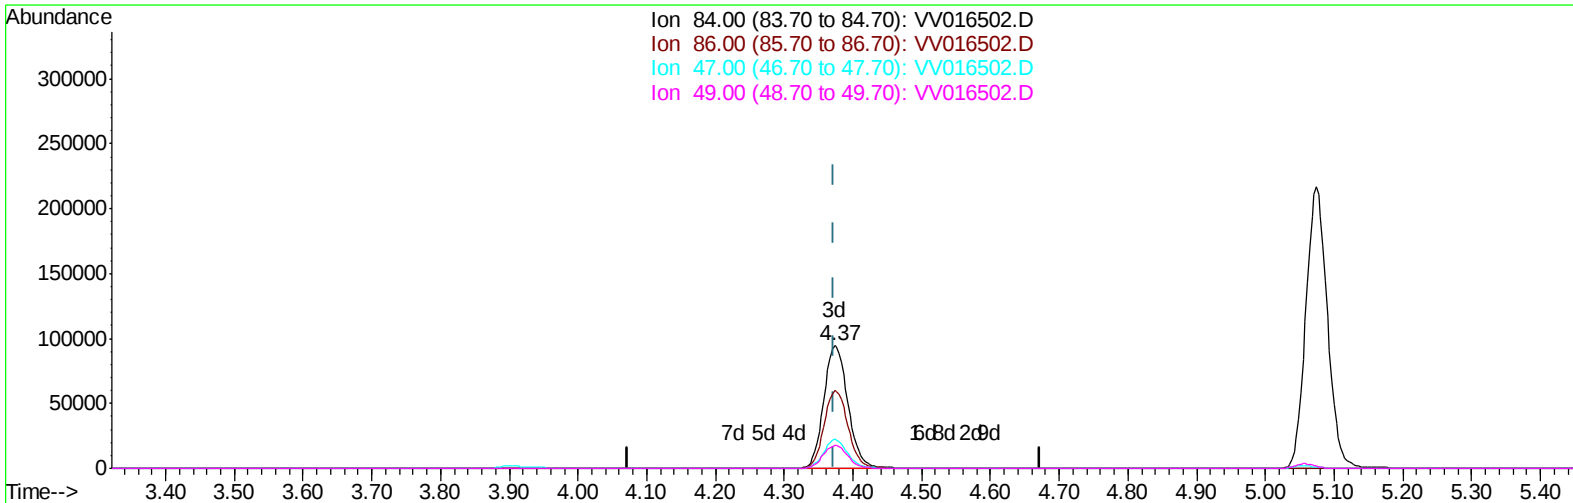

TIC: VV016502.D

(24) Chloroform-d (S)

4.373min (-0.000) 46.45ug/L m

response 229791

Ion	Exp%	Act%
84.00	100	100
86.00	61.90	0.08#
47.00	45.00	0.05#
49.00	27.10	0.03#