

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016498.D
 Acq On : 04 Jun 2020 10:32
 Operator : SY/MD
 Sample : VV0604WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	170965	177092	12.58%	1.630%
2	1.576	145	151	163	rVB	150349	175266	12.45%	1.613%
3	2.122	312	321	341	rVB	272698	402604	28.59%	3.705%
4	2.611	470	473	477	rBV6	985	1101	0.08%	0.010%
5	2.711	502	504	506	rBV2	1034	547	0.04%	0.005%
6	2.746	510	515	517	rBV6	1916	1763	0.13%	0.016%
7	2.929	570	572	574	rBV3	1060	469	0.03%	0.004%
8	3.119	625	631	635	rBV7	2010	2906	0.21%	0.027%
9	3.151	639	641	643	rVV2	971	343	0.02%	0.003%
10	3.257	670	674	675	rBV4	867	616	0.04%	0.006%
11	3.296	683	686	689	rBV4	1616	969	0.07%	0.009%
12	3.383	712	713	719	rVB5	1473	890	0.06%	0.008%
13	3.463	737	738	739	rBV	855	317	0.02%	0.003%
14	3.518	754	755	757	rBV2	608	230	0.02%	0.002%
15	3.560	766	768	769	rBV2	1270	367	0.03%	0.003%
16	3.717	815	817	818	rBV2	663	257	0.02%	0.002%
17	3.749	823	827	831	rBV4	1673	1657	0.12%	0.015%
18	3.788	837	839	842	rBV4	1440	656	0.05%	0.006%
19	3.804	842	844	845	rBV2	1031	411	0.03%	0.004%
20	3.827	849	851	852	rBV2	1137	545	0.04%	0.005%
21	3.894	861	872	899	rBV	122073	328328	23.32%	3.022%
22	4.222	972	974	975	rBV2	1491	534	0.04%	0.005%
23	4.293	994	996	1003	rBV7	1509	1732	0.12%	0.016%
24	4.373	1008	1021	1043	rVB	231848	561068	39.85%	5.164%
25	4.736	1132	1134	1136	rVB3	1157	443	0.03%	0.004%
26	4.749	1136	1138	1141	rBV3	1823	922	0.07%	0.008%
27	4.833	1159	1164	1165	rBV4	1612	1678	0.12%	0.015%
28	4.913	1187	1189	1191	rBV3	927	325	0.02%	0.003%
29	4.955	1200	1202	1204	rBV3	1495	688	0.05%	0.006%
30	5.068	1221	1237	1260	rBV2	553438	1408058	100.00%	12.958%
31	5.576	1391	1395	1396	rBV4	1175	944	0.07%	0.009%
32	5.637	1402	1414	1438	rBV	429908	844568	59.98%	7.773%
33	6.090	1543	1555	1574	rBV	326327	651595	46.28%	5.997%
34	6.273	1610	1612	1613	rBV2	1425	462	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016498.D
 Acq On : 04 Jun 2020 10:32
 Operator : SY/MD
 Sample : VV0604WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.389	1646	1648	1651	rBV3	1111	633	0.04%	0.006%
36	6.466	1671	1672	1674	rBV2	1062	601	0.04%	0.006%
37	6.482	1674	1677	1680	rVV3	1612	1266	0.09%	0.012%
38	6.759	1760	1763	1769	rVB8	1483	1365	0.10%	0.013%
39	6.788	1769	1772	1778	rVB5	2033	1916	0.14%	0.018%
40	6.820	1778	1782	1785	rBV3	1359	816	0.06%	0.008%
41	6.843	1785	1789	1790	rBV3	791	587	0.04%	0.005%
42	6.855	1790	1793	1795	rBV4	1353	913	0.06%	0.008%
43	6.881	1799	1801	1803	rBV3	836	447	0.03%	0.004%
44	7.003	1826	1839	1859	rBV	177905	324628	23.06%	2.988%
45	7.334	1930	1942	1960	rBV	662219	1148103	81.54%	10.566%
46	7.640	2027	2037	2053	rBV	127805	216874	15.40%	1.996%
47	8.042	2160	2162	2164	rBV3	1194	615	0.04%	0.006%
48	8.103	2171	2181	2203	rBV	416724	701738	49.84%	6.458%
49	8.572	2325	2327	2331	rBV3	880	560	0.04%	0.005%
50	8.595	2331	2334	2337	rBV5	1268	949	0.07%	0.009%
51	8.752	2381	2383	2385	rBV3	1273	422	0.03%	0.004%
52	8.781	2390	2392	2395	rBV3	879	567	0.04%	0.005%
53	8.871	2408	2420	2436	rBV	646515	1041568	73.97%	9.586%
54	9.013	2461	2464	2465	rBV3	1385	751	0.05%	0.007%
55	9.437	2592	2596	2597	rBV3	967	562	0.04%	0.005%
56	9.450	2597	2600	2602	rBV3	935	541	0.04%	0.005%
57	9.476	2607	2608	2609	rBV	940	288	0.02%	0.003%
58	9.649	2659	2662	2664	rBV3	1527	995	0.07%	0.009%
59	9.762	2693	2697	2702	rBV6	1350	1645	0.12%	0.015%
60	9.785	2702	2704	2706	rVB3	1468	550	0.04%	0.005%
61	9.797	2706	2708	2710	rBV2	915	513	0.04%	0.005%
62	9.842	2717	2722	2723	rBV5	1779	1407	0.10%	0.013%
63	10.164	2820	2822	2824	rVB4	1322	409	0.03%	0.004%
64	10.238	2833	2845	2861	rBV	448075	695699	49.41%	6.403%
65	10.444	2905	2909	2912	rBV5	2036	1475	0.10%	0.014%
66	10.694	2984	2987	2989	rBV3	1822	1240	0.09%	0.011%
67	10.723	2993	2996	2998	rVV3	1307	786	0.06%	0.007%
68	10.749	3002	3004	3006	rBV3	681	380	0.03%	0.003%
69	11.270	3155	3166	3192	rBV	672315	1013148	71.95%	9.324%
70	11.559	3253	3256	3257	rBV3	834	428	0.03%	0.004%
71	11.646	3271	3283	3301	rBV	704803	1098323	78.00%	10.108%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016498.D
 Acq On : 04 Jun 2020 10:32
 Operator : SY/MD
 Sample : VV0604WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	12.128	3432	3433	3434	rBV	995	297	0.02%	0.003%
73	12.440	3526	3530	3532	rBV4	1169	810	0.06%	0.007%
74	12.640	3590	3592	3593	rBV2	831	354	0.03%	0.003%
75	12.714	3613	3615	3616	rBV2	1228	525	0.04%	0.005%
76	12.800	3640	3642	3643	rBV2	628	189	0.01%	0.002%
77	12.820	3646	3648	3651	rVB4	1170	603	0.04%	0.006%
78	12.871	3663	3664	3665	rBV	1081	339	0.02%	0.003%
79	12.939	3683	3685	3686	rBV2	660	206	0.01%	0.002%
80	13.029	3711	3713	3716	rVB4	1044	458	0.03%	0.004%
81	13.103	3734	3736	3739	rBV3	1165	912	0.06%	0.008%
82	13.145	3746	3749	3751	rBV3	1685	1093	0.08%	0.010%
83	13.222	3771	3773	3775	rBV3	1455	897	0.06%	0.008%
84	13.530	3859	3869	3879	rBV3	8682	15863	1.13%	0.146%
85	13.669	3908	3912	3915	rBV3	1172	999	0.07%	0.009%
86	13.823	3958	3960	3961	rBV2	1442	611	0.04%	0.006%
87	13.993	4012	4013	4022	rVB8	1559	1486	0.11%	0.014%
88	14.029	4022	4024	4025	rBV2	886	268	0.02%	0.002%
89	14.238	4088	4089	4092	rBV3	1044	516	0.04%	0.005%
90	14.337	4117	4120	4123	rBV5	1455	1147	0.08%	0.011%
91	14.447	4151	4154	4160	rBV6	1497	1545	0.11%	0.014%
92	14.733	4241	4243	4248	rBV5	1533	1221	0.09%	0.011%
93	14.836	4272	4275	4276	rBV2	1690	989	0.07%	0.009%
94	15.466	4469	4471	4473	rBV2	1522	600	0.04%	0.006%


Sum of corrected areas: 10865987

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016498.D
Acq On : 04 Jun 2020 10:32
Operator : SY/MD
Sample : VV0604WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK67

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

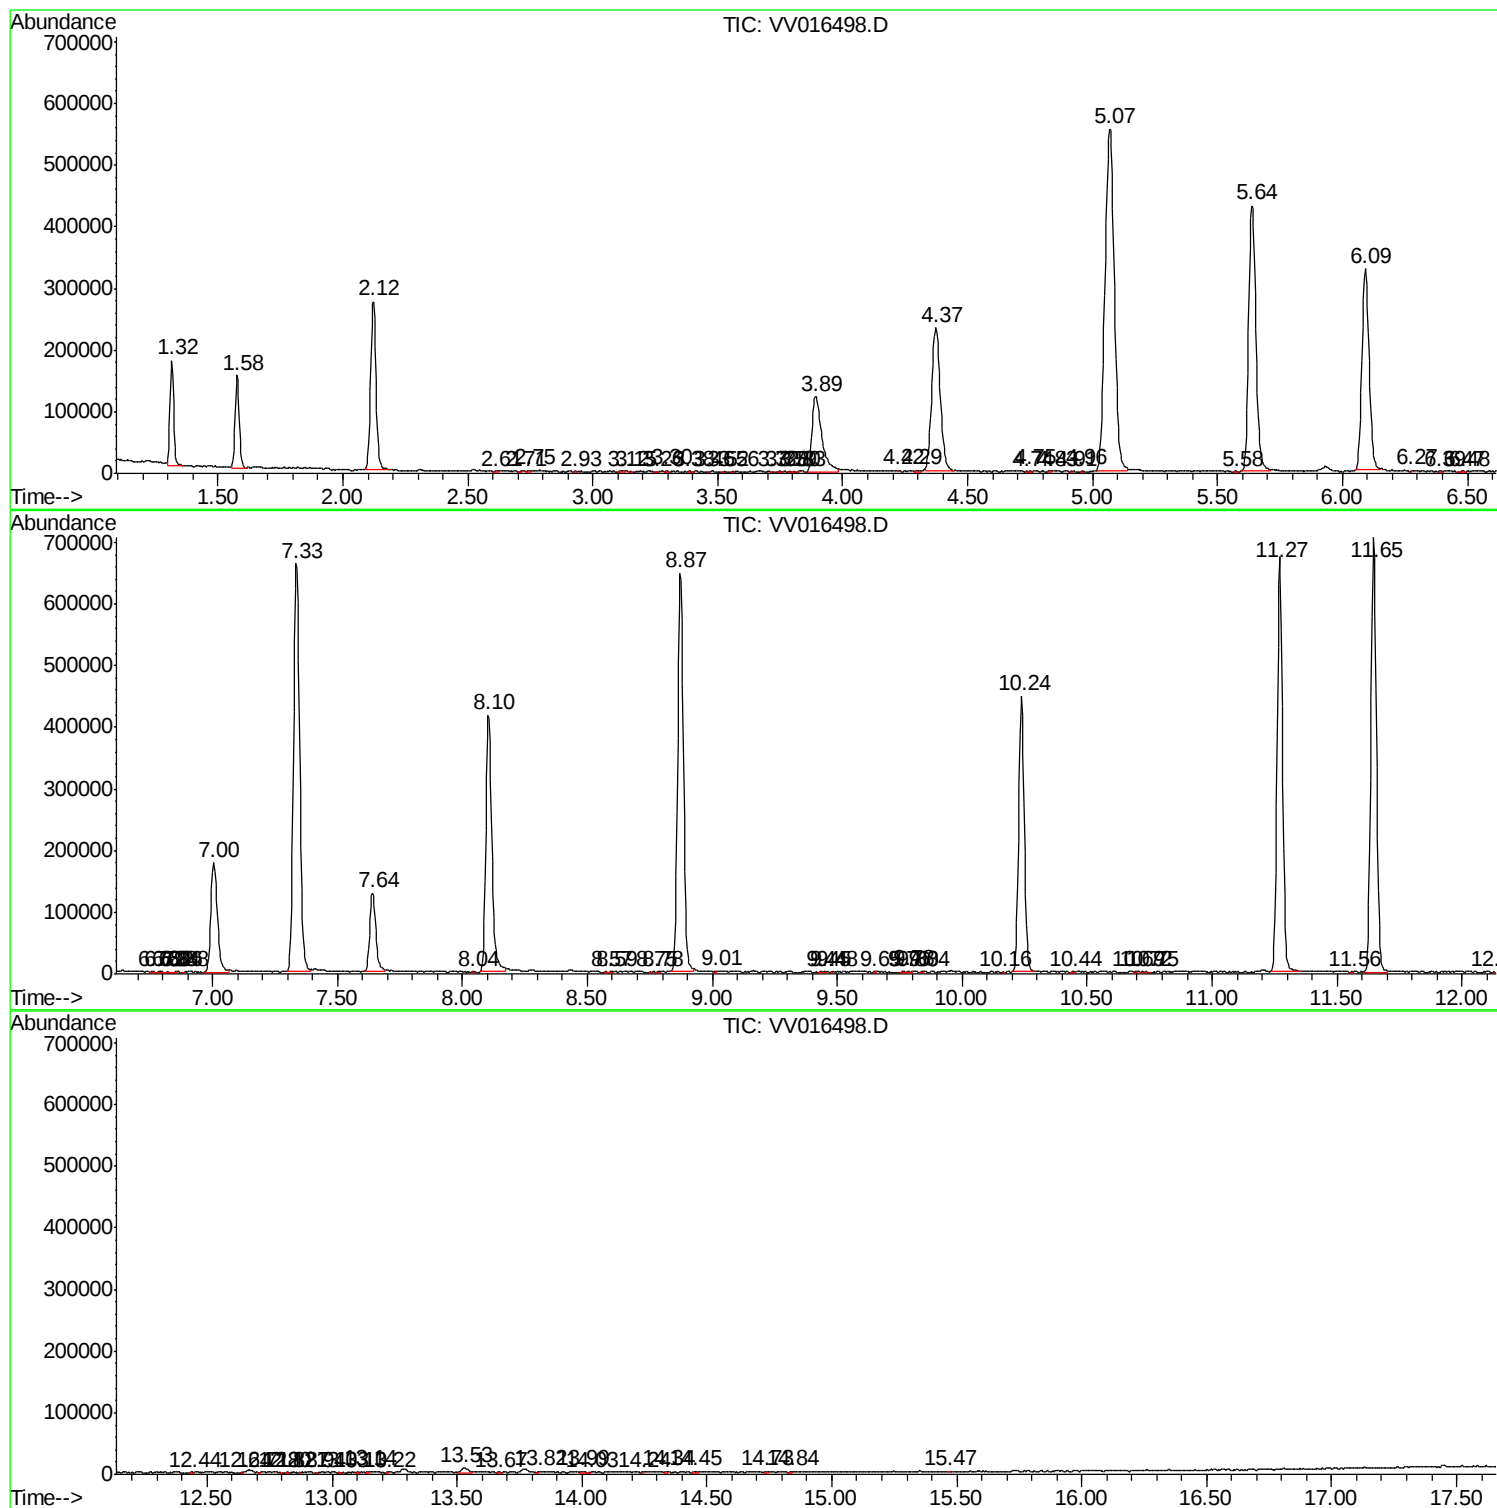

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016498.D
Acq On : 04 Jun 2020 10:32
Operator : SY/MD
Sample : VV0604WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK67

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060420\
Data File : VV016498.D
Acq On : 04 Jun 2020 10:32
Operator : SY/MD
Sample : VV0604WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK67

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc