

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016499.D
 Acq On : 04 Jun 2020 10:58
 Operator : SY/MD
 Sample : L2844-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	85	rVB	170523	179550	12.30%	1.634%
2	1.569	144	149	158	rVB	116269	124838	8.55%	1.136%
3	2.119	311	320	337	rVB	276800	404149	27.69%	3.679%
4	2.634	478	480	481	rBV2	1290	541	0.04%	0.005%
5	2.807	532	534	538	rBV2	1089	627	0.04%	0.006%
6	2.936	569	574	579	rBV7	1781	2076	0.14%	0.019%
7	3.065	611	614	617	rVB4	1050	708	0.05%	0.006%
8	3.087	617	621	625	rBV5	1244	1288	0.09%	0.012%
9	3.232	663	666	669	rVB3	1199	890	0.06%	0.008%
10	3.277	678	680	683	rVB3	1468	730	0.05%	0.007%
11	3.344	697	701	703	rBV3	1110	790	0.05%	0.007%
12	3.418	721	724	728	rVB4	1700	1141	0.08%	0.010%
13	3.444	728	732	736	rVB6	1525	1449	0.10%	0.013%
14	3.466	736	739	740	rBV3	1441	879	0.06%	0.008%
15	3.531	756	759	764	rVB6	1184	953	0.07%	0.009%
16	3.682	804	806	809	rBV3	1054	551	0.04%	0.005%
17	3.708	809	814	817	rBV6	1789	1319	0.09%	0.012%
18	3.727	817	820	822	rBV3	999	506	0.03%	0.005%
19	3.740	822	824	827	rBV3	926	495	0.03%	0.005%
20	3.833	850	853	856	rBV4	1260	890	0.06%	0.008%
21	3.897	862	873	900	rBV2	119142	326028	22.34%	2.968%
22	4.373	1003	1021	1042	rBV2	239065	588826	40.35%	5.360%
23	4.640	1099	1104	1106	rBV4	1133	945	0.06%	0.009%
24	4.753	1137	1139	1141	rBV2	905	577	0.04%	0.005%
25	4.955	1197	1202	1204	rBV4	1141	1112	0.08%	0.010%
26	5.068	1221	1237	1260	rBV3	568541	1459447	100.00%	13.285%
27	5.341	1321	1322	1324	rBV2	1547	690	0.05%	0.006%
28	5.450	1354	1356	1361	rVB5	2026	1146	0.08%	0.010%
29	5.473	1361	1363	1365	rVB3	1525	648	0.04%	0.006%
30	5.640	1401	1415	1438	rBV	439808	870085	59.62%	7.920%
31	6.042	1538	1540	1542	rBV3	1180	628	0.04%	0.006%
32	6.093	1542	1556	1575	rVV	340350	682089	46.74%	6.209%
33	6.547	1694	1697	1698	rBV2	1277	585	0.04%	0.005%
34	6.691	1740	1742	1744	rBV3	1948	869	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016499.D
 Acq On : 04 Jun 2020 10:58
 Operator : SY/MD
 Sample : L2844-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.707	1744	1747	1750	rVB5	2374	1491	0.10%	0.014%
36	6.730	1750	1754	1758	rBV6	1920	1579	0.11%	0.014%
37	6.894	1802	1805	1807	rBV3	1216	601	0.04%	0.005%
38	6.955	1822	1824	1827	rBV3	926	645	0.04%	0.006%
39	7.007	1827	1840	1856	rBV	183802	329738	22.59%	3.002%
40	7.338	1931	1943	1959	rBV	685863	1174292	80.46%	10.690%
41	7.640	2027	2037	2057	rBV	131236	221762	15.19%	2.019%
42	7.785	2081	2082	2084	rBV2	984	497	0.03%	0.005%
43	7.900	2116	2118	2121	rBV4	1084	772	0.05%	0.007%
44	8.106	2171	2182	2205	rBV	418808	716593	49.10%	6.523%
45	8.643	2345	2349	2351	rBV4	1520	993	0.07%	0.009%
46	8.871	2408	2420	2441	rBV	653857	1066794	73.10%	9.711%
47	9.084	2484	2486	2488	rBV3	2014	1083	0.07%	0.010%
48	9.125	2497	2499	2502	rBV4	1396	894	0.06%	0.008%
49	9.151	2505	2507	2510	rBV4	1799	1216	0.08%	0.011%
50	9.203	2522	2523	2528	rBV4	1366	1216	0.08%	0.011%
51	9.238	2532	2534	2537	rVB3	1774	1016	0.07%	0.009%
52	9.370	2572	2575	2579	rVB6	1183	964	0.07%	0.009%
53	9.399	2582	2584	2589	rVV4	1244	753	0.05%	0.007%
54	9.691	2673	2675	2677	rVB3	1391	591	0.04%	0.005%
55	9.707	2677	2680	2682	rBV4	1592	972	0.07%	0.009%
56	9.836	2717	2720	2721	rBV2	967	529	0.04%	0.005%
57	9.871	2729	2731	2734	rBV4	775	550	0.04%	0.005%
58	9.884	2734	2735	2738	rVB3	1104	545	0.04%	0.005%
59	10.013	2773	2775	2778	rBV4	1240	728	0.05%	0.007%
60	10.145	2813	2816	2818	rBV3	1096	718	0.05%	0.007%
61	10.170	2821	2824	2827	rBV4	1269	860	0.06%	0.008%
62	10.238	2833	2845	2860	rBV	450596	699571	47.93%	6.368%
63	10.338	2874	2876	2879	rBV3	968	593	0.04%	0.005%
64	10.524	2932	2934	2937	rBV4	1262	955	0.07%	0.009%
65	10.733	2996	2999	3001	rBV4	1764	1348	0.09%	0.012%
66	10.788	3012	3016	3019	rBV6	761	783	0.05%	0.007%
67	11.061	3098	3101	3104	rBV3	1508	1157	0.08%	0.011%
68	11.138	3124	3125	3128	rVB3	997	543	0.04%	0.005%
69	11.270	3154	3166	3180	rBV	655869	986178	67.57%	8.977%
70	11.646	3270	3283	3300	rBV	696453	1074404	73.62%	9.780%
71	11.797	3328	3330	3335	rBV4	864	736	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016499.D
 Acq On : 04 Jun 2020 10:58
 Operator : SY/MD
 Sample : L2844-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.836	3340	3342	3345	rBV5	1420	733	0.05%	0.007%
73	11.868	3348	3352	3353	rBV4	1235	664	0.05%	0.006%
74	11.987	3387	3389	3391	rBV3	1614	914	0.06%	0.008%
75	12.035	3399	3404	3408	rBV8	1271	1508	0.10%	0.014%
76	12.058	3408	3411	3412	rVV3	1094	570	0.04%	0.005%
77	12.077	3415	3417	3421	rVV5	1696	1075	0.07%	0.010%
78	12.096	3421	3423	3427	rVV3	1121	608	0.04%	0.006%
79	12.157	3439	3442	3444	rBV5	944	694	0.05%	0.006%
80	12.276	3472	3479	3484	rBV9	1732	2807	0.19%	0.026%
81	12.312	3486	3490	3494	rBV5	1834	1521	0.10%	0.014%
82	12.386	3509	3513	3515	rBV4	1653	1188	0.08%	0.011%
83	12.399	3515	3517	3520	rVB3	1473	998	0.07%	0.009%
84	12.492	3543	3546	3547	rBV3	1229	571	0.04%	0.005%
85	12.566	3566	3569	3574	rBV7	1381	1327	0.09%	0.012%
86	12.585	3574	3575	3577	rBV2	1172	551	0.04%	0.005%
87	12.675	3600	3603	3610	rVB7	2466	2088	0.14%	0.019%
88	12.730	3619	3620	3624	rVB3	1143	813	0.06%	0.007%
89	12.755	3624	3628	3629	rBV2	1535	1028	0.07%	0.009%
90	12.794	3639	3640	3643	rVB3	1745	505	0.03%	0.005%
91	12.810	3643	3645	3647	rBV2	1184	530	0.04%	0.005%
92	13.164	3752	3755	3757	rBV3	1142	619	0.04%	0.006%
93	13.202	3765	3767	3769	rBV3	870	518	0.04%	0.005%
94	13.386	3822	3824	3825	rBV3	1311	658	0.05%	0.006%
95	13.489	3854	3856	3860	rVB4	1263	570	0.04%	0.005%
96	13.527	3863	3868	3875	rBV7	4082	6460	0.44%	0.059%
97	13.675	3911	3914	3916	rBV4	1086	707	0.05%	0.006%
98	13.743	3933	3935	3936	rBV2	1777	669	0.05%	0.006%
99	13.948	3996	3999	4001	rBV3	1534	868	0.06%	0.008%
100	14.649	4215	4217	4221	rBV3	1390	876	0.06%	0.008%


Sum of corrected areas: 10985343

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016499.D
Acq On : 04 Jun 2020 10:58
Operator : SY/MD
Sample : L2844-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

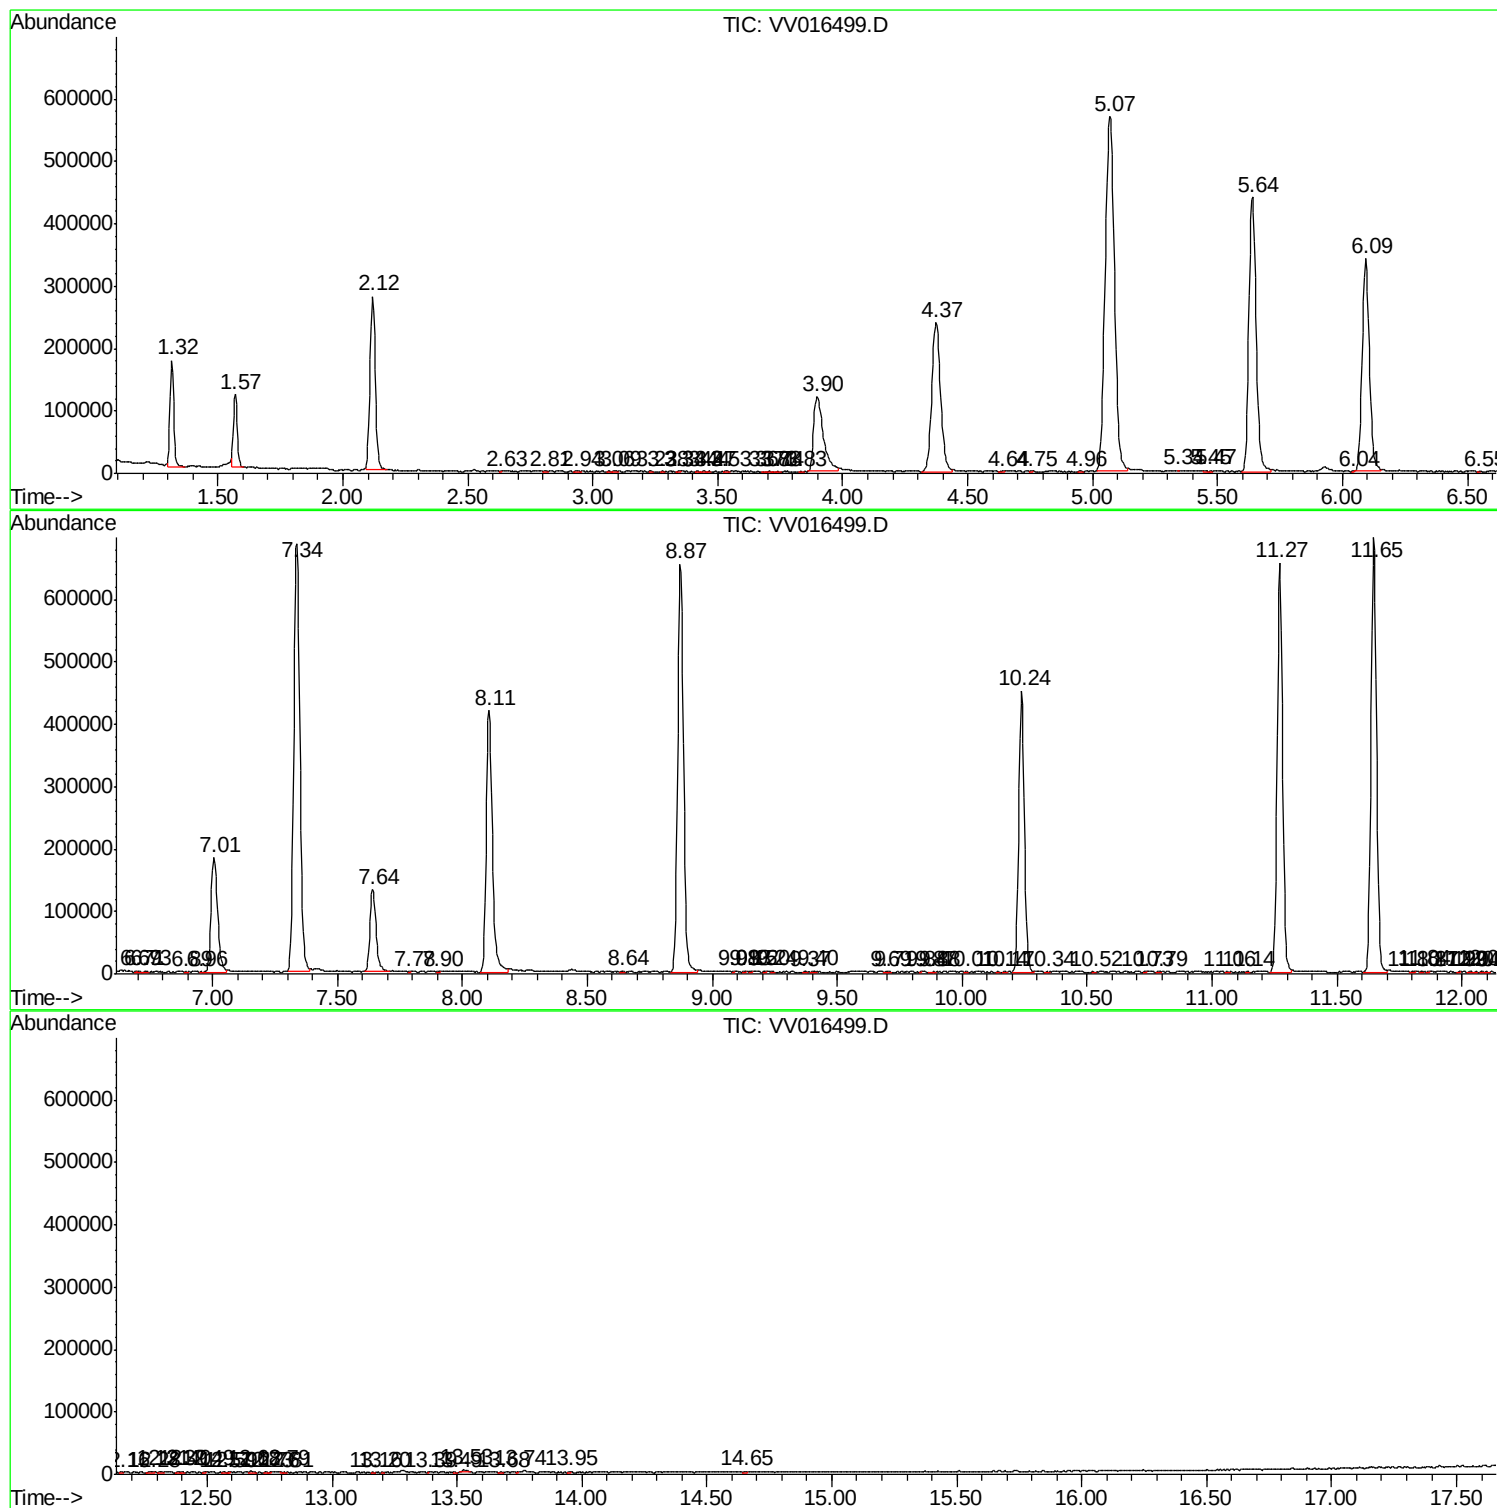

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016499.D
Acq On : 04 Jun 2020 10:58
Operator : SY/MD
Sample : L2844-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016499.D
Acq On : 04 Jun 2020 10:58
Operator : SY/MD
Sample : L2844-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc