

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016501.D
 Acq On : 04 Jun 2020 11:45
 Operator : SY/MD
 Sample : L2869-02DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	172964	178204	12.22%	1.460%
2	1.566	144	148	159	rVB	95500	99547	6.83%	0.815%
3	2.113	308	318	336	rBV	285641	430959	29.55%	3.530%
4	2.283	369	371	373	rBV3	1415	751	0.05%	0.006%
5	2.402	404	408	409	rBV3	1011	629	0.04%	0.005%
6	2.595	466	468	471	rBV3	1155	876	0.06%	0.007%
7	2.692	496	498	500	rBV3	1186	602	0.04%	0.005%
8	2.933	570	573	574	rBV3	1712	857	0.06%	0.007%
9	2.952	577	579	583	rVB4	930	618	0.04%	0.005%
10	3.020	596	600	604	rBV7	1240	1240	0.09%	0.010%
11	3.283	678	682	685	rBV4	1092	1058	0.07%	0.009%
12	3.322	692	694	700	rVB6	1079	796	0.05%	0.007%
13	3.351	700	703	706	rBV4	871	797	0.05%	0.007%
14	3.412	716	722	724	rBV7	1160	1207	0.08%	0.010%
15	3.563	766	769	771	rBV4	1052	502	0.03%	0.004%
16	3.618	784	786	789	rVB3	1110	609	0.04%	0.005%
17	3.637	789	792	793	rBV2	1226	712	0.05%	0.006%
18	3.666	797	801	803	rBV4	867	735	0.05%	0.006%
19	3.695	807	810	814	rBV3	996	628	0.04%	0.005%
20	3.852	856	859	861	rBV3	1043	516	0.04%	0.004%
21	3.904	861	875	908	rBV2	107920	322512	22.11%	2.642%
22	4.373	1006	1021	1047	rVB2	230557	567859	38.93%	4.652%
23	4.653	1107	1108	1111	rBV4	847	516	0.04%	0.004%
24	4.701	1119	1123	1126	rBV6	1549	1061	0.07%	0.009%
25	4.753	1136	1139	1141	rBV4	1006	555	0.04%	0.005%
26	4.766	1141	1143	1145	rBV3	947	510	0.03%	0.004%
27	4.817	1156	1159	1163	rVV5	1256	1094	0.08%	0.009%
28	4.923	1188	1192	1196	rVB5	1475	1283	0.09%	0.011%
29	5.068	1220	1237	1261	rBV2	577511	1458489	100.00%	11.947%
30	5.640	1401	1415	1442	rBV	461113	927766	63.61%	7.600%
31	5.936	1493	1507	1529	rBV	585219	1135284	77.84%	9.300%
32	6.093	1544	1556	1577	rVB	325013	646724	44.34%	5.298%
33	6.544	1694	1696	1698	rBV4	1214	608	0.04%	0.005%
34	6.556	1698	1700	1703	rVV4	1387	798	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016501.D
 Acq On : 04 Jun 2020 11:45
 Operator : SY/MD
 Sample : L2869-02DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.573	1703	1705	1708	rVV4	785	573	0.04%	0.005%
36	6.589	1708	1710	1713	rBV4	1195	645	0.04%	0.005%
37	6.775	1764	1768	1769	rBV3	855	700	0.05%	0.006%
38	6.855	1792	1793	1796	rBV2	1262	670	0.05%	0.005%
39	7.007	1826	1840	1861	rBV	186846	334990	22.97%	2.744%
40	7.338	1931	1943	1960	rBV	669483	1143497	78.40%	9.367%
41	7.640	2027	2037	2052	rBV	129556	221135	15.16%	1.811%
42	7.724	2060	2063	2069	rVB6	1707	1208	0.08%	0.010%
43	7.807	2087	2089	2095	rBV7	1534	1408	0.10%	0.012%
44	7.997	2142	2148	2151	rBV6	2996	3498	0.24%	0.029%
45	8.061	2166	2168	2170	rBV2	1133	714	0.05%	0.006%
46	8.109	2172	2183	2205	rBV	376515	725202	49.72%	5.941%
47	8.871	2406	2420	2440	rBV	698696	1116390	76.54%	9.145%
48	9.129	2497	2500	2502	rBV4	1089	690	0.05%	0.006%
49	9.428	2590	2593	2596	rBV5	1300	920	0.06%	0.008%
50	9.473	2602	2607	2608	rBV4	934	582	0.04%	0.005%
51	9.707	2678	2680	2681	rBV2	1156	540	0.04%	0.004%
52	9.974	2761	2763	2766	rBV3	1000	553	0.04%	0.005%
53	10.113	2801	2806	2808	rBV4	1371	923	0.06%	0.008%
54	10.238	2834	2845	2864	rBV	426475	687680	47.15%	5.633%
55	10.360	2880	2883	2885	rBV4	1108	755	0.05%	0.006%
56	10.447	2907	2910	2912	rBV4	997	547	0.04%	0.004%
57	10.498	2923	2926	2927	rBV2	1124	664	0.05%	0.005%
58	10.637	2966	2969	2972	rBV4	1563	1104	0.08%	0.009%
59	10.714	2990	2993	2995	rBV3	1404	774	0.05%	0.006%
60	10.740	2998	3001	3002	rBV3	1126	658	0.05%	0.005%
61	10.817	3023	3025	3028	rBV3	1111	606	0.04%	0.005%
62	10.852	3032	3036	3038	rBV3	1845	1147	0.08%	0.009%
63	10.990	3077	3079	3085	rVB6	1054	771	0.05%	0.006%
64	11.132	3121	3123	3129	rVB7	959	715	0.05%	0.006%
65	11.158	3129	3131	3134	rBV5	896	617	0.04%	0.005%
66	11.270	3155	3166	3183	rBV	686879	1056745	72.45%	8.656%
67	11.550	3250	3253	3254	rBV2	1298	815	0.06%	0.007%
68	11.582	3260	3263	3269	rVB8	1543	1776	0.12%	0.015%
69	11.646	3269	3283	3301	rBV	688240	1078809	73.97%	8.837%
70	11.762	3315	3319	3322	rVB6	1028	807	0.06%	0.007%
71	11.920	3366	3368	3371	rVB2	1117	697	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016501.D
 Acq On : 04 Jun 2020 11:45
 Operator : SY/MD
 Sample : L2869-02DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.971	3381	3384	3389	rVB7	1453	907	0.06%	0.007%
73	12.026	3397	3401	3403	rBV2	994	689	0.05%	0.006%
74	12.039	3403	3405	3409	rBV4	1284	907	0.06%	0.007%
75	12.100	3418	3424	3431	rBV4	2115	2961	0.20%	0.024%
76	12.151	3438	3440	3444	rVB2	1459	804	0.06%	0.007%
77	12.318	3490	3492	3496	rVB4	1275	687	0.05%	0.006%
78	12.350	3500	3502	3505	rBV3	1243	792	0.05%	0.006%
79	12.495	3542	3547	3548	rBV3	1437	1039	0.07%	0.009%
80	12.540	3557	3561	3562	rBV4	1040	614	0.04%	0.005%
81	12.633	3585	3590	3591	rBV3	953	852	0.06%	0.007%
82	12.858	3656	3660	3662	rVV4	1858	1430	0.10%	0.012%
83	12.878	3664	3666	3670	rVB4	1677	679	0.05%	0.006%
84	12.910	3670	3676	3679	rBV6	1902	2097	0.14%	0.017%
85	13.016	3703	3709	3711	rBV7	1615	1352	0.09%	0.011%
86	13.045	3716	3718	3720	rVV3	1561	768	0.05%	0.006%
87	13.061	3720	3723	3726	rVB5	1198	891	0.06%	0.007%
88	13.260	3783	3785	3790	rVV4	1183	941	0.06%	0.008%
89	13.411	3829	3832	3834	rBV3	1026	700	0.05%	0.006%
90	13.447	3841	3843	3846	rBV4	1357	715	0.05%	0.006%
91	13.637	3898	3902	3905	rBV5	1237	883	0.06%	0.007%
92	13.662	3908	3910	3913	rVV4	1971	907	0.06%	0.007%
93	13.678	3913	3915	3920	rVB3	962	813	0.06%	0.007%
94	13.717	3925	3927	3929	rBV3	1176	588	0.04%	0.005%
95	14.042	4025	4028	4030	rBV4	1836	1056	0.07%	0.009%
96	14.058	4030	4033	4036	rVV4	1578	1363	0.09%	0.011%
97	14.360	4125	4127	4131	rBV4	1210	726	0.05%	0.006%
98	14.701	4231	4233	4241	rBV8	1356	1356	0.09%	0.011%
99	14.746	4243	4247	4251	rBV5	1598	1925	0.13%	0.016%
100	14.984	4319	4321	4322	rBV2	1695	709	0.05%	0.006%


Sum of corrected areas: 12207578

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016501.D
Acq On : 04 Jun 2020 11:45
Operator : SY/MD
Sample : L2869-02DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

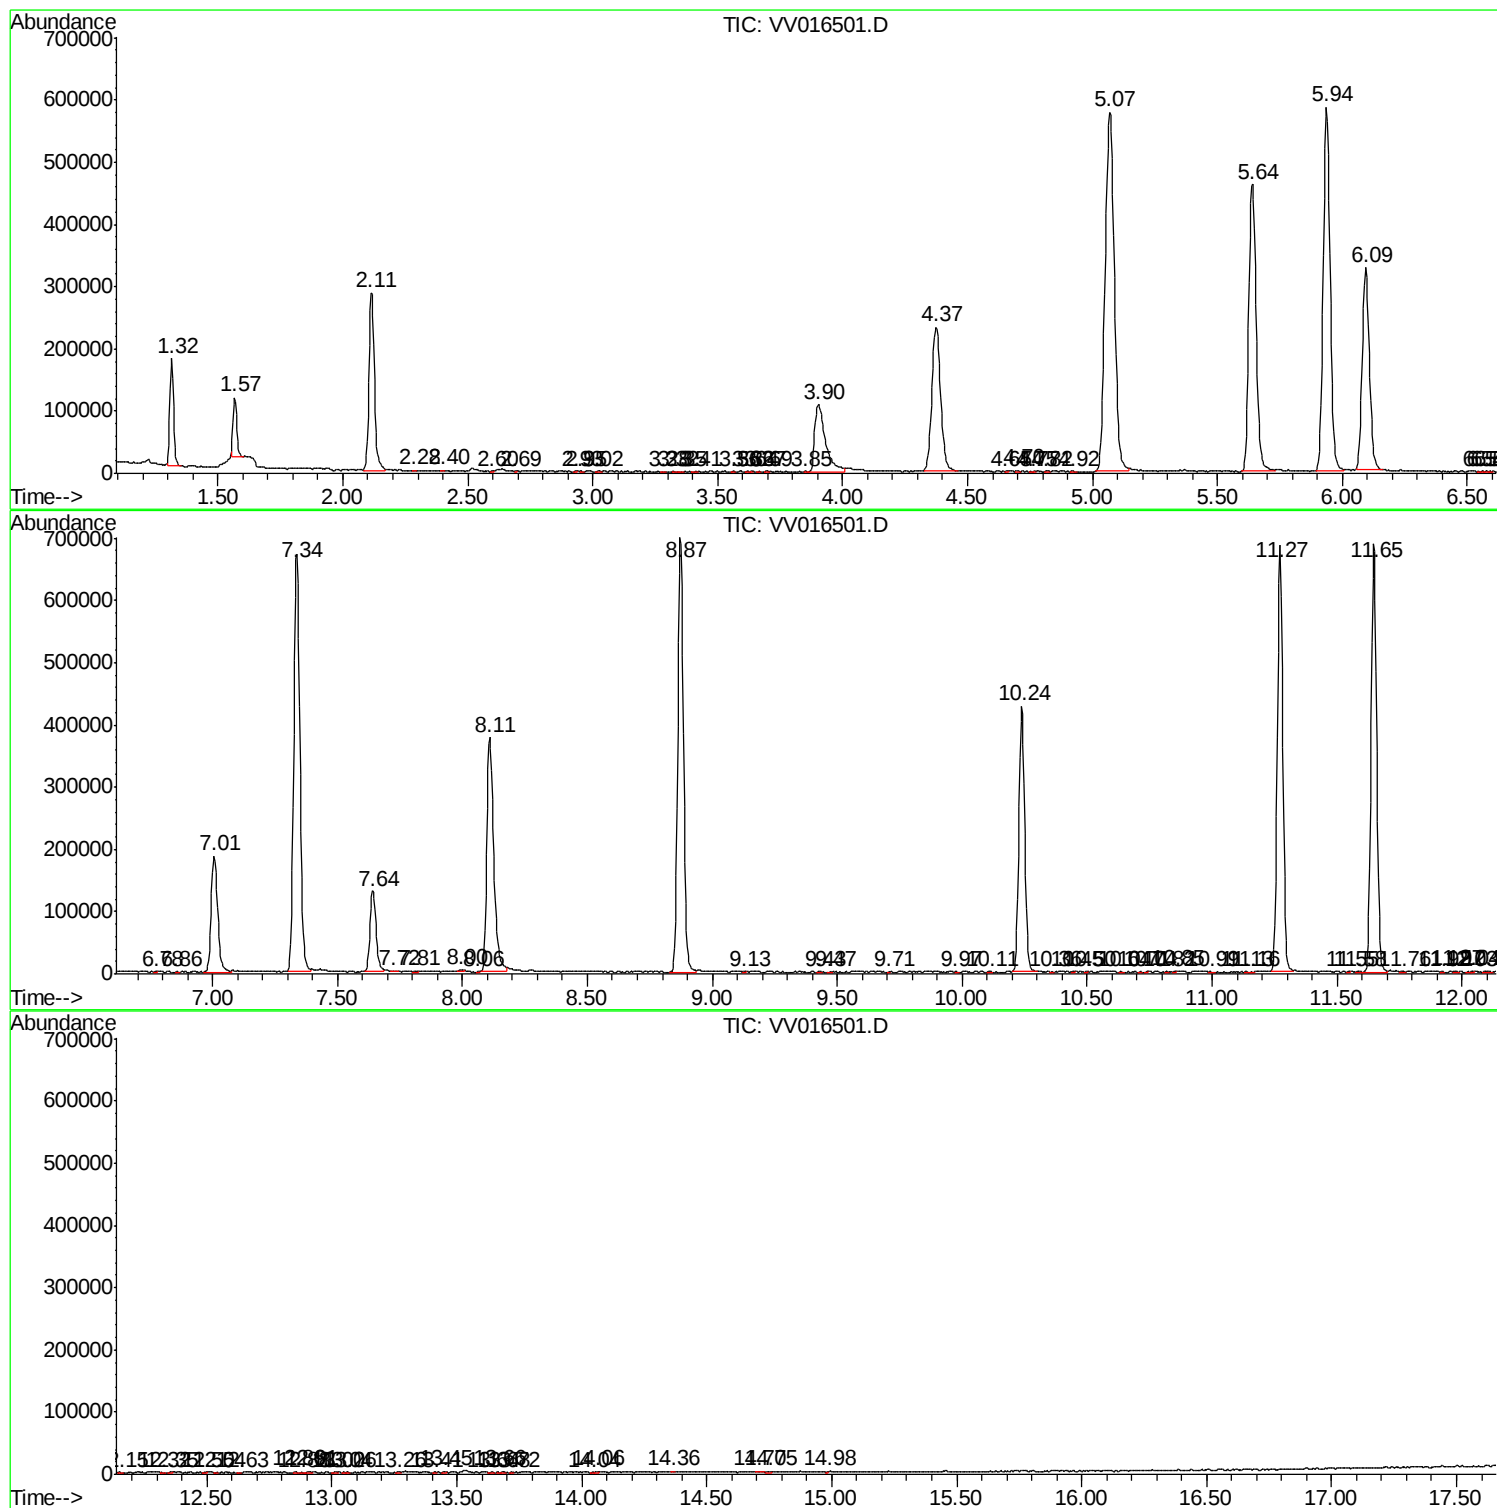

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016501.D
Acq On : 04 Jun 2020 11:45
Operator : SY/MD
Sample : L2869-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016501.D
Acq On : 04 Jun 2020 11:45
Operator : SY/MD
Sample : L2869-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc