

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016502.D
 Acq On : 04 Jun 2020 12:08
 Operator : SY/MD
 Sample : L2869-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	168018	179419	12.43%	1.558%
2	1.566	143	148	163	rVB	110531	145956	10.11%	1.268%
3	2.116	310	319	335	rBV	275400	409303	28.35%	3.555%
4	2.524	440	446	454	rVB9	5401	8440	0.58%	0.073%
5	2.573	459	461	466	rVB5	1625	1152	0.08%	0.010%
6	2.621	470	476	479	rBV8	3184	3807	0.26%	0.033%
7	2.827	536	540	541	rBV2	1357	653	0.05%	0.006%
8	3.026	600	602	605	rBV4	841	621	0.04%	0.005%
9	3.116	627	630	632	rVV2	1120	636	0.04%	0.006%
10	3.203	653	657	660	rBV4	1145	1010	0.07%	0.009%
11	3.290	682	684	686	rBV3	1640	866	0.06%	0.008%
12	3.302	686	688	690	rVV4	1557	687	0.05%	0.006%
13	3.405	717	720	723	rVB5	1092	786	0.05%	0.007%
14	3.528	751	758	761	rBV7	1228	1292	0.09%	0.011%
15	3.595	777	779	784	rVB6	1129	771	0.05%	0.007%
16	3.624	784	788	790	rBV5	1561	1127	0.08%	0.010%
17	3.765	830	832	835	rVB3	1484	760	0.05%	0.007%
18	3.785	835	838	839	rBV3	1241	628	0.04%	0.005%
19	3.817	844	848	849	rBV4	1097	770	0.05%	0.007%
20	3.901	864	874	900	rBV2	110273	314229	21.77%	2.729%
21	4.296	993	997	999	rVB4	1419	988	0.07%	0.009%
22	4.373	1007	1021	1048	rVB	225527	550736	38.15%	4.783%
23	4.611	1090	1095	1098	rBV6	1635	1416	0.10%	0.012%
24	4.740	1133	1135	1137	rBV2	1198	648	0.04%	0.006%
25	4.753	1137	1139	1143	rVV4	1227	889	0.06%	0.008%
26	4.830	1159	1163	1165	rBV4	1559	1146	0.08%	0.010%
27	4.878	1174	1178	1180	rBV5	1238	787	0.05%	0.007%
28	4.907	1183	1187	1189	rVV2	985	616	0.04%	0.005%
29	5.071	1218	1238	1266	rBV2	560507	1443593	100.00%	12.537%
30	5.392	1335	1338	1339	rBV3	1519	898	0.06%	0.008%
31	5.476	1362	1364	1369	rVB5	918	771	0.05%	0.007%
32	5.640	1401	1415	1434	rBV	449789	892807	61.85%	7.754%
33	5.807	1463	1467	1470	rBV5	1910	1729	0.12%	0.015%
34	5.936	1493	1507	1528	rBV	309150	608901	42.18%	5.288%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016502.D
 Acq On : 04 Jun 2020 12:08
 Operator : SY/MD
 Sample : L2869-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.093	1544	1556	1577	rVB	318014	634834	43.98%	5.513%
36	6.209	1588	1592	1593	rBV3	1337	895	0.06%	0.008%
37	6.315	1622	1625	1629	rBV7	1354	1394	0.10%	0.012%
38	6.453	1666	1668	1670	rBV2	1411	743	0.05%	0.006%
39	6.502	1682	1683	1687	rBV4	819	698	0.05%	0.006%
40	6.878	1793	1800	1802	rBV7	1522	1683	0.12%	0.015%
41	6.920	1811	1813	1815	rBV3	1265	749	0.05%	0.007%
42	7.006	1827	1840	1855	rBV	178095	321635	22.28%	2.793%
43	7.277	1922	1924	1928	rBV5	970	694	0.05%	0.006%
44	7.338	1931	1943	1959	rBV	662266	1137116	78.77%	9.875%
45	7.640	2027	2037	2054	rBV	128168	221153	15.32%	1.921%
46	7.788	2078	2083	2086	rBV5	1628	1666	0.12%	0.014%
47	8.109	2172	2183	2204	rBV	410898	725263	50.24%	6.298%
48	8.649	2349	2351	2355	rVB5	1268	803	0.06%	0.007%
49	8.756	2381	2384	2387	rBV5	1472	1045	0.07%	0.009%
50	8.875	2407	2421	2436	rBV	658627	1071861	74.25%	9.309%
51	9.293	2549	2551	2555	rBV3	1143	932	0.06%	0.008%
52	9.331	2561	2563	2566	rBV3	939	694	0.05%	0.006%
53	9.453	2596	2601	2605	rBV6	1219	1137	0.08%	0.010%
54	9.563	2633	2635	2638	rVB3	1399	626	0.04%	0.005%
55	9.630	2654	2656	2659	rVB3	1815	877	0.06%	0.008%
56	9.781	2701	2703	2706	rVV4	1086	710	0.05%	0.006%
57	9.804	2708	2710	2713	rVB2	1421	789	0.05%	0.007%
58	9.849	2720	2724	2726	rBV2	1041	652	0.05%	0.006%
59	10.135	2807	2813	2815	rBV6	1411	1305	0.09%	0.011%
60	10.238	2830	2845	2865	rBV	428378	681876	47.23%	5.922%
61	10.363	2883	2884	2888	rVB4	1434	744	0.05%	0.006%
62	10.418	2899	2901	2903	rVV3	1695	793	0.05%	0.007%
63	10.482	2918	2921	2925	rBV4	1562	1389	0.10%	0.012%
64	10.630	2963	2967	2969	rBV4	985	746	0.05%	0.006%
65	10.662	2973	2977	2982	rVB6	1005	1041	0.07%	0.009%
66	10.919	3055	3057	3060	rVB4	1510	859	0.06%	0.007%
67	11.096	3109	3112	3115	rBV5	1328	1202	0.08%	0.010%
68	11.183	3136	3139	3141	rBV3	1761	1133	0.08%	0.010%
69	11.270	3154	3166	3185	rBV	668902	1028498	71.25%	8.932%
70	11.408	3207	3209	3213	rVB5	1280	800	0.06%	0.007%
71	11.469	3223	3228	3230	rBV4	2097	1936	0.13%	0.017%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016502.D
 Acq On : 04 Jun 2020 12:08
 Operator : SY/MD
 Sample : L2869-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.534	3245	3248	3249	rBV3	1410	667	0.05%	0.006%
73	11.646	3271	3283	3300	rVV	677650	1056271	73.17%	9.173%
74	11.894	3358	3360	3364	rVB4	1424	866	0.06%	0.008%
75	12.215	3456	3460	3461	rBV3	1490	996	0.07%	0.009%
76	12.286	3479	3482	3488	rBV7	1153	1040	0.07%	0.009%
77	12.312	3488	3490	3494	rVB4	1073	698	0.05%	0.006%
78	12.354	3500	3503	3505	rBV2	1233	925	0.06%	0.008%
79	12.524	3553	3556	3560	rBV3	828	686	0.05%	0.006%
80	12.585	3572	3575	3577	rBV3	1392	738	0.05%	0.006%
81	12.614	3580	3584	3586	rBV4	1180	717	0.05%	0.006%
82	12.720	3613	3617	3619	rBV3	1964	1214	0.08%	0.011%
83	12.749	3623	3626	3628	rBV3	1229	832	0.06%	0.007%
84	12.903	3670	3674	3677	rBV5	1191	1114	0.08%	0.010%
85	13.064	3721	3724	3726	rVB3	1562	759	0.05%	0.007%
86	13.090	3726	3732	3735	rBV6	1375	1743	0.12%	0.015%
87	13.222	3771	3773	3775	rBV3	1776	914	0.06%	0.008%
88	13.373	3818	3820	3827	rBV7	1453	1703	0.12%	0.015%
89	13.595	3886	3889	3890	rBV3	1496	863	0.06%	0.007%
90	13.704	3920	3923	3926	rBV5	1288	871	0.06%	0.008%
91	13.762	3939	3941	3944	rBV3	1331	835	0.06%	0.007%
92	13.855	3966	3970	3975	rVV8	1890	1934	0.13%	0.017%
93	13.897	3981	3983	3986	rBV4	1370	1050	0.07%	0.009%
94	13.980	4008	4009	4013	rBV4	1003	786	0.05%	0.007%
95	14.228	4084	4086	4091	rVB4	1276	910	0.06%	0.008%
96	14.257	4093	4095	4098	rBV3	1443	896	0.06%	0.008%
97	14.579	4190	4195	4199	rBV9	1934	2121	0.15%	0.018%
98	14.607	4199	4204	4205	rBV4	1336	1180	0.08%	0.010%
99	14.646	4214	4216	4218	rBV4	1424	616	0.04%	0.005%
100	14.755	4246	4250	4252	rBV4	1509	1099	0.08%	0.010%


Sum of corrected areas: 11514853

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016502.D
Acq On : 04 Jun 2020 12:08
Operator : SY/MD
Sample : L2869-03DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

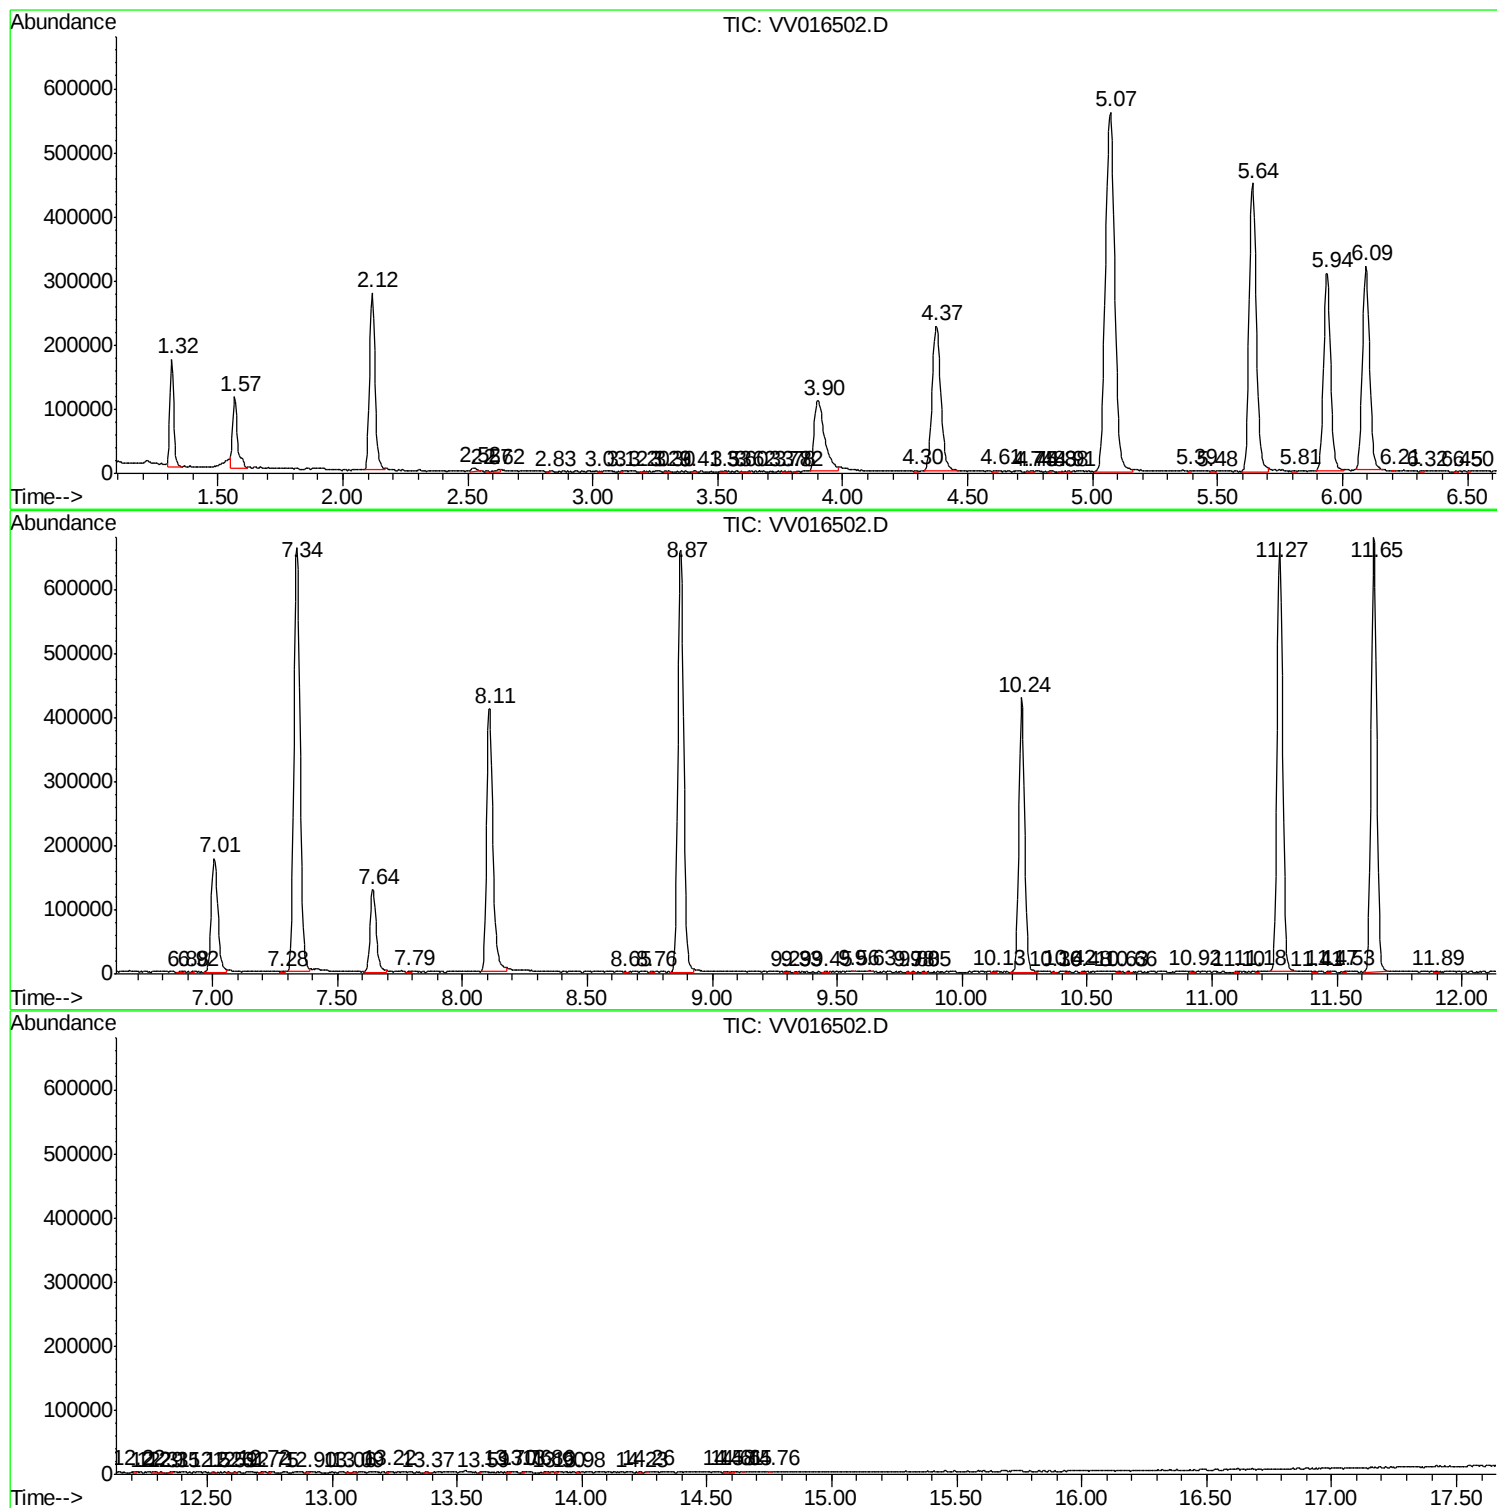

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016502.D
Acq On : 04 Jun 2020 12:08
Operator : SY/MD
Sample : L2869-03DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016502.D
Acq On : 04 Jun 2020 12:08
Operator : SY/MD
Sample : L2869-03DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc