

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016504.D
 Acq On : 04 Jun 2020 12:56
 Operator : SY/MD
 Sample : L2869-06DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	82	rVB	166006	172330	12.58%	1.534%
2	1.573	144	150	165	rVB	124550	143803	10.49%	1.280%
3	2.123	311	321	338	rBV	272825	405979	29.63%	3.614%
4	2.602	468	470	473	rBV4	1101	565	0.04%	0.005%
5	2.688	494	497	500	rVB5	1260	927	0.07%	0.008%
6	2.714	500	505	509	rBV7	1722	1962	0.14%	0.017%
7	2.978	585	587	592	rBV6	751	511	0.04%	0.005%
8	3.110	626	628	632	rVB5	1246	576	0.04%	0.005%
9	3.155	638	642	646	rVB6	1344	1196	0.09%	0.011%
10	3.267	675	677	680	rBV4	945	492	0.04%	0.004%
11	3.335	695	698	700	rBV4	1018	550	0.04%	0.005%
12	3.402	716	719	721	rBV3	831	564	0.04%	0.005%
13	3.598	778	780	784	rVB2	966	554	0.04%	0.005%
14	3.708	812	814	817	rBV3	875	560	0.04%	0.005%
15	3.785	835	838	842	rBV3	1076	845	0.06%	0.008%
16	3.823	847	850	853	rBV2	1107	778	0.06%	0.007%
17	3.897	863	873	899	rBV	109051	291472	21.27%	2.594%
18	4.376	1007	1022	1043	rBV	224153	537215	39.20%	4.782%
19	4.582	1084	1086	1087	rBV2	1070	513	0.04%	0.005%
20	4.605	1091	1093	1096	rBV4	1620	1241	0.09%	0.011%
21	4.627	1098	1100	1101	rBV2	1413	571	0.04%	0.005%
22	4.746	1133	1137	1139	rVV4	1086	638	0.05%	0.006%
23	4.817	1157	1159	1164	rBV4	1557	1321	0.10%	0.012%
24	5.003	1214	1217	1219	rBV4	1163	711	0.05%	0.006%
25	5.071	1222	1238	1259	rVV2	539459	1370348	100.00%	12.198%
26	5.640	1402	1415	1441	rBV	451655	905483	66.08%	8.060%
27	5.939	1494	1508	1527	rBV	347480	685447	50.02%	6.101%
28	6.093	1544	1556	1580	rVB	308282	624265	45.56%	5.557%
29	6.280	1612	1614	1616	rBV2	1296	681	0.05%	0.006%
30	6.373	1641	1643	1645	rBV3	1017	510	0.04%	0.005%
31	6.396	1647	1650	1654	rBV5	1969	1449	0.11%	0.013%
32	6.476	1671	1675	1677	rVB4	1100	734	0.05%	0.007%
33	6.550	1695	1698	1705	rVB7	1573	1370	0.10%	0.012%
34	6.614	1716	1718	1721	rVB3	1134	684	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016504.D
 Acq On : 04 Jun 2020 12:56
 Operator : SY/MD
 Sample : L2869-06DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.634	1721	1724	1728	rBV4	1899	2001	0.15%	0.018%
36	6.753	1759	1761	1766	rVB5	1294	885	0.06%	0.008%
37	6.775	1766	1768	1772	rBV3	1146	825	0.06%	0.007%
38	7.007	1830	1840	1862	rBV	167000	299578	21.86%	2.667%
39	7.283	1924	1926	1929	rBV3	1091	560	0.04%	0.005%
40	7.338	1931	1943	1963	rVV	632536	1088898	79.46%	9.693%
41	7.553	2007	2010	2012	rBV3	1852	815	0.06%	0.007%
42	7.643	2027	2038	2056	rBV	120307	204782	14.94%	1.823%
43	8.036	2158	2160	2162	rBV4	1299	809	0.06%	0.007%
44	8.106	2172	2182	2200	rBV	401791	663831	48.44%	5.909%
45	8.611	2335	2339	2342	rBV5	1452	1669	0.12%	0.015%
46	8.756	2382	2384	2389	rVB5	1801	1433	0.10%	0.013%
47	8.875	2408	2421	2440	rBV	676433	1088745	79.45%	9.691%
48	9.138	2501	2503	2505	rBV3	1715	1063	0.08%	0.009%
49	9.238	2533	2534	2537	rBV3	902	522	0.04%	0.005%
50	9.405	2584	2586	2589	rBV3	1273	801	0.06%	0.007%
51	9.450	2598	2600	2602	rBV3	1388	678	0.05%	0.006%
52	9.524	2619	2623	2626	rBV5	1051	905	0.07%	0.008%
53	9.572	2636	2638	2643	rBV4	1259	999	0.07%	0.009%
54	9.627	2651	2655	2658	rBV5	1646	1649	0.12%	0.015%
55	9.675	2667	2670	2675	rBV6	1170	1245	0.09%	0.011%
56	9.778	2699	2702	2705	rVB4	1268	839	0.06%	0.007%
57	9.949	2752	2755	2757	rVV4	1285	799	0.06%	0.007%
58	9.981	2763	2765	2766	rBV2	1017	551	0.04%	0.005%
59	10.145	2814	2816	2819	rVB3	1260	684	0.05%	0.006%
60	10.238	2833	2845	2864	rVV	414739	649421	47.39%	5.781%
61	10.363	2882	2884	2888	rBV4	978	538	0.04%	0.005%
62	10.556	2941	2944	2945	rBV	1383	687	0.05%	0.006%
63	10.605	2957	2959	2969	rVB9	2098	2470	0.18%	0.022%
64	10.685	2981	2984	2986	rBV3	1008	559	0.04%	0.005%
65	10.704	2988	2990	2993	rVB3	1842	881	0.06%	0.008%
66	10.720	2993	2995	2997	rBV2	894	538	0.04%	0.005%
67	10.778	3011	3013	3015	rVB3	1262	533	0.04%	0.005%
68	10.791	3015	3017	3020	rBV2	1309	791	0.06%	0.007%
69	10.839	3030	3032	3037	rVB5	1714	1343	0.10%	0.012%
70	10.887	3041	3047	3053	rBV10	1792	2522	0.18%	0.022%
71	10.926	3057	3059	3061	rBV3	1225	684	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016504.D
 Acq On : 04 Jun 2020 12:56
 Operator : SY/MD
 Sample : L2869-06DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.013	3083	3086	3088	rVB4	1319	646	0.05%	0.006%
73	11.048	3095	3097	3099	rVB3	1230	535	0.04%	0.005%
74	11.270	3154	3166	3184	rBV	671030	1023538	74.69%	9.111%
75	11.531	3244	3247	3250	rBV4	1412	1118	0.08%	0.010%
76	11.646	3272	3283	3302	rBV	640694	1002058	73.12%	8.920%
77	11.788	3324	3327	3328	rBV2	1000	504	0.04%	0.004%
78	12.026	3396	3401	3405	rBV7	1483	1860	0.14%	0.017%
79	12.084	3414	3419	3421	rBV5	1558	1283	0.09%	0.011%
80	12.145	3435	3438	3442	rBV5	1269	1017	0.07%	0.009%
81	12.257	3468	3473	3474	rBV6	1656	1378	0.10%	0.012%
82	12.328	3493	3495	3499	rVV4	1398	872	0.06%	0.008%
83	12.460	3532	3536	3540	rBV6	1468	909	0.07%	0.008%
84	12.566	3565	3569	3571	rBV4	1054	751	0.05%	0.007%
85	12.617	3583	3585	3589	rVB4	1473	814	0.06%	0.007%
86	12.852	3653	3658	3661	rBV5	1115	863	0.06%	0.008%
87	13.039	3714	3716	3719	rBV3	1369	867	0.06%	0.008%
88	13.084	3728	3730	3736	rVB6	1448	1052	0.08%	0.009%
89	13.260	3783	3785	3786	rBV2	954	492	0.04%	0.004%
90	13.360	3813	3816	3819	rVB4	1453	874	0.06%	0.008%
91	13.386	3819	3824	3827	rBV5	1294	1124	0.08%	0.010%
92	13.457	3844	3846	3848	rBV3	1181	723	0.05%	0.006%
93	13.505	3858	3861	3862	rBV2	1051	594	0.04%	0.005%
94	13.781	3945	3947	3950	rVB3	1655	851	0.06%	0.008%
95	13.842	3963	3966	3968	rBV4	1703	973	0.07%	0.009%
96	14.019	4018	4021	4024	rBV3	1405	994	0.07%	0.009%
97	14.190	4069	4074	4077	rVB5	1731	1412	0.10%	0.013%
98	14.498	4166	4170	4171	rBV3	1045	694	0.05%	0.006%
99	14.720	4235	4239	4241	rBV4	1032	1010	0.07%	0.009%
100	15.370	4439	4441	4446	rBV5	1819	1209	0.09%	0.011%


Sum of corrected areas: 11234393

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016504.D
Acq On : 04 Jun 2020 12:56
Operator : SY/MD
Sample : L2869-06DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

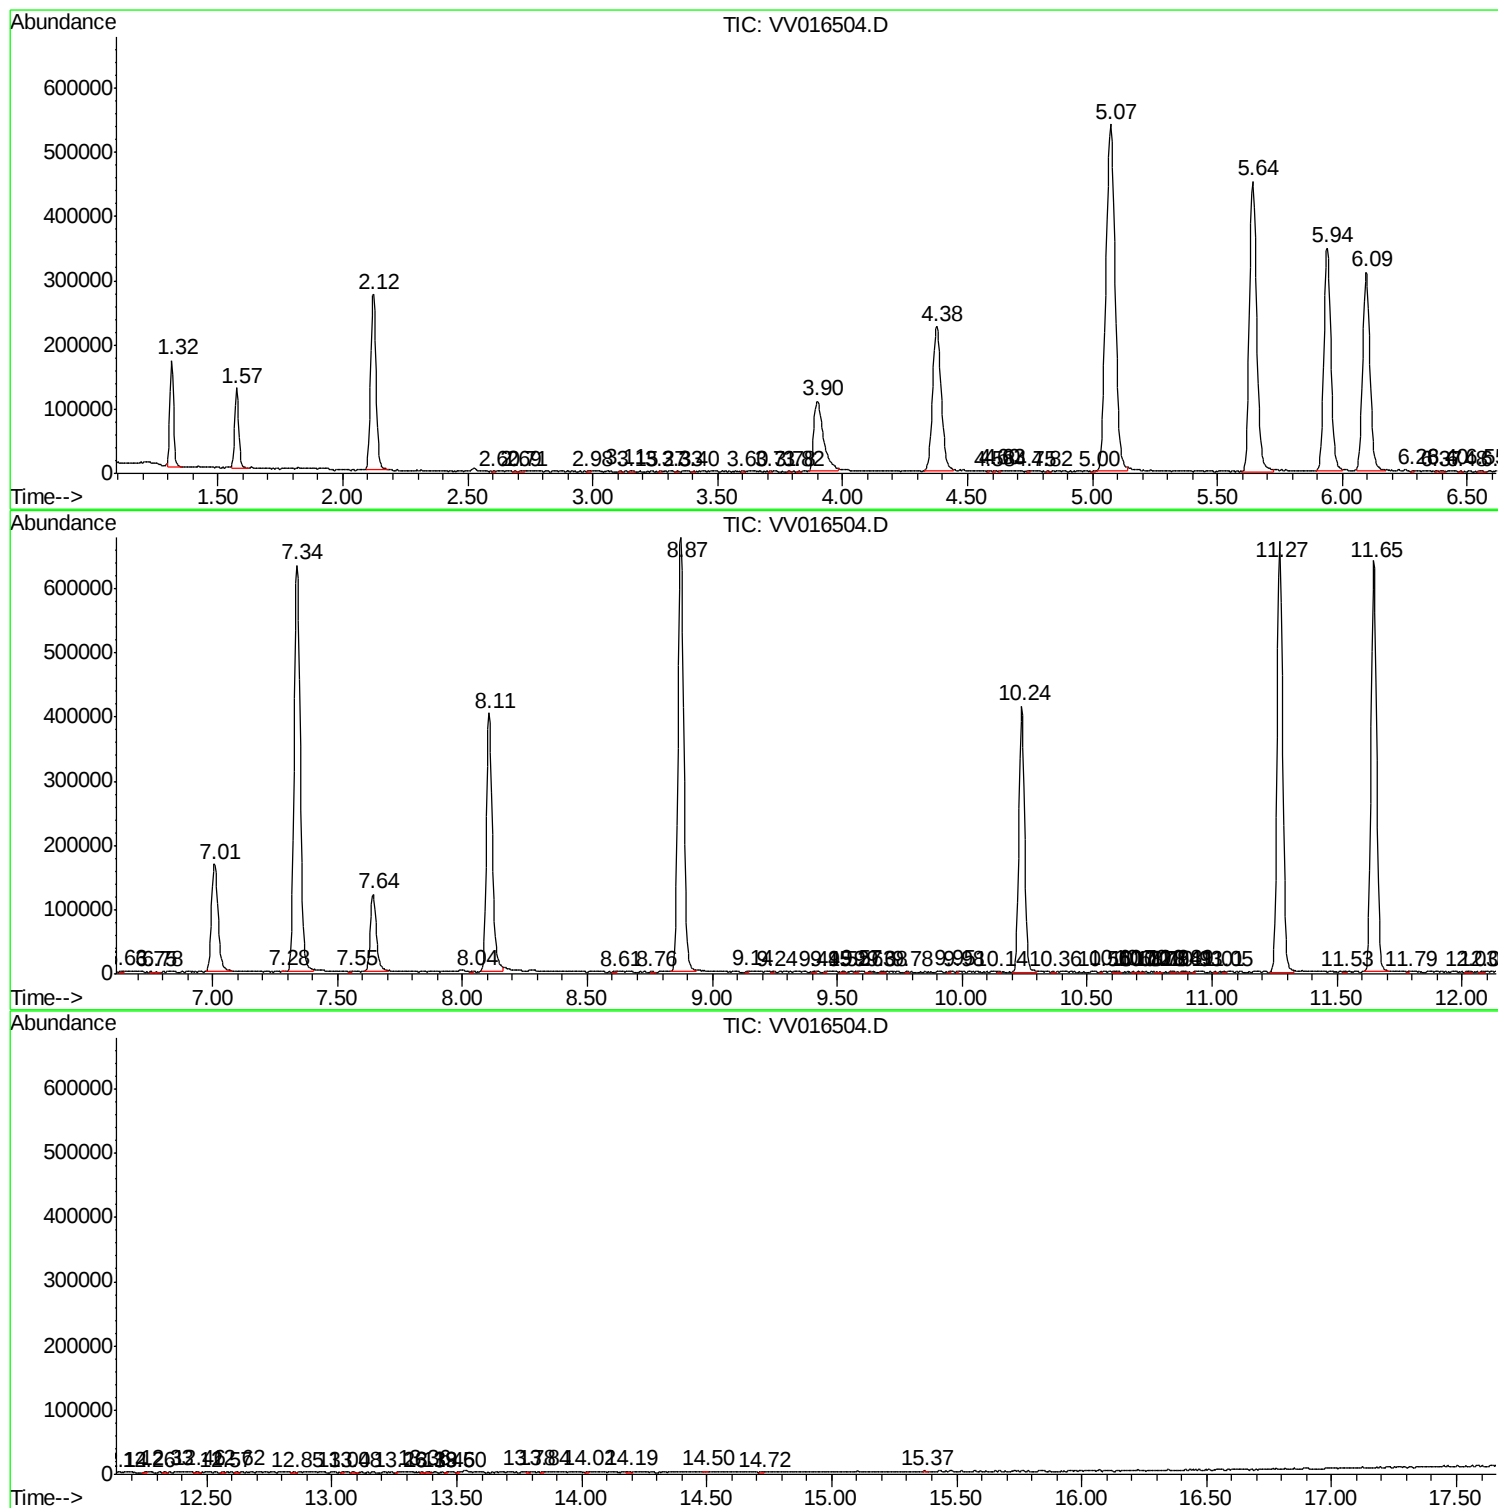

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016504.D
Acq On : 04 Jun 2020 12:56
Operator : SY/MD
Sample : L2869-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060420\
Data File : VV016504.D
Acq On : 04 Jun 2020 12:56
Operator : SY/MD
Sample : L2869-06DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
DBFG6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc