

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016506.D
 Acq On : 04 Jun 2020 13:43
 Operator : SY/MD
 Sample : L2869-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	173406	171093	12.42%	1.599%
2	1.569	143	149	163	rVB	125434	145474	10.56%	1.359%
3	2.119	311	320	338	rVB	277088	406620	29.51%	3.799%
4	2.479	430	432	435	rBV3	1251	710	0.05%	0.007%
5	2.637	477	481	483	rBV4	1031	967	0.07%	0.009%
6	2.759	516	519	520	rBV3	1138	674	0.05%	0.006%
7	2.817	535	537	540	rBV3	1667	1132	0.08%	0.011%
8	2.997	589	593	595	rVV4	982	592	0.04%	0.006%
9	3.325	693	695	697	rBV3	1141	597	0.04%	0.006%
10	3.338	697	699	701	rVB3	1513	620	0.04%	0.006%
11	3.370	706	709	710	rBV3	1385	745	0.05%	0.007%
12	3.508	749	752	755	rBV4	1235	789	0.06%	0.007%
13	3.547	761	764	766	rBV4	1095	745	0.05%	0.007%
14	3.740	822	824	827	rVB3	926	608	0.04%	0.006%
15	3.814	845	847	850	rVB4	1863	934	0.07%	0.009%
16	3.897	862	873	898	rBV	112243	291549	21.16%	2.724%
17	4.106	936	938	941	rBV4	1303	641	0.05%	0.006%
18	4.306	997	1000	1002	rBV5	1136	980	0.07%	0.009%
19	4.376	1007	1022	1044	rVV2	222424	538020	39.04%	5.027%
20	4.521	1064	1067	1070	rBV4	1560	1161	0.08%	0.011%
21	4.736	1130	1134	1136	rBV3	1160	959	0.07%	0.009%
22	4.830	1159	1163	1167	rBV5	1046	836	0.06%	0.008%
23	5.071	1221	1238	1260	rBV2	542371	1378103	100.00%	12.876%
24	5.322	1313	1316	1319	rBV4	1671	1264	0.09%	0.012%
25	5.453	1355	1357	1360	rBV4	1456	1026	0.07%	0.010%
26	5.640	1403	1415	1435	rBV	445323	879060	63.79%	8.213%
27	5.871	1485	1487	1489	rBV2	1146	756	0.05%	0.007%
28	5.932	1496	1506	1516	rBV2	7564	17447	1.27%	0.163%
29	6.035	1534	1538	1540	rBV4	1682	1135	0.08%	0.011%
30	6.093	1540	1556	1581	rVV	311933	641308	46.54%	5.992%
31	6.350	1630	1636	1638	rVB7	1324	1143	0.08%	0.011%
32	6.453	1666	1668	1673	rVB5	1055	625	0.05%	0.006%
33	6.627	1718	1722	1725	rBV5	1738	1852	0.13%	0.017%
34	6.685	1735	1740	1741	rBV4	1995	1407	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016506.D
 Acq On : 04 Jun 2020 13:43
 Operator : SY/MD
 Sample : L2869-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.817	1778	1781	1788	rBV8	1292	1562	0.11%	0.015%
36	6.858	1792	1794	1798	rBV3	878	660	0.05%	0.006%
37	6.923	1806	1814	1815	rBV7	1354	1516	0.11%	0.014%
38	7.006	1829	1840	1860	rBV	168400	303249	22.00%	2.833%
39	7.338	1927	1943	1966	rBV	639321	1099447	79.78%	10.272%
40	7.643	2029	2038	2056	rVB	119145	198990	14.44%	1.859%
41	8.106	2169	2182	2212	rBV	421256	702621	50.98%	6.565%
42	8.582	2327	2330	2333	rVV4	1403	1279	0.09%	0.012%
43	8.704	2365	2368	2371	rBV4	946	847	0.06%	0.008%
44	8.743	2378	2380	2385	rBV5	1651	1467	0.11%	0.014%
45	8.784	2389	2393	2395	rBV4	1654	1288	0.09%	0.012%
46	8.874	2409	2421	2444	rBV	680012	1079957	78.37%	10.090%
47	9.100	2487	2491	2494	rBV4	1793	1475	0.11%	0.014%
48	9.193	2518	2520	2522	rBV3	1363	572	0.04%	0.005%
49	9.328	2560	2562	2565	rVB3	1744	1125	0.08%	0.011%
50	9.354	2565	2570	2573	rBV7	1817	1481	0.11%	0.014%
51	9.373	2573	2576	2580	rVB4	1099	903	0.07%	0.008%
52	9.463	2601	2604	2607	rBV5	1395	1030	0.07%	0.010%
53	9.498	2613	2615	2619	rVB5	1042	689	0.05%	0.006%
54	9.569	2634	2637	2639	rBV4	1427	1060	0.08%	0.010%
55	9.608	2645	2649	2653	rBV6	1600	1700	0.12%	0.016%
56	9.659	2660	2665	2667	rBV6	941	781	0.06%	0.007%
57	9.707	2677	2680	2682	rBV3	1171	680	0.05%	0.006%
58	9.839	2720	2721	2726	rVB5	1166	837	0.06%	0.008%
59	10.042	2780	2784	2786	rBV4	1688	1080	0.08%	0.010%
60	10.109	2800	2805	2809	rBV6	2123	2414	0.18%	0.023%
61	10.157	2815	2820	2822	rBV6	1236	1070	0.08%	0.010%
62	10.238	2833	2845	2860	rBV	427554	665768	48.31%	6.220%
63	10.392	2889	2893	2894	rBV3	1163	881	0.06%	0.008%
64	10.450	2908	2911	2912	rBV3	1173	734	0.05%	0.007%
65	10.582	2946	2952	2954	rBV5	1300	1463	0.11%	0.014%
66	10.772	3007	3011	3013	rBV4	1326	897	0.07%	0.008%
67	10.862	3037	3039	3042	rVV3	2080	1146	0.08%	0.011%
68	10.878	3042	3044	3048	rVB2	1452	779	0.06%	0.007%
69	11.090	3108	3110	3112	rBV3	1383	641	0.05%	0.006%
70	11.103	3112	3114	3118	rVB4	1798	1033	0.07%	0.010%
71	11.270	3155	3166	3185	rBV	686801	1055084	76.56%	9.858%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016506.D
 Acq On : 04 Jun 2020 13:43
 Operator : SY/MD
 Sample : L2869-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.453	3220	3223	3225	rBV3	1035	626	0.05%	0.006%
73	11.485	3231	3233	3241	rVB9	931	887	0.06%	0.008%
74	11.646	3271	3283	3306	rBV	664454	1046016	75.90%	9.773%
75	11.829	3337	3340	3342	rBV3	1216	863	0.06%	0.008%
76	11.865	3349	3351	3354	rBV3	1262	794	0.06%	0.007%
77	11.932	3370	3372	3376	rVB4	1220	751	0.05%	0.007%
78	11.993	3389	3391	3394	rBV3	830	636	0.05%	0.006%
79	12.099	3421	3424	3426	rBV4	898	644	0.05%	0.006%
80	12.238	3464	3467	3469	rVB4	1692	796	0.06%	0.007%
81	12.263	3469	3475	3477	rBV6	1314	1146	0.08%	0.011%
82	12.305	3485	3488	3493	rBV6	1615	1290	0.09%	0.012%
83	12.669	3594	3601	3606	rBV8	2235	2673	0.19%	0.025%
84	12.707	3610	3613	3617	rBV5	1526	1412	0.10%	0.013%
85	12.839	3651	3654	3658	rBV3	1238	796	0.06%	0.007%
86	12.865	3658	3662	3664	rBV3	1362	1138	0.08%	0.011%
87	13.106	3733	3737	3738	rBV4	726	601	0.04%	0.006%
88	13.128	3740	3744	3746	rBV4	1423	1020	0.07%	0.010%
89	13.270	3783	3788	3790	rBV3	1839	1677	0.12%	0.016%
90	13.328	3803	3806	3809	rBV5	1206	866	0.06%	0.008%
91	13.447	3839	3843	3844	rBV3	1463	906	0.07%	0.008%
92	13.604	3890	3892	3896	rBV5	1328	875	0.06%	0.008%
93	13.717	3923	3927	3928	rBV4	1570	889	0.06%	0.008%
94	13.759	3935	3940	3941	rBV5	1474	1019	0.07%	0.010%
95	13.845	3962	3967	3968	rBV5	1287	1048	0.08%	0.010%
96	13.926	3990	3992	3996	rVB4	1475	604	0.04%	0.006%
97	14.022	4018	4022	4024	rBV4	1349	761	0.06%	0.007%
98	14.032	4024	4025	4028	rBV3	971	618	0.04%	0.006%
99	14.151	4060	4062	4064	rBV3	1307	752	0.05%	0.007%
100	14.434	4147	4150	4154	rBV3	1150	975	0.07%	0.009%


Sum of corrected areas: 10702857

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016506.D
Acq On : 04 Jun 2020 13:43
Operator : SY/MD
Sample : L2869-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

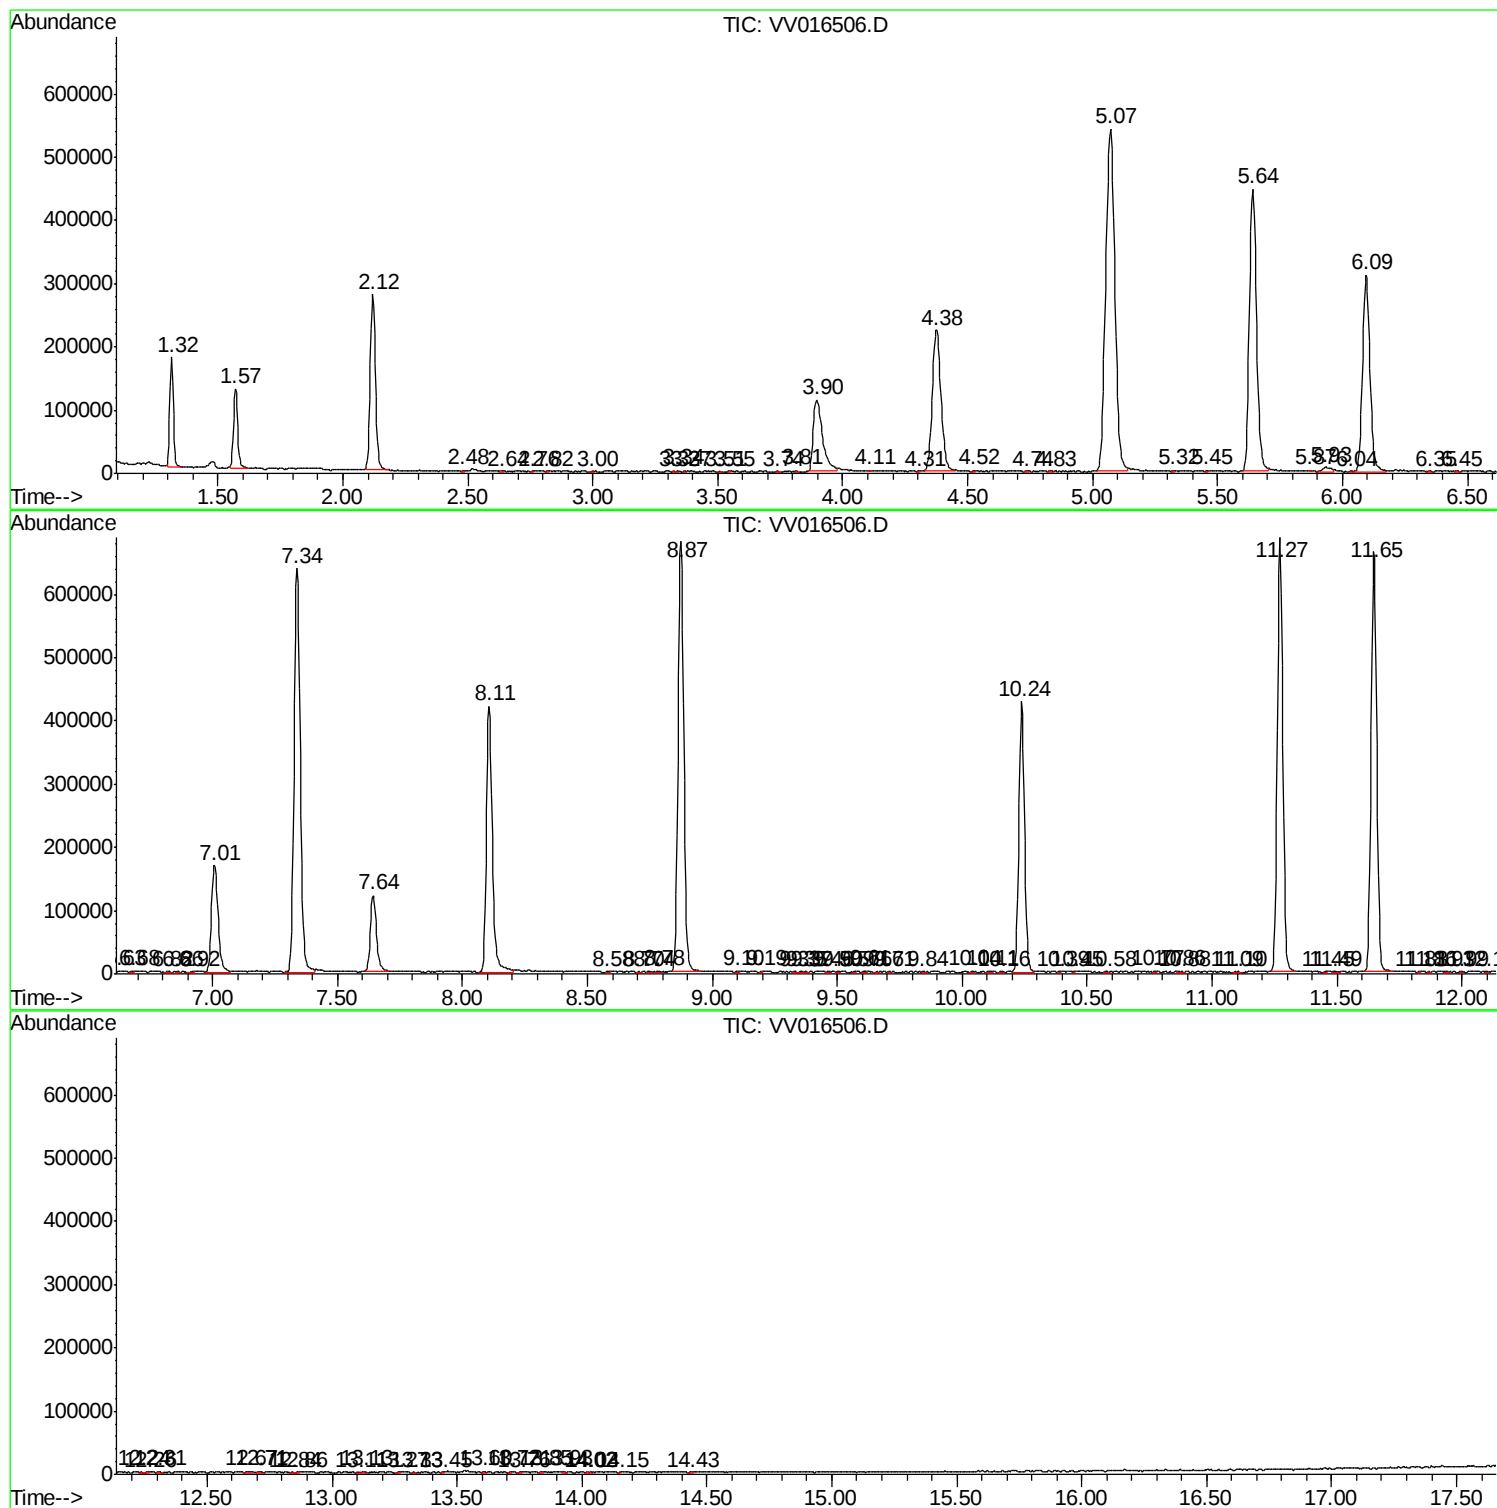

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016506.D
Acq On : 04 Jun 2020 13:43
Operator : SY/MD
Sample : L2869-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016506.D
Acq On : 04 Jun 2020 13:43
Operator : SY/MD
Sample : L2869-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc