

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016507.D
 Acq On : 04 Jun 2020 14:07
 Operator : SY/MD
 Sample : L2849-11DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB2	235697	249109	18.98%	2.423%
2	1.573	143	150	161	rVB	118655	139278	10.61%	1.355%
3	2.119	311	320	331	rBV	262700	380012	28.96%	3.696%
4	2.727	505	509	513	rVB5	1511	1049	0.08%	0.010%
5	2.749	513	516	519	rBV3	1434	1027	0.08%	0.010%
6	2.775	522	524	527	rBV4	1331	873	0.07%	0.008%
7	2.891	557	560	563	rBV4	1386	1140	0.09%	0.011%
8	2.942	575	576	579	rBV3	1198	599	0.05%	0.006%
9	3.020	596	600	602	rBV3	1132	1138	0.09%	0.011%
10	3.071	614	616	617	rBV	889	449	0.03%	0.004%
11	3.106	625	627	630	rBV4	898	429	0.03%	0.004%
12	3.142	633	638	639	rBV5	1440	922	0.07%	0.009%
13	3.296	683	686	688	rBV4	1665	934	0.07%	0.009%
14	3.328	694	696	698	rVB4	944	362	0.03%	0.004%
15	3.344	698	701	704	rBV4	1612	1301	0.10%	0.013%
16	3.396	715	717	719	rBV3	825	542	0.04%	0.005%
17	3.557	765	767	771	rVB5	1047	463	0.04%	0.005%
18	3.685	805	807	809	rBV2	1555	819	0.06%	0.008%
19	3.698	809	811	815	rVB3	1505	835	0.06%	0.008%
20	3.717	815	817	819	rBV2	584	323	0.02%	0.003%
21	3.749	824	827	829	rBV4	1260	807	0.06%	0.008%
22	3.817	845	848	851	rBV5	1406	1150	0.09%	0.011%
23	3.897	862	873	877	rBV	109840	206629	15.75%	2.010%
24	4.238	977	979	981	rVB2	1327	546	0.04%	0.005%
25	4.309	995	1001	1003	rBV6	1822	1917	0.15%	0.019%
26	4.373	1007	1021	1044	rVV2	207860	518585	39.52%	5.044%
27	4.560	1077	1079	1080	rBV2	1327	468	0.04%	0.005%
28	4.804	1153	1155	1157	rBV3	888	572	0.04%	0.006%
29	5.000	1213	1216	1217	rBV3	1072	558	0.04%	0.005%
30	5.071	1222	1238	1262	rVV2	515046	1312168	100.00%	12.763%
31	5.640	1403	1415	1438	rBV	444981	870717	66.36%	8.469%
32	5.891	1489	1493	1495	rBV5	1231	1164	0.09%	0.011%
33	6.093	1542	1556	1581	rBV	297079	606798	46.24%	5.902%
34	6.364	1637	1640	1642	rBV4	1018	778	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016507.D
 Acq On : 04 Jun 2020 14:07
 Operator : SY/MD
 Sample : L2849-11DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.425	1656	1659	1660	rBV3	1247	640	0.05%	0.006%
36	6.486	1673	1678	1683	rBV8	1272	1508	0.11%	0.015%
37	6.801	1774	1776	1781	rVB6	1367	880	0.07%	0.009%
38	6.827	1781	1784	1787	rBV4	1675	1114	0.08%	0.011%
39	6.891	1799	1804	1806	rBV5	1203	1040	0.08%	0.010%
40	6.904	1806	1808	1809	rBV	917	376	0.03%	0.004%
41	7.007	1829	1840	1857	rBV	162297	290301	22.12%	2.824%
42	7.338	1931	1943	1964	rBV	618860	1046109	79.72%	10.175%
43	7.643	2029	2038	2054	rBV2	114565	188882	14.39%	1.837%
44	7.727	2062	2064	2069	rBV4	1650	1767	0.13%	0.017%
45	7.897	2115	2117	2120	rVB3	1128	396	0.03%	0.004%
46	7.916	2121	2123	2128	rVV5	1463	1208	0.09%	0.012%
47	8.048	2160	2164	2169	rBV8	1946	2041	0.16%	0.020%
48	8.106	2172	2182	2209	rVV	402763	667932	50.90%	6.497%
49	8.585	2328	2331	2332	rBV3	1105	513	0.04%	0.005%
50	8.595	2332	2334	2336	rVV3	1191	523	0.04%	0.005%
51	8.875	2408	2421	2442	rBV	663051	1072821	81.76%	10.435%
52	9.148	2503	2506	2507	rBV4	2164	1268	0.10%	0.012%
53	9.228	2529	2531	2532	rBV2	720	315	0.02%	0.003%
54	9.277	2542	2546	2547	rBV4	1290	901	0.07%	0.009%
55	9.296	2550	2552	2553	rBV2	1183	466	0.04%	0.005%
56	9.498	2613	2615	2617	rBV3	813	421	0.03%	0.004%
57	9.727	2678	2686	2688	rBV7	2187	3009	0.23%	0.029%
58	9.797	2705	2708	2710	rBV4	940	641	0.05%	0.006%
59	9.852	2723	2725	2726	rBV	726	294	0.02%	0.003%
60	9.923	2745	2747	2749	rBV3	1109	611	0.05%	0.006%
61	10.003	2768	2772	2774	rBV3	1315	853	0.07%	0.008%
62	10.019	2774	2777	2778	rBV2	1385	719	0.05%	0.007%
63	10.125	2808	2810	2812	rBV3	1307	676	0.05%	0.007%
64	10.164	2820	2822	2823	rBV2	1108	508	0.04%	0.005%
65	10.238	2834	2845	2859	rBV	410623	633010	48.24%	6.157%
66	10.331	2870	2874	2876	rBV4	1650	1169	0.09%	0.011%
67	10.534	2934	2937	2939	rBV4	900	535	0.04%	0.005%
68	10.733	2997	2999	3001	rBV2	1008	431	0.03%	0.004%
69	10.785	3013	3015	3018	rBV3	1323	776	0.06%	0.008%
70	10.797	3018	3019	3022	rVB3	1242	599	0.05%	0.006%
71	11.183	3135	3139	3140	rBV3	1141	758	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016507.D
 Acq On : 04 Jun 2020 14:07
 Operator : SY/MD
 Sample : L2849-11DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.222	3149	3151	3153	rBV3	1025	549	0.04%	0.005%
73	11.270	3155	3166	3182	rVV	675761	1033189	78.74%	10.050%
74	11.473	3227	3229	3233	rBV5	1336	836	0.06%	0.008%
75	11.646	3272	3283	3298	rBV	638090	993500	75.71%	9.664%
76	11.929	3368	3371	3375	rBV5	2101	1504	0.11%	0.015%
77	11.948	3375	3377	3380	rVV3	1505	723	0.06%	0.007%
78	11.968	3380	3383	3387	rVB4	1825	1318	0.10%	0.013%
79	12.051	3407	3409	3412	rBV3	1444	653	0.05%	0.006%
80	12.096	3420	3423	3424	rBV3	1292	646	0.05%	0.006%
81	12.170	3443	3446	3449	rBV4	1402	1161	0.09%	0.011%
82	12.202	3454	3456	3459	rBV3	1113	547	0.04%	0.005%
83	12.257	3469	3473	3475	rBV5	2095	1661	0.13%	0.016%
84	12.312	3488	3490	3491	rBV2	1149	375	0.03%	0.004%
85	12.511	3550	3552	3554	rBV3	1027	434	0.03%	0.004%
86	12.791	3633	3639	3640	rBV4	1558	1635	0.12%	0.016%
87	12.958	3687	3691	3693	rBV3	1740	1391	0.11%	0.014%
88	13.042	3714	3717	3722	rBV8	1228	1237	0.09%	0.012%
89	13.235	3773	3777	3780	rVB4	1012	711	0.05%	0.007%
90	13.363	3815	3817	3821	rBV4	1136	934	0.07%	0.009%
91	13.624	3896	3898	3900	rBV3	990	488	0.04%	0.005%
92	13.755	3936	3939	3942	rVB3	1782	1085	0.08%	0.011%
93	13.772	3942	3944	3947	rBV3	1776	1200	0.09%	0.012%
94	13.884	3977	3979	3981	rBV2	995	312	0.02%	0.003%
95	14.109	4047	4049	4054	rVB5	1190	825	0.06%	0.008%
96	14.173	4067	4069	4071	rVB2	1150	456	0.03%	0.004%
97	14.337	4118	4120	4121	rBV2	1324	582	0.04%	0.006%
98	14.582	4194	4196	4198	rBV3	1479	825	0.06%	0.008%
99	14.984	4317	4321	4322	rBV4	1154	990	0.08%	0.010%
100	15.183	4381	4383	4387	rBV4	1576	701	0.05%	0.007%


Sum of corrected areas: 10280940

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016507.D
Acq On : 04 Jun 2020 14:07
Operator : SY/MD
Sample : L2849-11DL 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

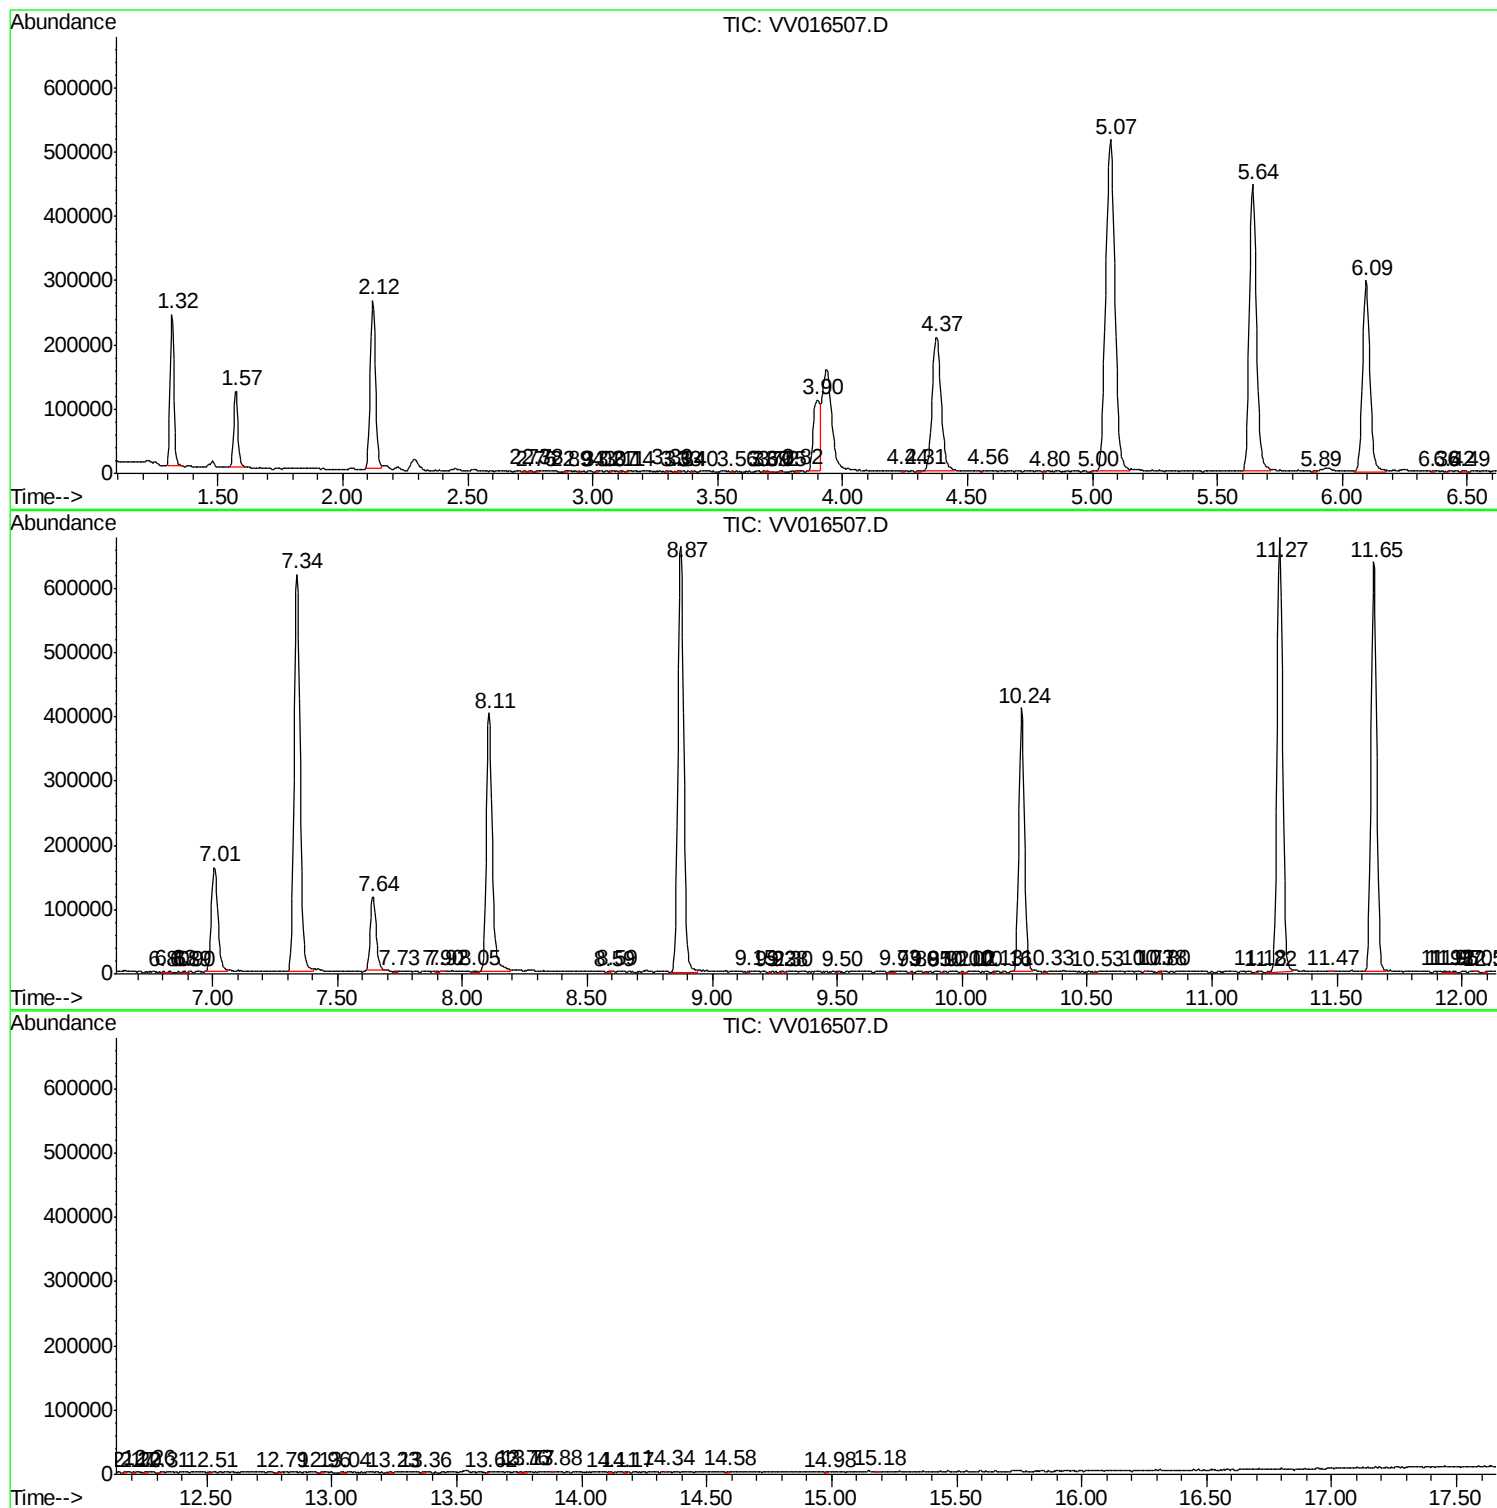

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016507.D
Acq On : 04 Jun 2020 14:07
Operator : SY/MD
Sample : L2849-11DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016507.D
Acq On : 04 Jun 2020 14:07
Operator : SY/MD
Sample : L2849-11DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR6DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc