

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016508.D
 Acq On : 04 Jun 2020 14:31
 Operator : SY/MD
 Sample : L2849-01DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETP6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	83	rVB2	349033	370624	28.28%	3.344%
2	2.113	309	318	334	rVB	260040	381975	29.15%	3.446%
3	2.434	413	418	421	rBV6	1416	1230	0.09%	0.011%
4	2.518	438	444	450	rBV8	3506	4621	0.35%	0.042%
5	2.769	515	522	527	rBV9	2578	4001	0.31%	0.036%
6	2.878	553	556	559	rBV4	1223	983	0.08%	0.009%
7	2.975	583	586	589	rBV4	1274	743	0.06%	0.007%
8	2.994	589	592	596	rBV5	961	889	0.07%	0.008%
9	3.123	629	632	635	rBV4	783	569	0.04%	0.005%
10	3.203	649	657	660	rBV9	1788	1717	0.13%	0.015%
11	3.238	664	668	673	rBV5	1726	2108	0.16%	0.019%
12	3.373	708	710	714	rBV4	1869	1363	0.10%	0.012%
13	3.515	751	754	757	rBV5	1059	683	0.05%	0.006%
14	3.631	787	790	792	rBV4	922	614	0.05%	0.006%
15	3.660	797	799	802	rVB3	1221	581	0.04%	0.005%
16	3.679	802	805	806	rBV3	1176	655	0.05%	0.006%
17	3.775	830	835	838	rBV5	1651	1503	0.11%	0.014%
18	3.814	842	847	850	rBV6	1516	1175	0.09%	0.011%
19	3.930	863	883	914	rBV2	319090	1023611	78.11%	9.236%
20	4.270	985	989	993	rBV7	1142	1199	0.09%	0.011%
21	4.309	997	1001	1004	rBV4	1608	1517	0.12%	0.014%
22	4.373	1006	1021	1039	rVV	206988	508480	38.80%	4.588%
23	4.685	1114	1118	1119	rBV3	1362	920	0.07%	0.008%
24	4.759	1137	1141	1145	rVB5	1923	1829	0.14%	0.017%
25	4.791	1145	1151	1152	rBV5	1248	1404	0.11%	0.013%
26	4.894	1181	1183	1185	rBV3	1264	687	0.05%	0.006%
27	4.923	1188	1192	1194	rVB4	1030	738	0.06%	0.007%
28	4.949	1198	1200	1204	rVB3	1412	933	0.07%	0.008%
29	4.978	1204	1209	1212	rVB7	1054	1044	0.08%	0.009%
30	4.994	1212	1214	1216	rBV3	1460	758	0.06%	0.007%
31	5.068	1220	1237	1258	rBV2	522261	1310438	100.00%	11.824%
32	5.537	1379	1383	1386	rBV5	1295	1118	0.09%	0.010%
33	5.640	1401	1415	1437	rBV	424191	857080	65.40%	7.733%
34	5.885	1487	1491	1492	rBV3	1146	607	0.05%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016508.D
 Acq On : 04 Jun 2020 14:31
 Operator : SY/MD
 Sample : L2849-01DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETPP6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	5.926	1497	1504	1507	rBV6	3371	4810	0.37%	0.043%
36	6.093	1542	1556	1588	rBV	289494	591098	45.11%	5.333%
37	6.396	1648	1650	1654	rVB6	1756	1055	0.08%	0.010%
38	6.521	1686	1689	1695	rVB6	1048	939	0.07%	0.008%
39	6.550	1695	1698	1702	rBV5	1456	1413	0.11%	0.013%
40	6.624	1717	1721	1723	rBV4	1460	979	0.07%	0.009%
41	6.640	1723	1726	1728	rBV2	2607	1874	0.14%	0.017%
42	6.833	1782	1786	1789	rVB6	1478	1049	0.08%	0.009%
43	7.007	1828	1840	1864	rBV	165488	297645	22.71%	2.686%
44	7.338	1931	1943	1963	rBV	599621	1027007	78.37%	9.267%
45	7.640	2027	2037	2050	rBV	116966	197270	15.05%	1.780%
46	7.965	2134	2138	2139	rBV3	1074	588	0.04%	0.005%
47	8.106	2172	2182	2205	rBV	395423	674819	51.50%	6.089%
48	8.428	2278	2282	2283	rBV4	1608	1017	0.08%	0.009%
49	8.569	2324	2326	2334	rBV6	1160	1047	0.08%	0.009%
50	8.872	2408	2420	2441	rVV	643729	1049566	80.09%	9.470%
51	9.068	2478	2481	2485	rBV5	1665	1367	0.10%	0.012%
52	9.113	2492	2495	2496	rBV2	1671	811	0.06%	0.007%
53	9.293	2548	2551	2553	rBV3	1124	635	0.05%	0.006%
54	9.363	2569	2573	2575	rBV2	1374	1007	0.08%	0.009%
55	9.634	2654	2657	2659	rBV3	1279	856	0.07%	0.008%
56	9.672	2667	2669	2672	rBV3	1225	859	0.07%	0.008%
57	9.743	2688	2691	2692	rBV3	1087	663	0.05%	0.006%
58	9.778	2699	2702	2706	rBV4	1682	1490	0.11%	0.013%
59	9.798	2706	2708	2711	rBV4	1330	949	0.07%	0.009%
60	9.852	2718	2725	2730	rVB9	1432	1843	0.14%	0.017%
61	9.891	2734	2737	2740	rBV4	1120	809	0.06%	0.007%
62	9.952	2752	2756	2757	rBV4	1215	948	0.07%	0.009%
63	10.035	2781	2782	2788	rVB4	990	747	0.06%	0.007%
64	10.084	2791	2797	2800	rBV8	1763	1572	0.12%	0.014%
65	10.180	2825	2827	2830	rBV4	943	611	0.05%	0.006%
66	10.238	2832	2845	2862	rBV	406781	643834	49.13%	5.809%
67	10.392	2890	2893	2894	rBV2	1178	722	0.06%	0.007%
68	10.453	2910	2912	2915	rBV4	1344	1024	0.08%	0.009%
69	10.595	2953	2956	2958	rBV4	699	548	0.04%	0.005%
70	10.679	2978	2982	2983	rBV3	1003	597	0.05%	0.005%
71	10.707	2990	2991	2994	rBV2	937	603	0.05%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016508.D
 Acq On : 04 Jun 2020 14:31
 Operator : SY/MD
 Sample : L2849-01DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETP6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.746	3001	3003	3006	rBV3	1806	1096	0.08%	0.010%
73	10.859	3034	3038	3039	rBV3	1093	793	0.06%	0.007%
74	11.180	3133	3138	3139	rBV4	1146	969	0.07%	0.009%
75	11.270	3153	3166	3185	rBV	676285	1031623	78.72%	9.308%
76	11.534	3244	3248	3250	rBV5	1518	1186	0.09%	0.011%
77	11.646	3271	3283	3303	rBV	650054	1019675	77.81%	9.200%
78	11.839	3339	3343	3347	rBV6	1817	1231	0.09%	0.011%
79	11.900	3359	3362	3367	rBV5	1790	1771	0.14%	0.016%
80	11.942	3372	3375	3378	rBV3	829	588	0.04%	0.005%
81	11.990	3388	3390	3391	rBV3	1345	592	0.05%	0.005%
82	12.013	3395	3397	3399	rVB3	1241	582	0.04%	0.005%
83	12.103	3421	3425	3428	rBV6	1546	1646	0.13%	0.015%
84	12.273	3474	3478	3480	rBV4	1209	927	0.07%	0.008%
85	12.402	3514	3518	3519	rBV3	1442	939	0.07%	0.008%
86	12.463	3534	3537	3540	rBV5	1023	867	0.07%	0.008%
87	12.540	3558	3561	3563	rVB4	1389	726	0.06%	0.007%
88	12.563	3563	3568	3570	rBV5	1374	1173	0.09%	0.011%
89	12.656	3592	3597	3598	rBV5	928	835	0.06%	0.008%
90	12.691	3606	3608	3611	rVB4	1626	799	0.06%	0.007%
91	12.727	3616	3619	3622	rBV5	1245	1038	0.08%	0.009%
92	12.842	3649	3655	3659	rBV7	1302	1493	0.11%	0.013%
93	12.903	3670	3674	3679	rBV6	1740	1611	0.12%	0.015%
94	13.399	3825	3828	3830	rBV3	1331	856	0.07%	0.008%
95	13.656	3905	3908	3909	rBV3	1010	567	0.04%	0.005%
96	13.862	3968	3972	3973	rBV3	1113	888	0.07%	0.008%
97	14.058	4028	4033	4036	rBV5	1582	1729	0.13%	0.016%
98	14.161	4061	4065	4068	rBV4	1552	1425	0.11%	0.013%
99	14.328	4113	4117	4121	rBV7	1311	1502	0.11%	0.014%
100	15.080	4349	4351	4353	rBV2	1543	789	0.06%	0.007%


Sum of corrected areas: 11082984

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016508.D
Acq On : 04 Jun 2020 14:31
Operator : SY/MD
Sample : L2849-01DL 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTP6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

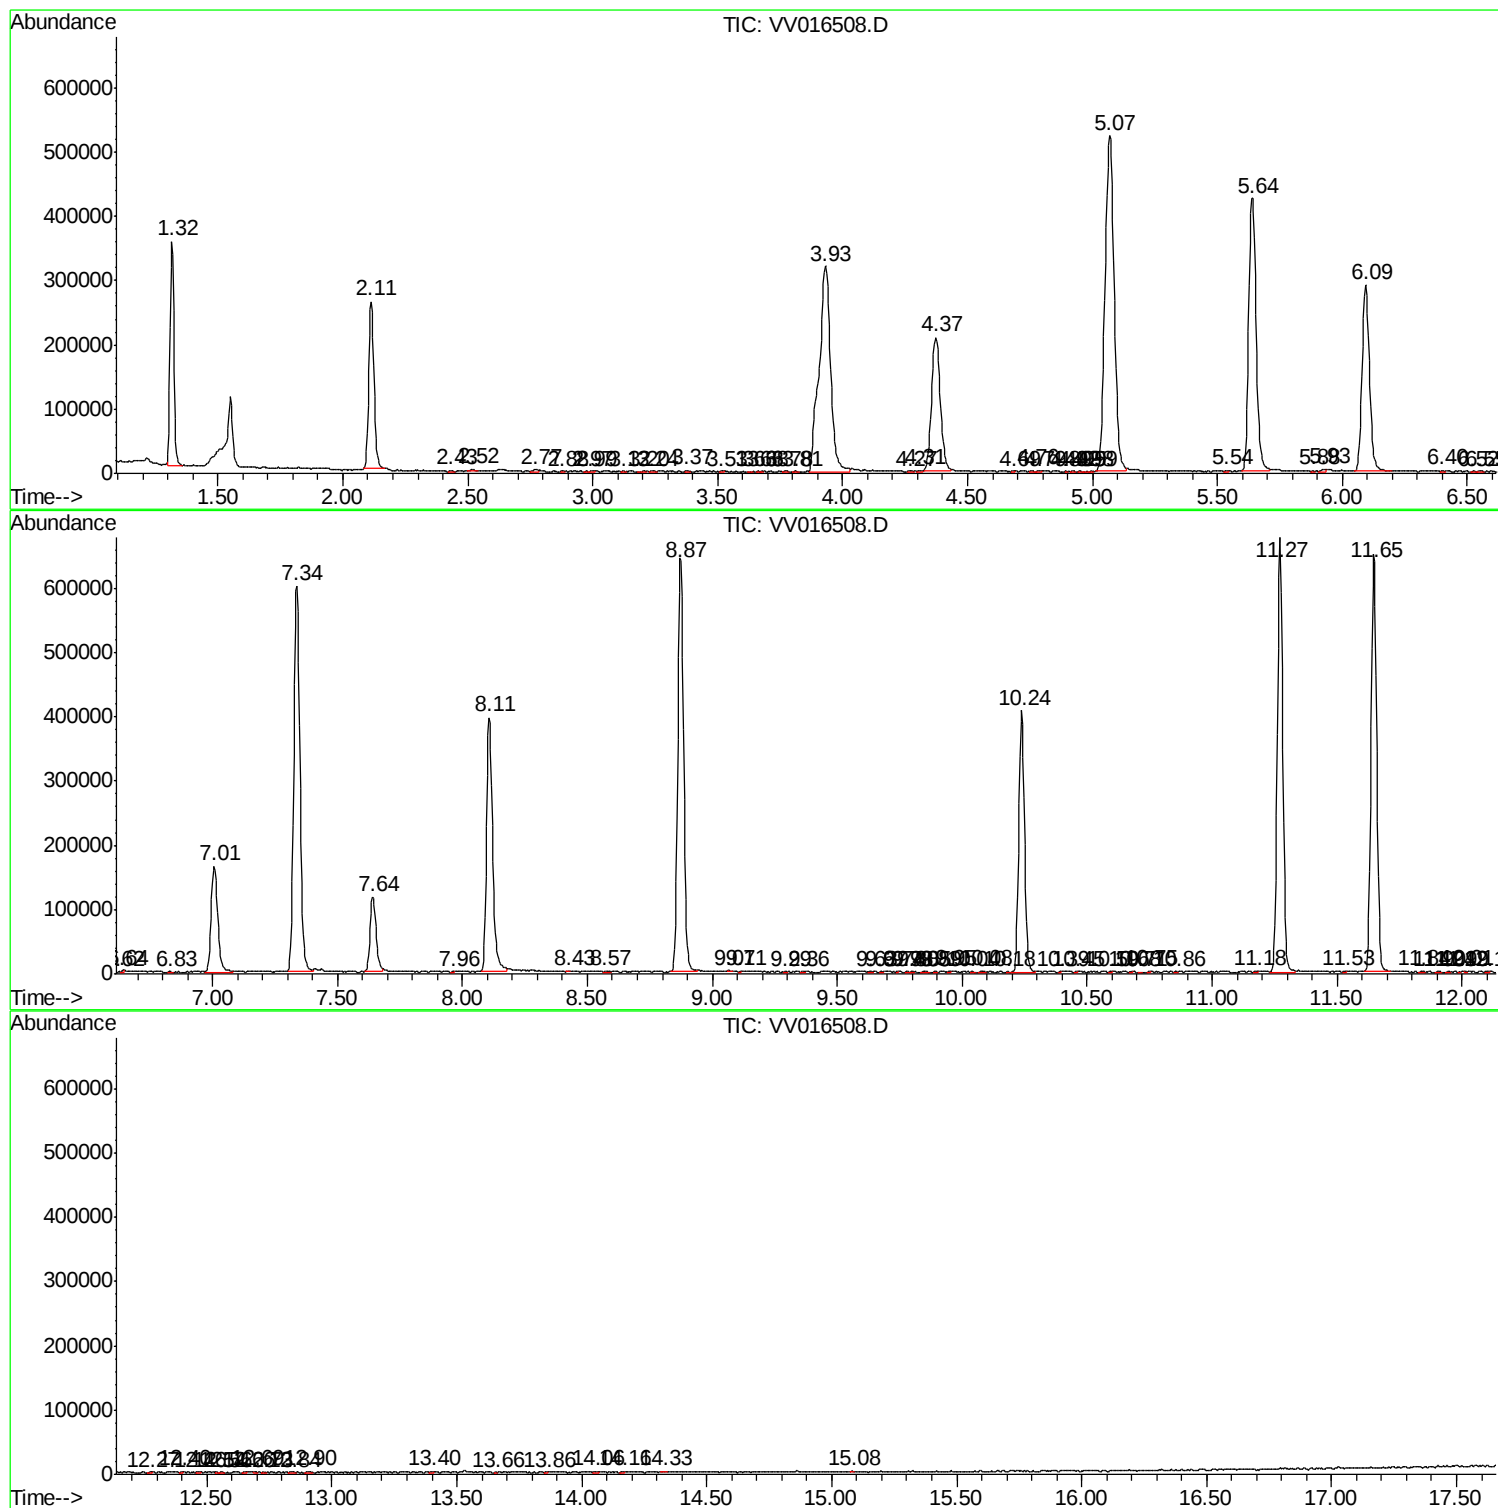

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016508.D
Acq On : 04 Jun 2020 14:31
Operator : SY/MD
Sample : L2849-01DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTP6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016508.D
Acq On : 04 Jun 2020 14:31
Operator : SY/MD
Sample : L2849-01DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTP6DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc