

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016509.D
 Acq On : 04 Jun 2020 14:55
 Operator : SY/MD
 Sample : L2849-02DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETP7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB2	333144	359569	25.67%	3.077%
2	1.563	141	147	157	rVB	121166	141426	10.10%	1.210%
3	2.116	310	319	339	rVB	275646	408716	29.17%	3.498%
4	2.502	435	439	440	rBV3	1784	1053	0.08%	0.009%
5	2.582	460	464	466	rBV5	1034	802	0.06%	0.007%
6	2.901	561	563	567	rVB5	1010	767	0.05%	0.007%
7	2.949	575	578	579	rBV4	1368	841	0.06%	0.007%
8	3.023	599	601	604	rVB3	1279	611	0.04%	0.005%
9	3.055	609	611	615	rVV5	927	727	0.05%	0.006%
10	3.139	633	637	638	rBV4	1877	1312	0.09%	0.011%
11	3.258	670	674	676	rBV5	1165	1076	0.08%	0.009%
12	3.338	696	699	701	rBV3	1506	964	0.07%	0.008%
13	3.351	701	703	706	rBV4	1353	770	0.05%	0.007%
14	3.563	767	769	773	rVB5	1282	877	0.06%	0.008%
15	3.589	773	777	783	rBV8	1897	1749	0.12%	0.015%
16	3.778	832	836	837	rBV3	1421	989	0.07%	0.008%
17	3.820	847	849	855	rVB6	957	915	0.07%	0.008%
18	3.936	862	885	910	rBV2	309616	1020106	72.82%	8.730%
19	4.264	985	987	989	rBV3	1064	653	0.05%	0.006%
20	4.373	1005	1021	1041	rBV	229935	552767	39.46%	4.731%
21	4.576	1080	1084	1086	rBV4	1708	1635	0.12%	0.014%
22	4.746	1135	1137	1140	rBV3	1243	645	0.05%	0.006%
23	4.849	1167	1169	1175	rVB7	1503	1063	0.08%	0.009%
24	4.894	1181	1183	1186	rBV4	1418	694	0.05%	0.006%
25	4.907	1186	1187	1191	rVV4	1147	688	0.05%	0.006%
26	4.926	1191	1193	1197	rVV4	1185	994	0.07%	0.009%
27	5.071	1218	1238	1267	rBV2	546052	1400932	100.00%	11.990%
28	5.386	1333	1336	1337	rBV3	1290	729	0.05%	0.006%
29	5.640	1402	1415	1440	rBV	452398	897143	64.04%	7.678%
30	5.910	1496	1499	1500	rBV3	1780	967	0.07%	0.008%
31	6.032	1534	1537	1540	rBV4	1166	864	0.06%	0.007%
32	6.093	1542	1556	1578	rVV	314879	632556	45.15%	5.414%
33	6.370	1639	1642	1644	rBV3	1659	991	0.07%	0.008%
34	6.627	1721	1722	1726	rBV3	1135	798	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016509.D
 Acq On : 04 Jun 2020 14:55
 Operator : SY/MD
 Sample : L2849-02DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETP7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.765	1761	1765	1767	rBV4	1625	1197	0.09%	0.010%
36	6.807	1777	1778	1783	rVV4	1203	968	0.07%	0.008%
37	7.007	1829	1840	1858	rBV	171528	305296	21.79%	2.613%
38	7.245	1912	1914	1919	rBV5	1200	1033	0.07%	0.009%
39	7.338	1929	1943	1965	rBV	646950	1103797	78.79%	9.447%
40	7.643	2028	2038	2053	rBV	121440	205960	14.70%	1.763%
41	7.855	2102	2104	2108	rVB5	1955	966	0.07%	0.008%
42	8.106	2172	2182	2203	rBV	413982	685020	48.90%	5.863%
43	8.425	2279	2281	2283	rBV2	1458	637	0.05%	0.005%
44	8.489	2299	2301	2302	rBV2	1334	738	0.05%	0.006%
45	8.752	2381	2383	2387	rBV5	1286	773	0.06%	0.007%
46	8.875	2409	2421	2438	rBV	681206	1097996	78.38%	9.397%
47	9.161	2506	2510	2511	rBV3	1187	767	0.05%	0.007%
48	9.289	2547	2550	2552	rBV3	1557	1124	0.08%	0.010%
49	9.434	2591	2595	2598	rBV4	1455	1035	0.07%	0.009%
50	9.450	2598	2600	2604	rVB3	1321	946	0.07%	0.008%
51	9.470	2604	2606	2608	rBV2	1041	694	0.05%	0.006%
52	9.560	2630	2634	2638	rBV7	2285	2117	0.15%	0.018%
53	9.640	2657	2659	2663	rVV4	1495	923	0.07%	0.008%
54	9.691	2673	2675	2677	rVB3	1513	623	0.04%	0.005%
55	9.704	2677	2679	2682	rBV3	962	652	0.05%	0.006%
56	9.749	2688	2693	2694	rBV4	804	662	0.05%	0.006%
57	10.170	2820	2824	2827	rBV4	1226	1102	0.08%	0.009%
58	10.238	2831	2845	2862	rBV	435354	671169	47.91%	5.744%
59	10.370	2883	2886	2891	rVB5	2042	1637	0.12%	0.014%
60	10.396	2891	2894	2898	rVB4	1535	1002	0.07%	0.009%
61	10.556	2941	2944	2948	rBV5	1312	1200	0.09%	0.010%
62	10.650	2969	2973	2975	rVB5	1140	668	0.05%	0.006%
63	10.807	3017	3022	3023	rBV5	2463	1641	0.12%	0.014%
64	10.836	3028	3031	3032	rVV3	1350	607	0.04%	0.005%
65	10.865	3036	3040	3044	rBV8	1715	1651	0.12%	0.014%
66	10.984	3075	3077	3080	rBV3	1070	729	0.05%	0.006%
67	11.051	3094	3098	3100	rBV5	1130	925	0.07%	0.008%
68	11.132	3120	3123	3127	rVB5	1378	1132	0.08%	0.010%
69	11.270	3152	3166	3185	rBV	696586	1060961	75.73%	9.080%
70	11.543	3248	3251	3259	rBV8	1788	1883	0.13%	0.016%
71	11.646	3271	3283	3304	rBV	681195	1056261	75.40%	9.040%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016509.D
 Acq On : 04 Jun 2020 14:55
 Operator : SY/MD
 Sample : L2849-02DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTP7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.775	3321	3323	3324	rBV2	1761	614	0.04%	0.005%
73	11.852	3345	3347	3352	rVB5	1400	1133	0.08%	0.010%
74	11.878	3352	3355	3358	rBV5	1180	926	0.07%	0.008%
75	11.990	3387	3390	3394	rBV5	1068	795	0.06%	0.007%
76	12.093	3419	3422	3423	rBV3	1163	595	0.04%	0.005%
77	12.238	3465	3467	3473	rBV6	1388	1569	0.11%	0.013%
78	12.334	3495	3497	3501	rVB4	1324	741	0.05%	0.006%
79	12.360	3501	3505	3506	rBV3	1191	920	0.07%	0.008%
80	12.453	3531	3534	3539	rBV6	1636	1444	0.10%	0.012%
81	12.604	3579	3581	3584	rVV4	1201	636	0.05%	0.005%
82	12.730	3616	3620	3621	rBV3	865	682	0.05%	0.006%
83	12.952	3688	3689	3692	rBV2	1057	645	0.05%	0.006%
84	12.993	3698	3702	3704	rBV3	1499	1331	0.10%	0.011%
85	13.051	3718	3720	3724	rBV4	1515	1301	0.09%	0.011%
86	13.129	3740	3744	3747	rBV5	1484	1124	0.08%	0.010%
87	13.154	3749	3752	3754	rBV3	1437	829	0.06%	0.007%
88	13.241	3777	3779	3784	rVB5	1420	1170	0.08%	0.010%
89	13.289	3790	3794	3797	rBV5	1428	1154	0.08%	0.010%
90	13.325	3802	3805	3808	rBV3	1404	980	0.07%	0.008%
91	13.395	3818	3827	3830	rBV7	2596	3958	0.28%	0.034%
92	13.463	3844	3848	3849	rBV4	1408	912	0.07%	0.008%
93	13.768	3941	3943	3946	rBV4	1202	822	0.06%	0.007%
94	13.826	3958	3961	3963	rBV3	1149	658	0.05%	0.006%
95	14.045	4026	4029	4032	rBV4	1117	929	0.07%	0.008%
96	14.431	4147	4149	4152	rBV4	1062	702	0.05%	0.006%
97	15.106	4356	4359	4362	rBV3	1579	855	0.06%	0.007%
98	15.135	4366	4368	4372	rBV4	1435	930	0.07%	0.008%
99	15.405	4450	4452	4454	rBV3	1326	684	0.05%	0.006%
100	15.945	4618	4620	4624	rBV4	2109	1625	0.12%	0.014%


Sum of corrected areas: 11684545

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016509.D
Acq On : 04 Jun 2020 14:55
Operator : SY/MD
Sample : L2849-02DL 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTP7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

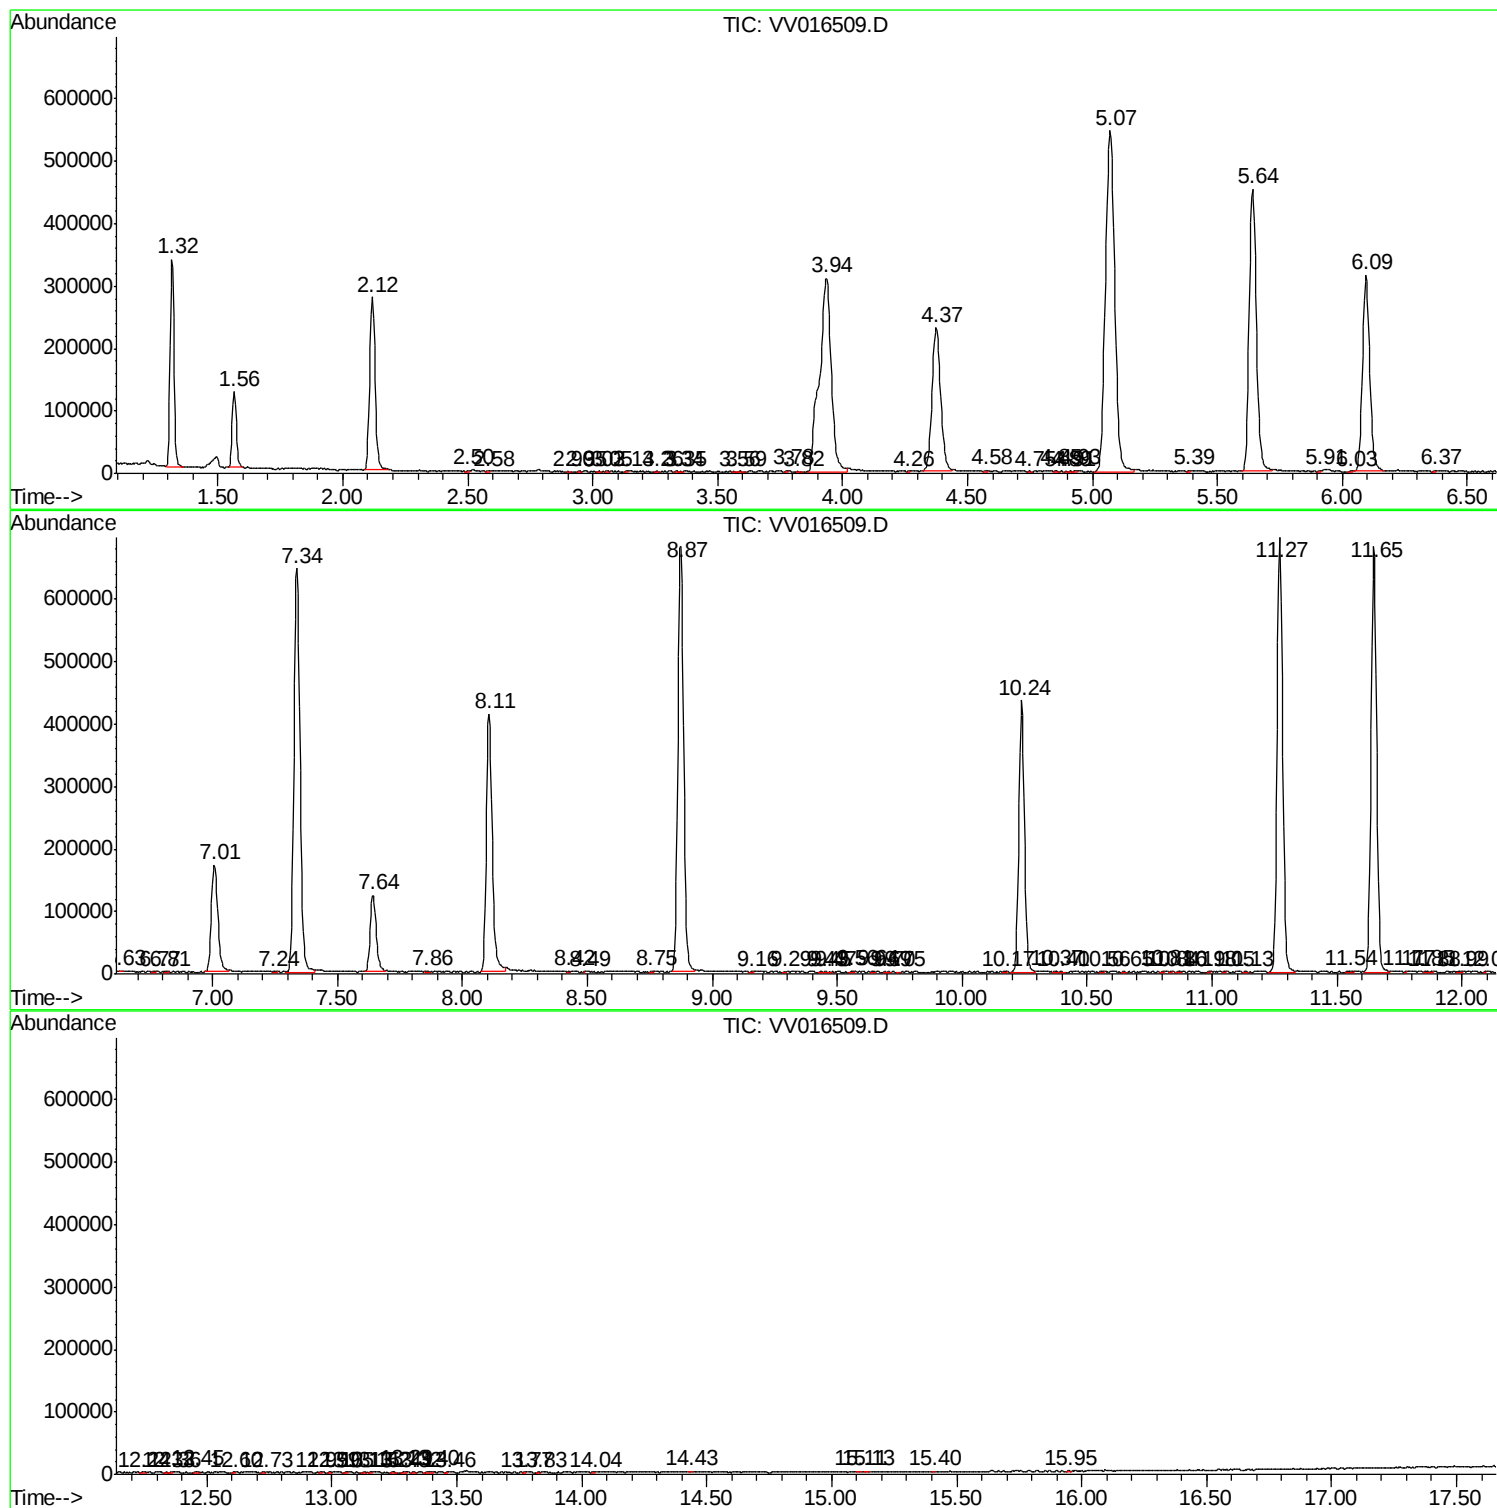

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016509.D
Acq On : 04 Jun 2020 14:55
Operator : SY/MD
Sample : L2849-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTP7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016509.D
Acq On : 04 Jun 2020 14:55
Operator : SY/MD
Sample : L2849-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTP7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc