

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016510.D
 Acq On : 04 Jun 2020 15:18
 Operator : SY/MD
 Sample : L2849-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTQ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	82	rVB2	184424	189670	14.25%	1.857%
2	1.570	142	149	166	rVB	116482	140518	10.56%	1.376%
3	2.119	311	320	334	rBV	269184	385675	28.98%	3.777%
4	2.515	439	443	444	rBV4	1610	1009	0.08%	0.010%
5	2.663	487	489	493	rVB5	1325	717	0.05%	0.007%
6	2.772	518	523	524	rBV5	1433	1122	0.08%	0.011%
7	2.930	569	572	575	rBV5	1360	760	0.06%	0.007%
8	2.949	575	578	582	rBV5	1274	1111	0.08%	0.011%
9	3.074	614	617	620	rBV2	1320	839	0.06%	0.008%
10	3.296	684	686	687	rBV	1092	494	0.04%	0.005%
11	3.370	703	709	712	rBV5	1211	1391	0.10%	0.014%
12	3.586	774	776	781	rVB5	1134	732	0.06%	0.007%
13	3.766	828	832	835	rBV4	979	953	0.07%	0.009%
14	3.827	848	851	853	rVV3	1269	707	0.05%	0.007%
15	3.897	862	873	901	rBV	105054	286020	21.49%	2.801%
16	4.174	957	959	962	rBV4	1415	1005	0.08%	0.010%
17	4.377	1008	1022	1041	rBV	211902	508953	38.25%	4.984%
18	4.531	1067	1070	1073	rBV5	1413	927	0.07%	0.009%
19	4.669	1110	1113	1114	rBV3	1370	698	0.05%	0.007%
20	4.743	1134	1136	1139	rBV2	851	551	0.04%	0.005%
21	4.766	1141	1143	1149	rVV6	1525	1349	0.10%	0.013%
22	4.820	1158	1160	1162	rBV3	852	541	0.04%	0.005%
23	4.852	1165	1170	1172	rBV5	1624	1157	0.09%	0.011%
24	4.885	1176	1180	1181	rBV3	1659	789	0.06%	0.008%
25	4.930	1189	1194	1195	rVB4	940	727	0.05%	0.007%
26	4.958	1195	1203	1207	rBV7	2095	2686	0.20%	0.026%
27	5.071	1218	1238	1262	rBV2	521168	1330741	100.00%	13.031%
28	5.357	1325	1327	1328	rBV2	1292	560	0.04%	0.005%
29	5.640	1402	1415	1445	rVV	425975	848074	63.73%	8.304%
30	5.778	1456	1458	1461	rBV3	1477	832	0.06%	0.008%
31	5.920	1498	1502	1503	rBV4	3383	2279	0.17%	0.022%
32	6.093	1540	1556	1578	rBV	302169	610605	45.88%	5.979%
33	6.373	1638	1643	1644	rBV5	1539	1388	0.10%	0.014%
34	6.483	1674	1677	1680	rBV5	1169	938	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016510.D
 Acq On : 04 Jun 2020 15:18
 Operator : SY/MD
 Sample : L2849-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTQ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.553	1697	1699	1702	rVB4	1271	565	0.04%	0.006%
36	6.785	1766	1771	1772	rBV4	1324	1024	0.08%	0.010%
37	6.929	1812	1816	1818	rBV3	1378	880	0.07%	0.009%
38	7.007	1830	1840	1856	rBV	160347	281200	21.13%	2.754%
39	7.254	1913	1917	1919	rBV4	1148	1048	0.08%	0.010%
40	7.338	1932	1943	1965	rBV	602991	1040032	78.15%	10.184%
41	7.643	2025	2038	2054	rBV	114883	201112	15.11%	1.969%
42	8.106	2172	2182	2209	rBV	396328	668923	50.27%	6.550%
43	8.875	2409	2421	2437	rBV	645116	1031265	77.50%	10.098%
44	9.026	2466	2468	2472	rBV5	1515	976	0.07%	0.010%
45	9.126	2497	2499	2502	rBV4	1438	669	0.05%	0.007%
46	9.151	2504	2507	2508	rBV3	1560	688	0.05%	0.007%
47	9.428	2586	2593	2595	rBV8	1505	1774	0.13%	0.017%
48	9.505	2614	2617	2619	rBV3	1107	786	0.06%	0.008%
49	9.572	2634	2638	2642	rBV7	1064	988	0.07%	0.010%
50	9.627	2653	2655	2656	rBV2	1305	511	0.04%	0.005%
51	9.675	2668	2670	2674	rVB4	1129	602	0.05%	0.006%
52	9.823	2713	2716	2718	rBV2	1215	885	0.07%	0.009%
53	10.039	2781	2783	2787	rVV6	1748	941	0.07%	0.009%
54	10.170	2822	2824	2831	rVB7	1291	983	0.07%	0.010%
55	10.238	2831	2845	2861	rBV	411436	639820	48.08%	6.265%
56	10.396	2892	2894	2897	rBV4	1825	1388	0.10%	0.014%
57	10.453	2909	2912	2913	rBV3	897	561	0.04%	0.005%
58	10.521	2931	2933	2936	rBV3	1097	691	0.05%	0.007%
59	10.550	2936	2942	2945	rBV4	1665	1517	0.11%	0.015%
60	10.675	2976	2981	2986	rVB9	1884	1942	0.15%	0.019%
61	10.717	2989	2994	2995	rBV4	833	575	0.04%	0.006%
62	10.791	3015	3017	3019	rBV3	1830	819	0.06%	0.008%
63	10.910	3052	3054	3056	rBV4	1105	511	0.04%	0.005%
64	11.010	3083	3085	3088	rVV4	727	549	0.04%	0.005%
65	11.077	3102	3106	3110	rBV6	1713	1530	0.11%	0.015%
66	11.177	3132	3137	3140	rBV6	1925	1885	0.14%	0.018%
67	11.270	3154	3166	3184	rBV	640643	982730	73.85%	9.623%
68	11.434	3216	3217	3219	rBV2	1466	656	0.05%	0.006%
69	11.479	3229	3231	3234	rVB3	1936	932	0.07%	0.009%
70	11.502	3234	3238	3241	rBV5	1678	1584	0.12%	0.016%
71	11.646	3272	3283	3300	rBV	633656	985430	74.05%	9.649%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016510.D
 Acq On : 04 Jun 2020 15:18
 Operator : SY/MD
 Sample : L2849-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTQ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.910	3361	3365	3367	rBV4	1160	909	0.07%	0.009%
73	11.955	3377	3379	3381	rBV3	1294	682	0.05%	0.007%
74	12.000	3392	3393	3397	rBV4	1132	600	0.05%	0.006%
75	12.019	3397	3399	3402	rVB4	1406	750	0.06%	0.007%
76	12.164	3440	3444	3446	rBV3	1678	1481	0.11%	0.015%
77	12.180	3447	3449	3455	rVV6	1559	1095	0.08%	0.011%
78	12.222	3459	3462	3466	rVB5	1747	1193	0.09%	0.012%
79	12.502	3547	3549	3552	rVB3	1584	824	0.06%	0.008%
80	12.521	3552	3555	3558	rBV3	1342	1061	0.08%	0.010%
81	12.543	3559	3562	3567	rVB5	1228	1180	0.09%	0.012%
82	12.572	3567	3571	3572	rBV3	1314	805	0.06%	0.008%
83	12.656	3594	3597	3601	rBV7	1612	1256	0.09%	0.012%
84	12.765	3628	3631	3633	rBV3	1258	516	0.04%	0.005%
85	12.807	3640	3644	3645	rBV3	881	657	0.05%	0.006%
86	12.913	3673	3677	3679	rBV3	1638	1303	0.10%	0.013%
87	12.945	3684	3687	3691	rVB3	1153	785	0.06%	0.008%
88	13.064	3722	3724	3725	rBV2	1334	502	0.04%	0.005%
89	13.164	3753	3755	3757	rBV3	1286	612	0.05%	0.006%
90	13.209	3767	3769	3772	rVB4	1517	949	0.07%	0.009%
91	13.264	3783	3786	3790	rBV4	1039	1030	0.08%	0.010%
92	13.360	3813	3816	3817	rBV2	867	500	0.04%	0.005%
93	13.460	3844	3847	3853	rBV6	1364	1706	0.13%	0.017%
94	14.055	4030	4032	4036	rBV5	1250	991	0.07%	0.010%
95	14.112	4049	4050	4054	rVB4	1409	577	0.04%	0.006%
96	14.186	4070	4073	4075	rBV4	1596	903	0.07%	0.009%
97	14.399	4136	4139	4142	rBV5	1330	796	0.06%	0.008%
98	14.630	4208	4211	4213	rBV4	1164	816	0.06%	0.008%
99	14.968	4312	4316	4317	rBV4	1549	1157	0.09%	0.011%
100	15.148	4369	4372	4373	rBV3	1704	1137	0.09%	0.011%


Sum of corrected areas: 10212263

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016510.D
Acq On : 04 Jun 2020 15:18
Operator : SY/MD
Sample : L2849-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTQ0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

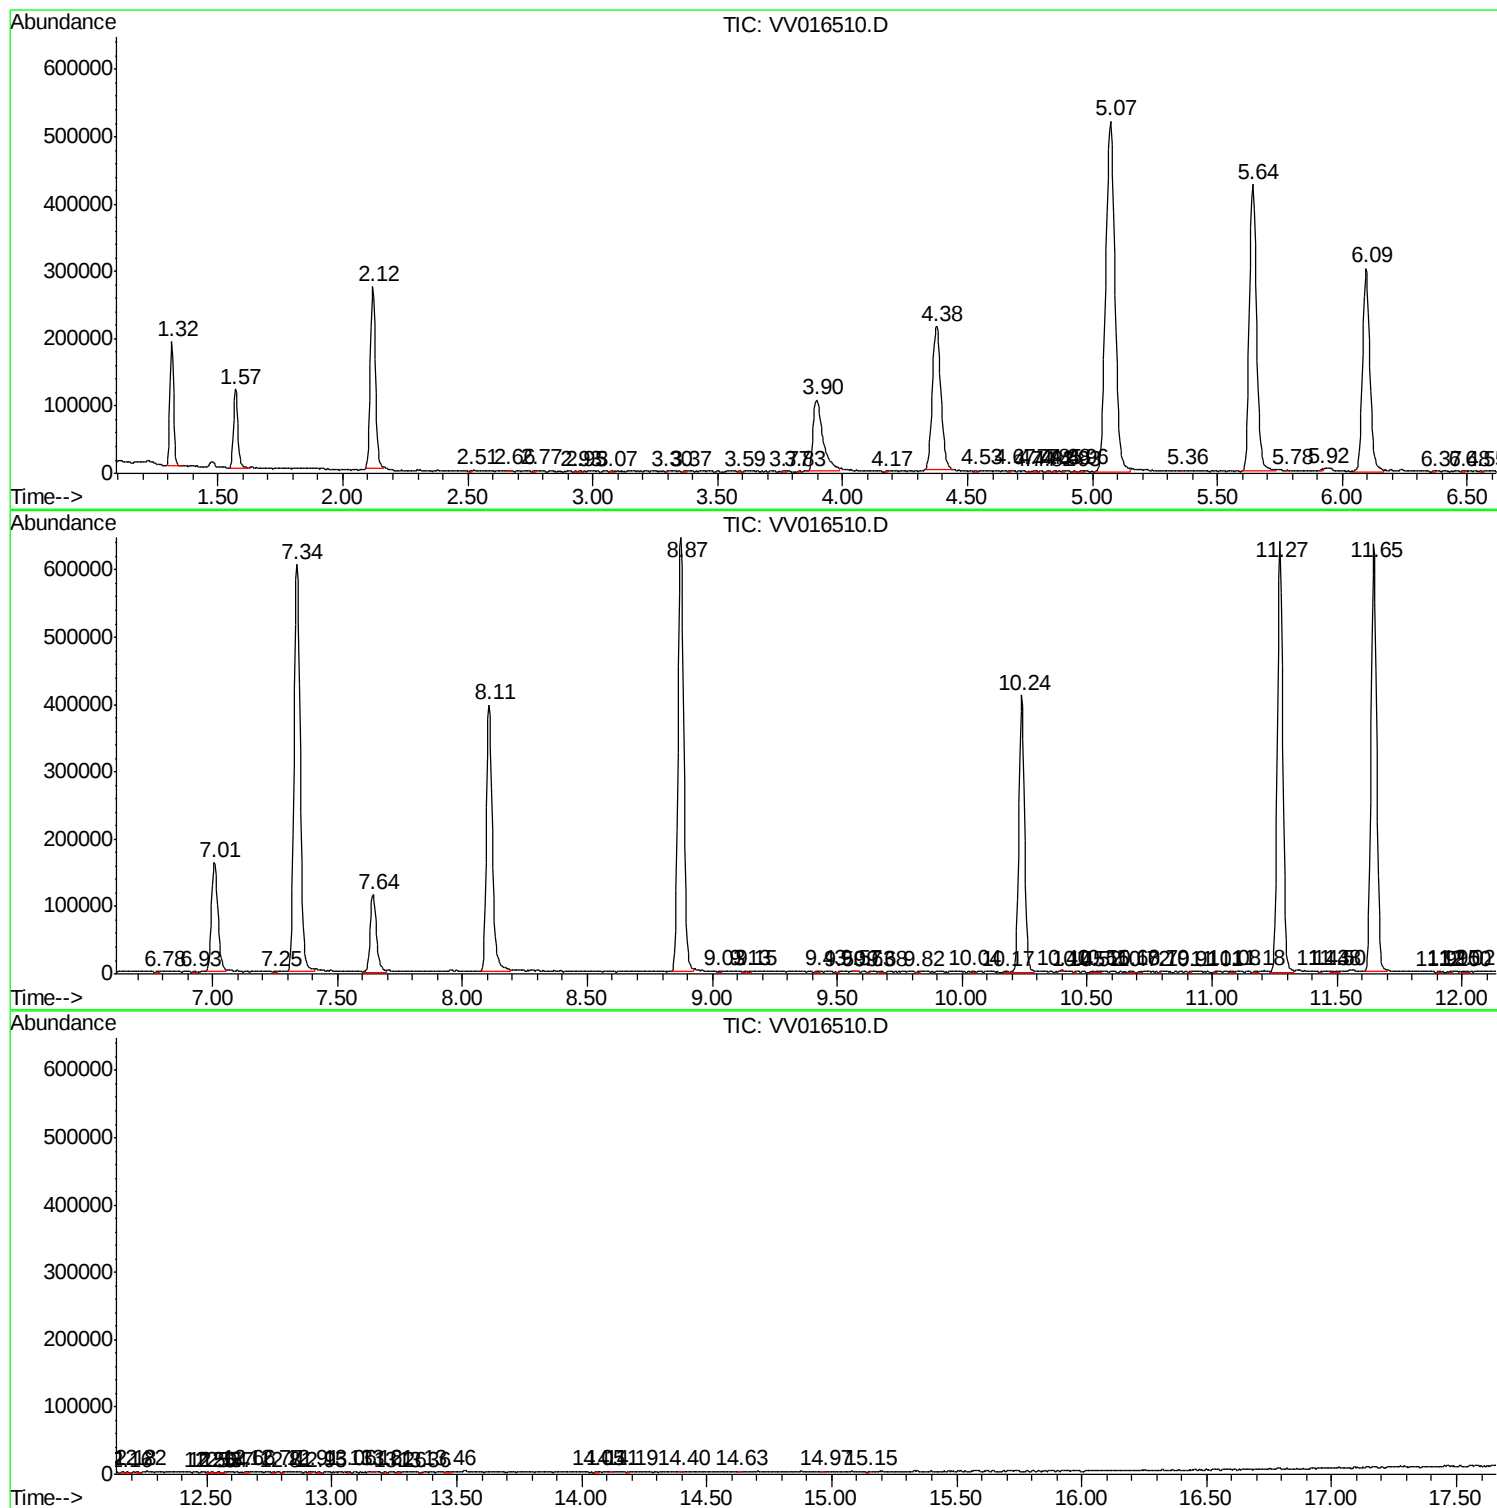

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016510.D
Acq On : 04 Jun 2020 15:18
Operator : SY/MD
Sample : L2849-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTQ0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016510.D
Acq On : 04 Jun 2020 15:18
Operator : SY/MD
Sample : L2849-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTQ0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc