

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016512.D
 Acq On : 04 Jun 2020 16:30
 Operator : SY/MD
 Sample : L2849-11DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB2	311371	330004	24.87%	2.829%
2	1.560	140	146	158	rVB	120398	143337	10.80%	1.229%
3	2.116	310	319	333	rBV	240868	348996	26.30%	2.992%
4	2.447	418	422	424	rBV5	1707	1379	0.10%	0.012%
5	2.778	516	525	527	rBV8	4743	5979	0.45%	0.051%
6	2.830	540	541	545	rBV3	1095	559	0.04%	0.005%
7	2.913	563	567	569	rBV5	1155	671	0.05%	0.006%
8	3.180	646	650	651	rBV3	1330	729	0.05%	0.006%
9	3.251	668	672	674	rBV5	1230	846	0.06%	0.007%
10	3.370	706	709	710	rBV3	1103	574	0.04%	0.005%
11	3.476	740	742	745	rVB4	1282	581	0.04%	0.005%
12	3.492	745	747	750	rBV3	1107	578	0.04%	0.005%
13	3.585	771	776	778	rBV4	1242	950	0.07%	0.008%
14	3.601	778	781	785	rVB5	1300	1004	0.08%	0.009%
15	3.646	791	795	798	rBV5	1118	1026	0.08%	0.009%
16	3.743	822	825	828	rBV3	1154	728	0.05%	0.006%
17	3.791	835	840	841	rBV5	1698	1242	0.09%	0.011%
18	3.933	862	884	915	rBV2	317370	1049940	79.14%	9.002%
19	4.373	1007	1021	1045	rVB	214163	520922	39.26%	4.466%
20	4.624	1097	1099	1103	rBV4	1242	913	0.07%	0.008%
21	4.691	1112	1120	1122	rBV7	2455	2824	0.21%	0.024%
22	4.769	1140	1144	1146	rBV4	1182	799	0.06%	0.007%
23	4.904	1179	1186	1190	rBV7	1224	1537	0.12%	0.013%
24	4.974	1206	1208	1212	rVV4	1275	818	0.06%	0.007%
25	5.068	1220	1237	1263	rBV2	520434	1326739	100.00%	11.375%
26	5.312	1309	1313	1315	rBV3	1196	1031	0.08%	0.009%
27	5.585	1395	1398	1402	rBV5	955	777	0.06%	0.007%
28	5.640	1402	1415	1440	rBV	451334	893496	67.35%	7.660%
29	6.093	1543	1556	1575	rBV	300268	610257	46.00%	5.232%
30	6.720	1748	1751	1752	rBV2	1166	661	0.05%	0.006%
31	6.907	1806	1809	1812	rBV3	908	746	0.06%	0.006%
32	7.006	1828	1840	1857	rBV	167299	299857	22.60%	2.571%
33	7.338	1931	1943	1962	rBV	624112	1060843	79.96%	9.095%
34	7.534	2001	2004	2011	rBV8	1473	1422	0.11%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016512.D
 Acq On : 04 Jun 2020 16:30
 Operator : SY/MD
 Sample : L2849-11DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	7.640	2027	2037	2057	rBV	119361	207681	15.65%	1.781%
36	7.916	2121	2123	2124	rBV2	1452	581	0.04%	0.005%
37	7.997	2144	2148	2156	rVB8	3047	4191	0.32%	0.036%
38	8.106	2170	2182	2205	rBV	442199	751017	56.61%	6.439%
39	8.412	2274	2277	2279	rBV3	1258	889	0.07%	0.008%
40	8.875	2408	2421	2443	rBV	697992	1110109	83.67%	9.518%
41	9.032	2466	2470	2480	rVB9	3843	5995	0.45%	0.051%
42	9.096	2487	2490	2495	rBV6	1565	1644	0.12%	0.014%
43	9.235	2528	2533	2537	rBV7	1582	1594	0.12%	0.014%
44	9.350	2567	2569	2571	rBV3	1288	745	0.06%	0.006%
45	9.386	2578	2580	2586	rVB7	2196	1730	0.13%	0.015%
46	9.421	2587	2591	2596	rVV7	1172	1095	0.08%	0.009%
47	9.640	2657	2659	2660	rBV2	1148	602	0.05%	0.005%
48	9.678	2667	2671	2673	rBV4	1632	1236	0.09%	0.011%
49	9.823	2712	2716	2717	rBV4	1310	874	0.07%	0.007%
50	9.894	2734	2738	2741	rBV6	963	904	0.07%	0.008%
51	10.174	2822	2825	2827	rVV3	1275	848	0.06%	0.007%
52	10.238	2834	2845	2861	rBV	435849	680547	51.29%	5.835%
53	10.473	2914	2918	2920	rVB6	1205	930	0.07%	0.008%
54	10.501	2920	2927	2929	rBV7	1626	1563	0.12%	0.013%
55	10.720	2991	2995	2996	rBV4	1065	761	0.06%	0.007%
56	10.784	3012	3015	3021	rBV7	1811	1717	0.13%	0.015%
57	10.810	3021	3023	3027	rVB4	1232	817	0.06%	0.007%
58	10.839	3027	3032	3036	rBV6	1683	1820	0.14%	0.016%
59	10.878	3040	3044	3047	rBV5	1695	1479	0.11%	0.013%
60	10.942	3055	3064	3069	rBV6	6011	9413	0.71%	0.081%
61	11.067	3097	3103	3109	rVB6	2396	2879	0.22%	0.025%
62	11.093	3109	3111	3115	rBV4	1061	891	0.07%	0.008%
63	11.270	3155	3166	3183	rBV	709830	1088909	82.07%	9.336%
64	11.427	3212	3215	3217	rBV3	1266	922	0.07%	0.008%
65	11.473	3225	3229	3231	rBV4	846	747	0.06%	0.006%
66	11.646	3271	3283	3300	rBV	673564	1056107	79.60%	9.055%
67	11.858	3347	3349	3351	rBV2	1133	640	0.05%	0.005%
68	11.997	3389	3392	3394	rBV3	1095	741	0.06%	0.006%
69	12.251	3468	3471	3473	rBV2	1747	1117	0.08%	0.010%
70	12.270	3473	3477	3479	rVV4	1758	1390	0.10%	0.012%
71	12.357	3500	3504	3505	rBV4	1224	857	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016512.D
 Acq On : 04 Jun 2020 16:30
 Operator : SY/MD
 Sample : L2849-11DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	12.392	3512	3515	3518	rBV3	1179	768	0.06%	0.007%
73	12.530	3554	3558	3559	rBV3	1155	811	0.06%	0.007%
74	12.611	3581	3583	3586	rVB4	1105	566	0.04%	0.005%
75	12.669	3595	3601	3610	rBV10	10312	16178	1.22%	0.139%
76	12.752	3623	3627	3631	rBV7	1208	1094	0.08%	0.009%
77	12.810	3642	3645	3649	rVB4	2015	1484	0.11%	0.013%
78	12.842	3649	3655	3658	rBV8	1679	2074	0.16%	0.018%
79	13.058	3720	3722	3724	rBV3	1003	595	0.04%	0.005%
80	13.132	3743	3745	3747	rBV3	1261	608	0.05%	0.005%
81	13.228	3773	3775	3778	rVB5	1482	663	0.05%	0.006%
82	13.286	3785	3793	3803	rVV4	13104	19741	1.49%	0.169%
83	13.421	3830	3835	3838	rBV7	1212	1151	0.09%	0.010%
84	13.440	3838	3841	3842	rBV2	1604	855	0.06%	0.007%
85	13.450	3842	3844	3849	rVB6	1684	1077	0.08%	0.009%
86	13.530	3862	3869	3880	rVB	13769	22109	1.67%	0.190%
87	13.678	3912	3915	3916	rBV3	943	625	0.05%	0.005%
88	13.771	3935	3944	3955	rVB5	13363	21405	1.61%	0.184%
89	13.858	3967	3971	3975	rBV5	2165	1637	0.12%	0.014%
90	13.884	3977	3979	3984	rVB5	1089	795	0.06%	0.007%
91	13.961	3998	4003	4006	rBV6	1603	1658	0.12%	0.014%
92	14.013	4014	4019	4023	rBV7	1368	1617	0.12%	0.014%
93	14.170	4062	4068	4071	rBV6	1319	1700	0.13%	0.015%
94	14.299	4104	4108	4109	rBV3	1389	1070	0.08%	0.009%
95	14.395	4137	4138	4142	rVB2	1383	586	0.04%	0.005%
96	14.440	4148	4152	4153	rBV2	962	647	0.05%	0.006%
97	14.575	4192	4194	4197	rBV4	822	625	0.05%	0.005%
98	14.704	4230	4234	4237	rBV4	1452	1322	0.10%	0.011%
99	14.768	4252	4254	4259	rBV4	1133	948	0.07%	0.008%
100	14.968	4313	4316	4317	rBV3	1216	691	0.05%	0.006%


Sum of corrected areas: 11663847

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016512.D
Acq On : 04 Jun 2020 16:30
Operator : SY/MD
Sample : L2849-11DL 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

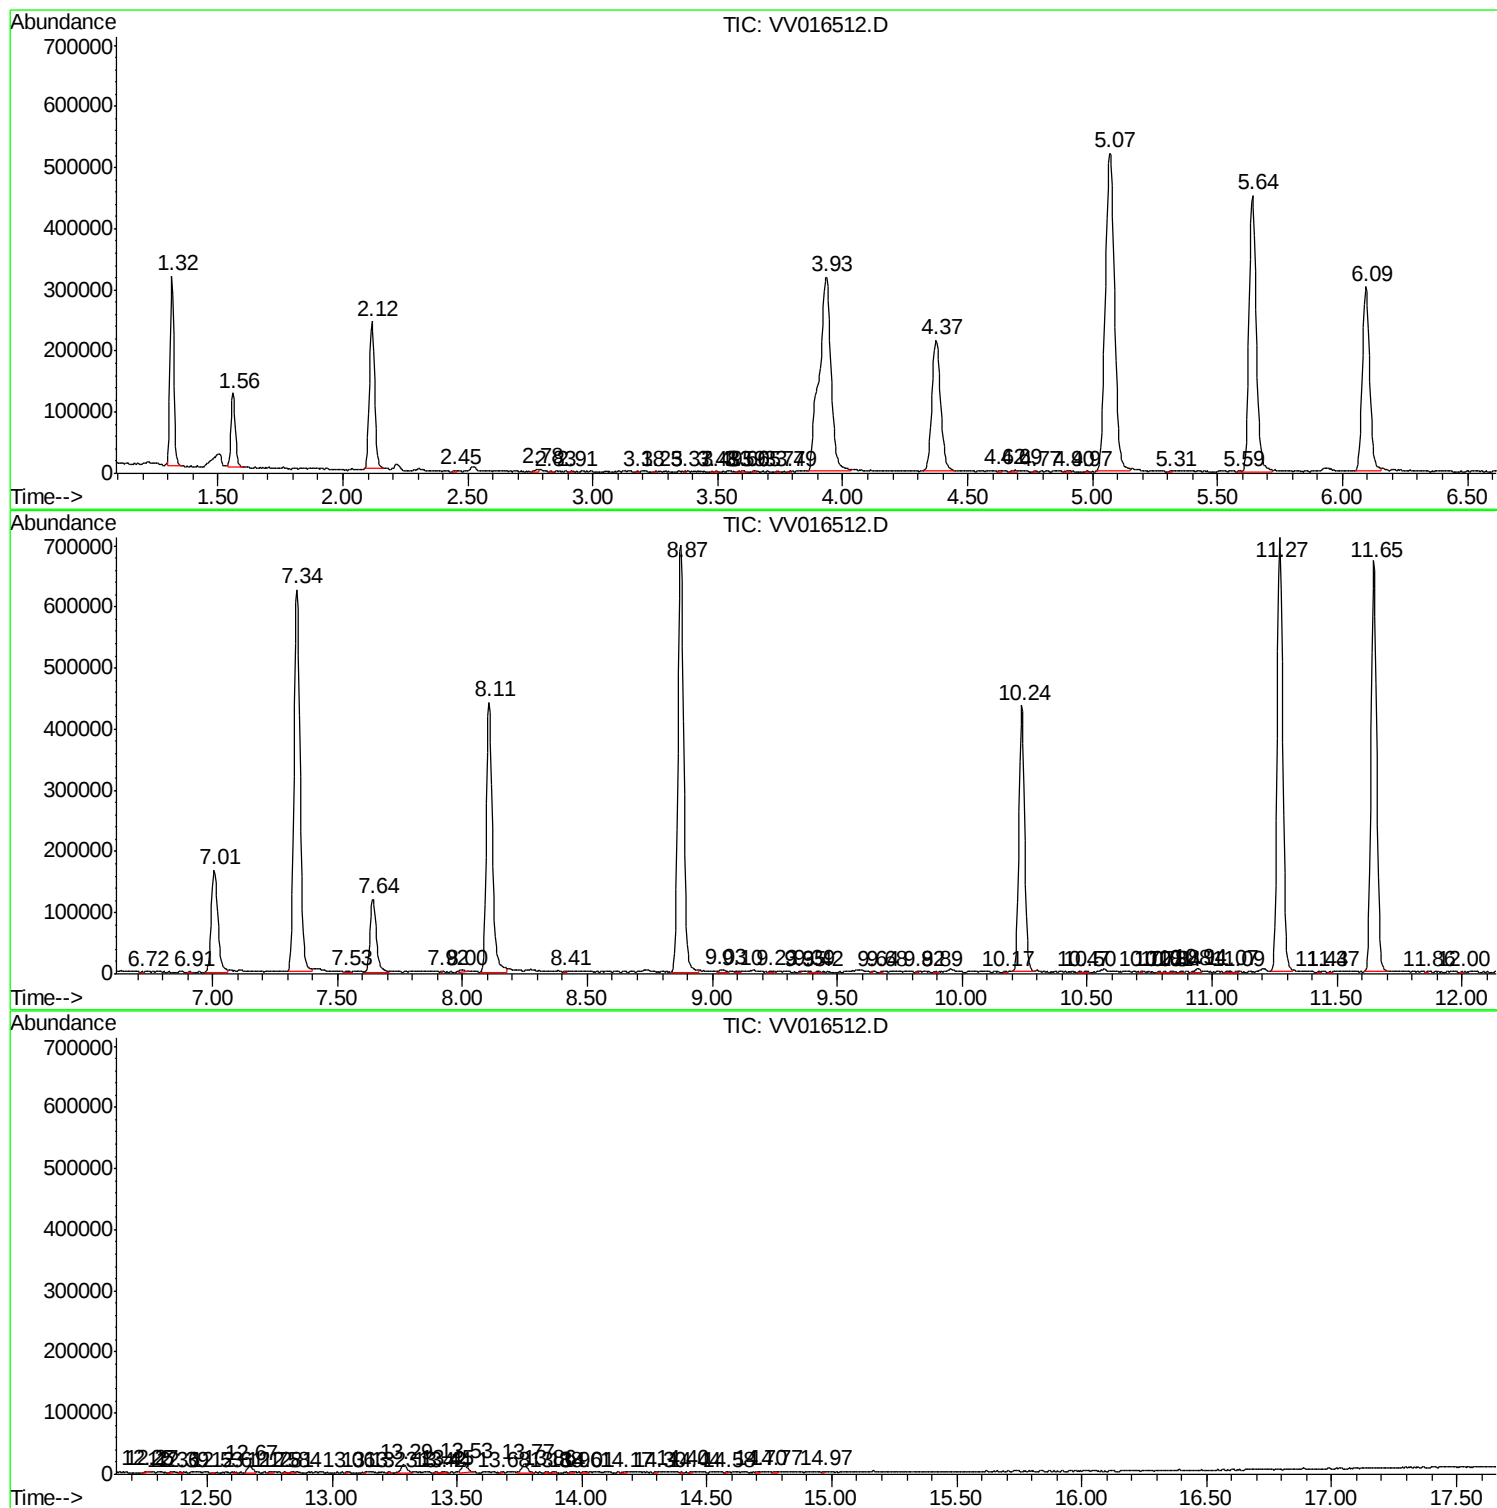

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016512.D
Acq On : 04 Jun 2020 16:30
Operator : SY/MD
Sample : L2849-11DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016512.D
Acq On : 04 Jun 2020 16:30
Operator : SY/MD
Sample : L2849-11DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc