

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016515.D
 Acq On : 04 Jun 2020 17:41
 Operator : SY/MD
 Sample : L2849-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTQ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	81	rVB	156598	159217	11.76%	1.534%
2	1.563	141	147	157	rVB	122638	141637	10.46%	1.364%
3	2.116	310	319	333	rBV	248726	353051	26.08%	3.401%
4	2.412	408	411	413	rBV4	1469	1000	0.07%	0.010%
5	2.608	466	472	475	rBV6	1523	1971	0.15%	0.019%
6	2.914	564	567	569	rBV4	705	477	0.04%	0.005%
7	2.959	577	581	583	rBV4	1223	1074	0.08%	0.010%
8	3.029	601	603	606	rVB4	1434	751	0.06%	0.007%
9	3.097	621	624	628	rVB5	1473	1053	0.08%	0.010%
10	3.209	656	659	661	rBV3	1583	987	0.07%	0.010%
11	3.251	668	672	674	rBV3	1224	1110	0.08%	0.011%
12	3.264	674	676	678	rVV3	925	583	0.04%	0.006%
13	3.306	687	689	695	rVB6	1574	1236	0.09%	0.012%
14	3.364	705	707	710	rBV3	1173	606	0.04%	0.006%
15	3.396	713	717	721	rBV5	1758	1665	0.12%	0.016%
16	3.444	729	732	734	rBV3	1297	796	0.06%	0.008%
17	3.663	798	800	803	rVB3	1126	653	0.05%	0.006%
18	3.701	808	812	814	rBV4	805	589	0.04%	0.006%
19	3.714	814	816	820	rVB4	1163	874	0.06%	0.008%
20	3.746	820	826	828	rBV6	1141	1021	0.08%	0.010%
21	3.788	834	839	843	rBV4	1254	1364	0.10%	0.013%
22	3.894	856	872	903	rBV2	111556	300052	22.16%	2.891%
23	4.254	981	984	986	rBV3	1151	779	0.06%	0.008%
24	4.373	1006	1021	1046	rVB	218978	529869	39.14%	5.105%
25	4.682	1115	1117	1122	rVB4	960	711	0.05%	0.007%
26	4.933	1192	1195	1198	rBV4	910	733	0.05%	0.007%
27	5.068	1219	1237	1264	rBV2	523979	1353849	100.00%	13.042%
28	5.454	1354	1357	1358	rBV3	855	513	0.04%	0.005%
29	5.518	1372	1377	1379	rBV4	1382	1153	0.09%	0.011%
30	5.640	1399	1415	1445	rBV	427847	863584	63.79%	8.319%
31	5.794	1461	1463	1466	rBV3	914	626	0.05%	0.006%
32	5.833	1473	1475	1477	rBV3	1571	769	0.06%	0.007%
33	6.032	1533	1537	1539	rBV5	1263	891	0.07%	0.009%
34	6.093	1543	1556	1574	rVV	312868	625571	46.21%	6.027%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016515.D
 Acq On : 04 Jun 2020 17:41
 Operator : SY/MD
 Sample : L2849-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTQ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.280	1612	1614	1617	rBV4	1144	743	0.05%	0.007%
36	6.373	1640	1643	1644	rBV	1491	660	0.05%	0.006%
37	6.418	1654	1657	1660	rBV4	1673	1226	0.09%	0.012%
38	6.502	1680	1683	1684	rBV4	1590	742	0.05%	0.007%
39	6.537	1691	1694	1698	rVB4	1254	867	0.06%	0.008%
40	6.836	1783	1787	1789	rBV4	1343	982	0.07%	0.009%
41	7.007	1830	1840	1858	rBV	166284	291846	21.56%	2.812%
42	7.264	1918	1920	1923	rVB4	2120	940	0.07%	0.009%
43	7.280	1923	1925	1930	rBV5	1086	1000	0.07%	0.010%
44	7.338	1930	1943	1962	rBV	624064	1081030	79.85%	10.414%
45	7.640	2028	2037	2060	rVB	117547	202193	14.93%	1.948%
46	8.106	2171	2182	2210	rBV	399683	668792	49.40%	6.443%
47	8.749	2380	2382	2386	rBV5	1187	788	0.06%	0.008%
48	8.872	2408	2420	2435	rBV	647297	1038723	76.72%	10.007%
49	9.225	2525	2530	2531	rBV3	1116	724	0.05%	0.007%
50	9.270	2541	2544	2548	rVB5	1142	845	0.06%	0.008%
51	9.344	2565	2567	2571	rBV4	1269	805	0.06%	0.008%
52	9.373	2571	2576	2580	rBV8	1274	1273	0.09%	0.012%
53	9.653	2656	2663	2665	rBV8	1838	1571	0.12%	0.015%
54	9.781	2699	2703	2705	rBV5	1729	1158	0.09%	0.011%
55	10.003	2770	2772	2776	rBV5	1318	1079	0.08%	0.010%
56	10.113	2802	2806	2807	rBV4	1141	904	0.07%	0.009%
57	10.238	2834	2845	2863	rBV	424940	664552	49.09%	6.402%
58	10.331	2872	2874	2878	rBV5	1201	860	0.06%	0.008%
59	10.508	2927	2929	2931	rBV2	1193	764	0.06%	0.007%
60	10.627	2963	2966	2968	rBV4	1016	670	0.05%	0.006%
61	10.714	2988	2993	2995	rBV5	1032	915	0.07%	0.009%
62	10.765	3005	3009	3011	rBV4	1162	869	0.06%	0.008%
63	10.833	3028	3030	3032	rBV3	1551	776	0.06%	0.007%
64	10.871	3038	3042	3045	rBV5	2089	1173	0.09%	0.011%
65	10.994	3076	3080	3083	rVB4	1306	816	0.06%	0.008%
66	11.035	3091	3093	3096	rBV3	1003	667	0.05%	0.006%
67	11.071	3101	3104	3107	rBV4	1124	706	0.05%	0.007%
68	11.145	3125	3127	3134	rVB8	1546	1436	0.11%	0.014%
69	11.187	3137	3140	3144	rBV5	1469	1367	0.10%	0.013%
70	11.270	3155	3166	3188	rBV	649370	1008310	74.48%	9.714%
71	11.399	3203	3206	3207	rBV3	949	483	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060420\
 Data File : VV016515.D
 Acq On : 04 Jun 2020 17:41
 Operator : SY/MD
 Sample : L2849-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTQ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.441	3217	3219	3223	rVB3	1401	987	0.07%	0.010%
73	11.463	3223	3226	3227	rBV3	1471	847	0.06%	0.008%
74	11.646	3272	3283	3297	rBV	651580	1018978	75.27%	9.816%
75	11.781	3323	3325	3328	rVB3	1183	556	0.04%	0.005%
76	11.945	3374	3376	3379	rVB3	1339	484	0.04%	0.005%
77	11.961	3379	3381	3384	rVB3	1184	650	0.05%	0.006%
78	11.981	3384	3387	3388	rBV2	1162	732	0.05%	0.007%
79	12.096	3421	3423	3425	rBV2	1069	530	0.04%	0.005%
80	12.183	3448	3450	3454	rBV4	1207	930	0.07%	0.009%
81	12.215	3458	3460	3462	rBV3	1138	484	0.04%	0.005%
82	12.354	3501	3503	3506	rBV3	1116	806	0.06%	0.008%
83	12.447	3529	3532	3534	rBV3	1119	671	0.05%	0.006%
84	12.460	3534	3536	3539	rVV4	1230	557	0.04%	0.005%
85	12.518	3551	3554	3557	rBV3	1186	686	0.05%	0.007%
86	12.968	3691	3694	3697	rBV5	1215	869	0.06%	0.008%
87	13.534	3862	3870	3874	rBV9	3415	5953	0.44%	0.057%
88	13.765	3939	3942	3943	rBV3	1152	701	0.05%	0.007%
89	13.871	3972	3975	3980	rBV6	942	897	0.07%	0.009%
90	13.894	3980	3982	3984	rBV3	1226	695	0.05%	0.007%
91	13.971	4003	4006	4008	rBV3	1606	817	0.06%	0.008%
92	14.299	4105	4108	4111	rVB4	1194	879	0.06%	0.008%
93	14.325	4111	4116	4119	rBV5	1341	1213	0.09%	0.012%
94	14.450	4153	4155	4158	rBV3	1219	780	0.06%	0.008%
95	14.469	4158	4161	4162	rBV3	1152	505	0.04%	0.005%
96	14.547	4183	4185	4189	rBV4	1134	796	0.06%	0.008%
97	14.608	4202	4204	4206	rBV2	1318	631	0.05%	0.006%
98	14.778	4252	4257	4259	rBV4	1777	1312	0.10%	0.013%
99	14.900	4291	4295	4296	rBV3	1071	660	0.05%	0.006%
100	16.074	4658	4660	4665	rBV4	1904	1641	0.12%	0.016%


Sum of corrected areas: 10380317

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060420\
Data File : VV016515.D
Acq On : 04 Jun 2020 17:41
Operator : SY/MD
Sample : L2849-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTQ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

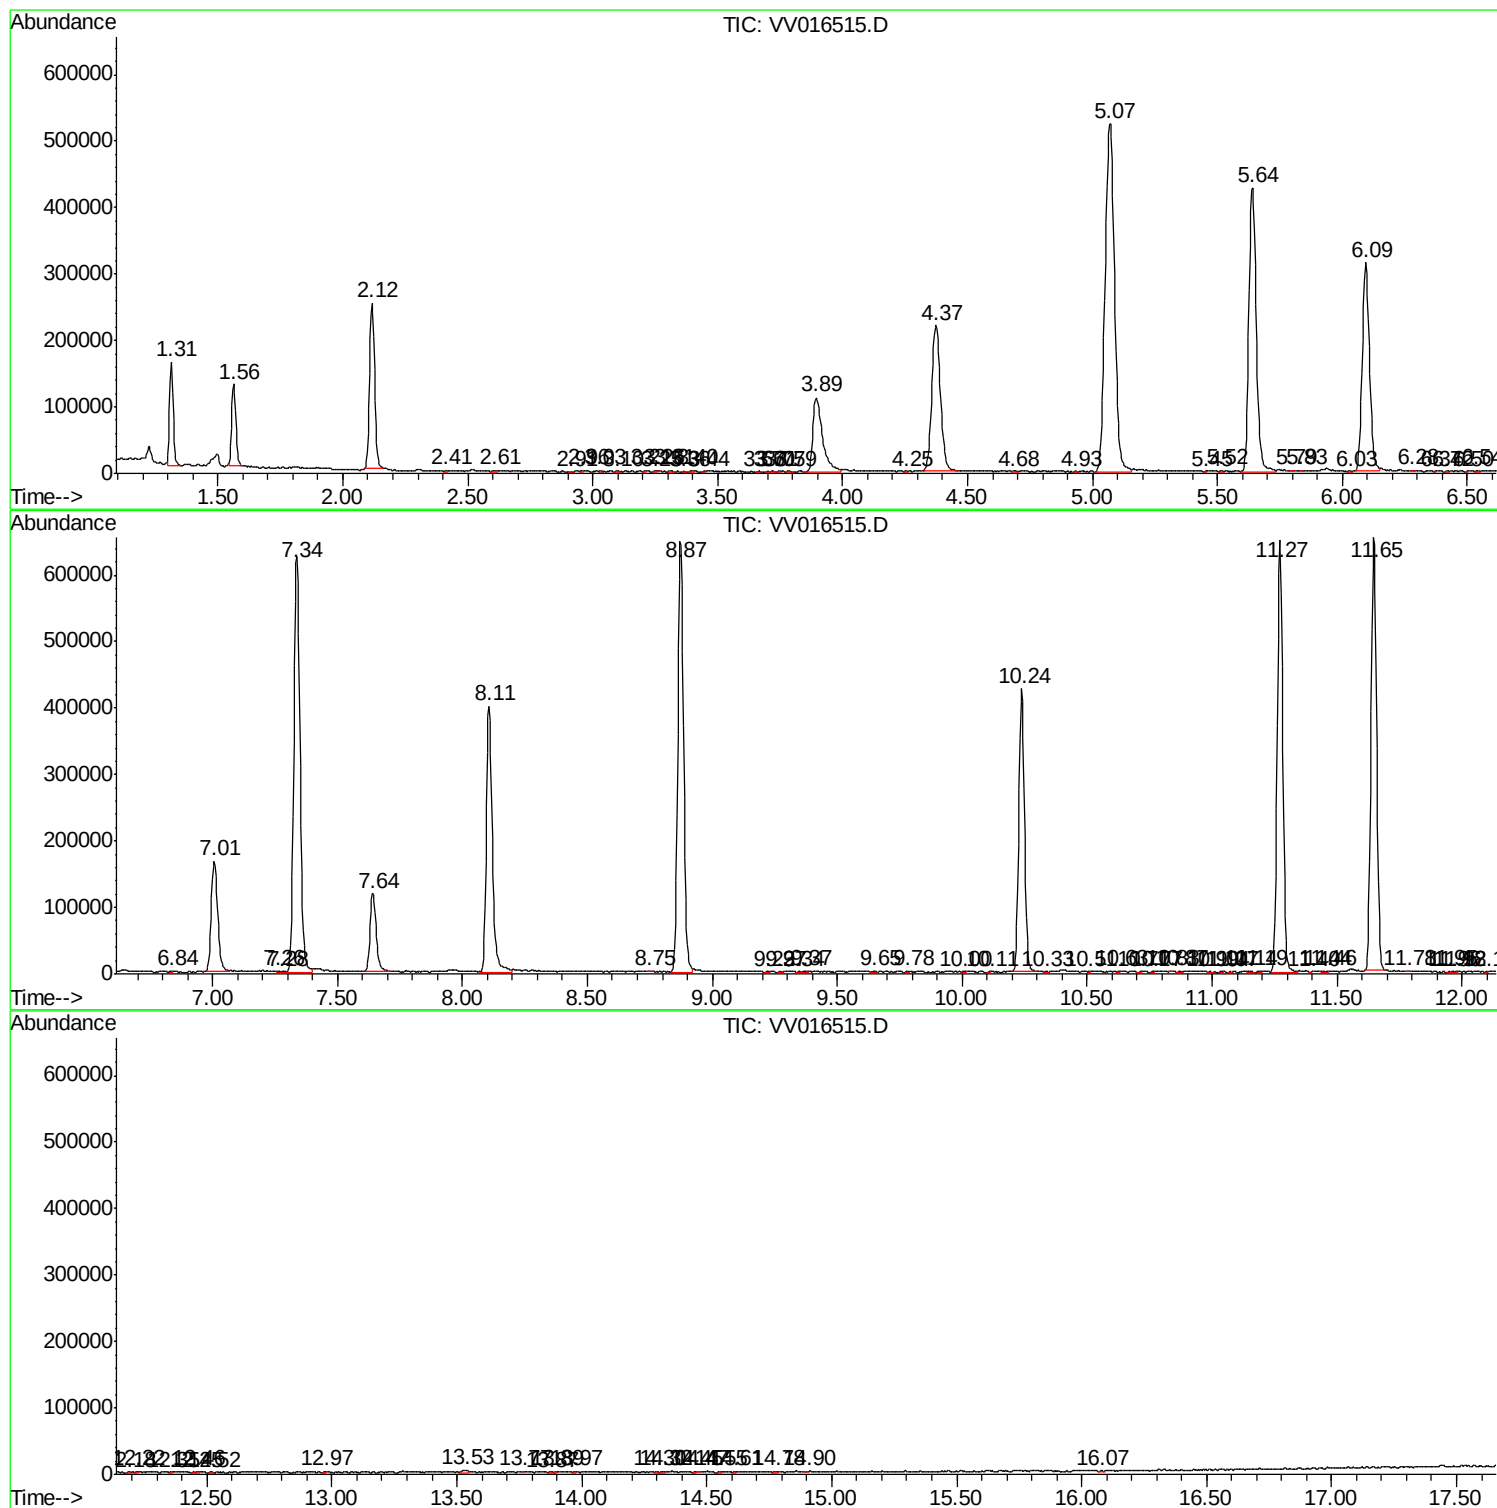

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016515.D
Acq On : 04 Jun 2020 17:41
Operator : SY/MD
Sample : L2849-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTQ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060420\
Data File : VV016515.D
Acq On : 04 Jun 2020 17:41
Operator : SY/MD
Sample : L2849-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTQ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc