


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV060420\
 Data File : VV016496.D
 Acq On : 04 Jun 2020 09:29
 Operator : SY/MD
 Sample : BFB80
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB80

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis
 Last Update : Fri Jun 05 01:52:01 2020

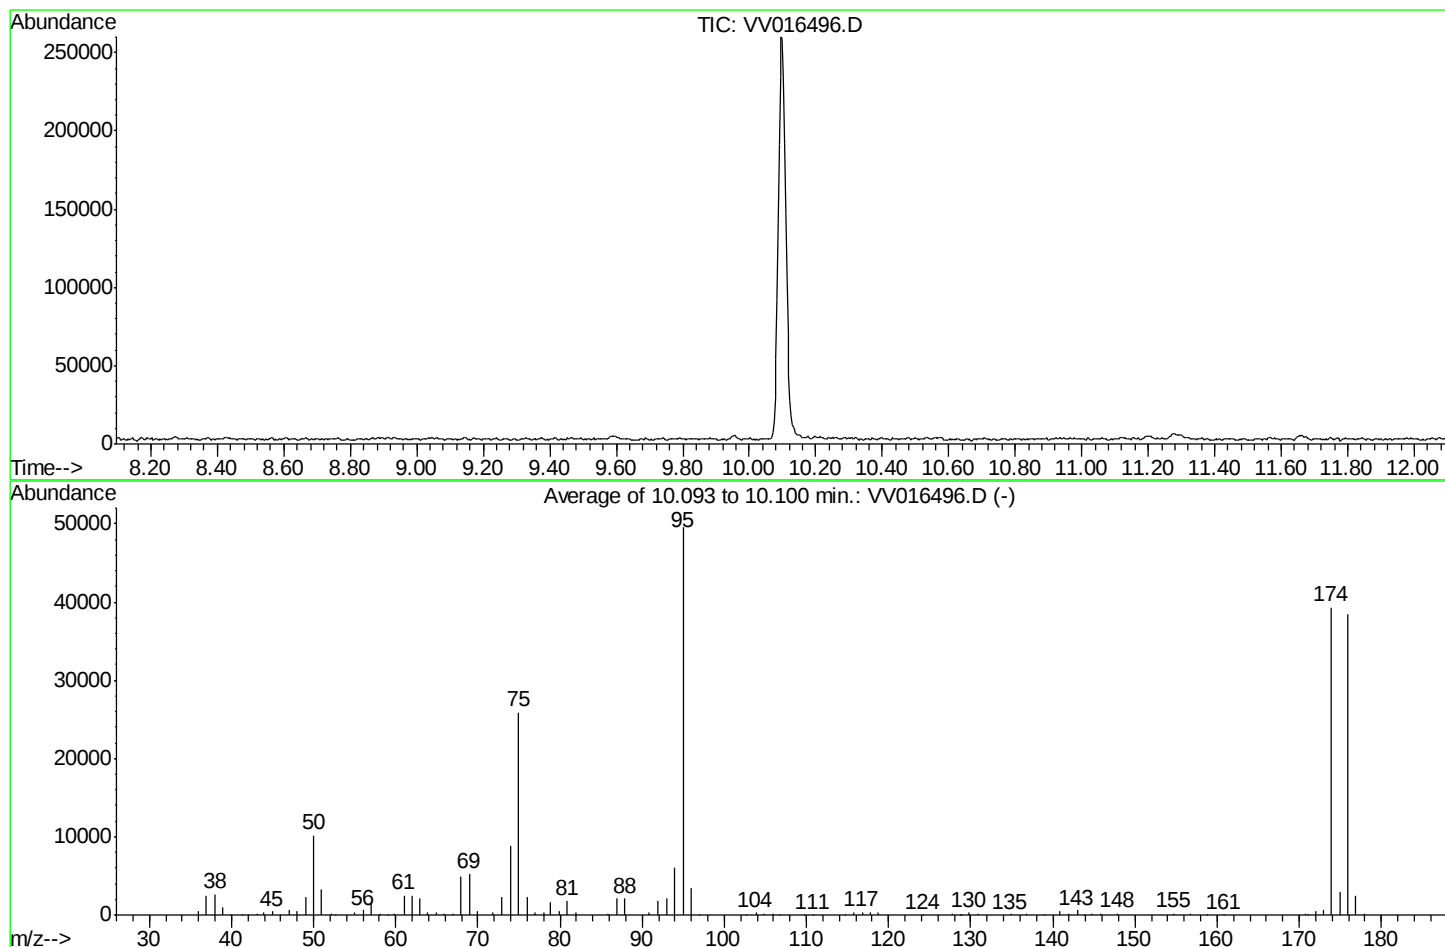

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	10226	PASS
75	95	30	80	52.2	25884	PASS
95	95	100	100	100.0	49562	PASS
96	95	5	9	6.9	3416	PASS
173	174	0.00	2	1.6	645	PASS
174	95	50	120	79.4	39330	PASS
175	174	5	9	7.6	2983	PASS
176	174	95	101	97.7	38424	PASS
177	176	5	9	6.4	2470	PASS

m/z	Abundance
36.00	434.0
37.00	2417.0
38.00	2533.0
39.00	1200.0
39.90	446.0
40.80	129.0
41.30	119.0
42.10	110.0
43.20	134.0
44.00	899.0
45.00	592.0
46.00	151.0
47.00	761.0
47.90	493.0
49.00	2257.0
50.00	9779.0
51.00	3212.0
52.10	167.0
55.00	261.0
56.00	753.0
57.00	1424.0
58.00	157.0
59.90	464.0
61.00	2315.0
62.00	2466.0
63.00	2104.0
63.90	331.0
64.90	351.0
67.10	139.0
67.90	4621.0
69.00	4939.0
70.00	432.0
71.90	412.0
72.90	2334.0
74.00	8284.0
75.00	24416.0
76.00	2289.0
77.00	362.0
78.00	277.0
78.90	1597.0
79.80	456.0
80.90	1651.0
82.00	290.0
85.80	123.0
87.00	1789.0
87.90	1930.0
90.80	236.0
91.90	1595.0
93.00	2154.0
94.00	5792.0
95.00	46136.0
96.00	3285.0
97.00	177.0
103.90	320.0
104.80	110.0
105.90	253.0
109.60	108.0
115.70	248.0
116.80	335.0
117.90	317.0
118.80	260.0
127.80	187.0
129.80	280.0
130.80	107.0
134.90	146.0
136.80	139.0
138.90	124.0
140.90	544.0
142.90	623.0
144.80	156.0
145.80	158.0
147.90	256.0
154.80	247.0
156.80	159.0
160.80	104.0
170.80	151.0
172.10	420.0
172.90	633.0
173.90	36008.0
174.90	2902.0
175.90	34912.0
176.90	2372.0
177.90	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.00	530.0
37.00	2735.0
38.00	2793.0
39.00	1256.0
39.90	418.0
40.90	111.0
41.30	116.0
43.20	182.0
44.00	830.0
45.00	532.0
45.90	133.0
47.00	681.0
47.90	504.0
49.00	2440.0
50.00	10629.0
51.00	3375.0
52.10	173.0
52.60	107.0
55.00	313.0
56.10	771.0
57.00	1533.0
58.10	156.0
59.00	102.0
59.90	490.0
61.00	2681.0
62.00	2558.0
63.00	2170.0
63.90	384.0
64.90	410.0
66.00	151.0
67.00	165.0
67.90	4975.0
69.00	5405.0
70.00	491.0
71.90	416.0
72.90	2351.0
74.00	9244.0
75.00	26880.0
76.00	2409.0
77.00	392.0
78.00	309.0
78.90	1712.0
79.80	459.0
80.90	1906.0
81.90	391.0
85.90	131.0
86.90	2108.0
87.90	2147.0
90.80	276.0
91.90	1834.0
93.00	2241.0
94.00	6246.0
95.00	51296.0
96.00	3524.0
96.90	155.0
103.90	333.0
104.80	145.0
105.90	264.0
106.70	103.0
110.80	111.0
115.80	279.0
116.80	405.0
117.80	339.0
118.80	321.0
127.80	157.0
128.70	103.0
129.80	292.0
130.80	153.0
134.90	160.0
136.80	134.0
140.90	535.0
142.00	181.0
142.90	661.0
143.80	114.0
144.80	168.0
145.80	168.0
147.90	253.0
154.70	260.0
156.80	141.0
158.70	109.0
160.80	112.0
170.80	139.0
172.10	475.0
172.90	674.0
173.90	40528.0
174.90	3069.0
175.90	39792.0
176.90	2549.0
177.90	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.00	576.0
37.00	2862.0
38.00	2636.0
39.00	1120.0
39.90	436.0
41.00	139.0
43.10	191.0
44.00	773.0
45.00	512.0
45.80	129.0
47.00	550.0
48.00	503.0
49.00	2368.0
50.00	10270.0
51.00	3106.0
52.10	226.0
55.00	303.0
56.10	783.0
57.00	1397.0
58.20	139.0
59.90	524.0
61.00	2619.0
62.00	2416.0
63.00	2073.0
63.90	422.0
64.90	425.0
65.90	208.0
67.10	236.0
67.90	4947.0
69.00	5428.0
70.00	492.0
71.80	355.0
73.00	2269.0
74.00	9136.0
75.00	26688.0
76.00	2262.0
77.00	366.0
78.00	336.0
78.80	1715.0
79.90	453.0
80.90	2024.0
81.90	506.0
86.00	123.0
86.90	2306.0
87.90	2154.0
90.90	281.0
91.90	1831.0
93.00	2174.0
94.00	5937.0
95.00	51256.0
96.00	3439.0
96.90	154.0
102.60	109.0
103.90	293.0
104.80	158.0
105.90	236.0
106.70	112.0
110.80	122.0
114.70	108.0
115.90	307.0
116.80	390.0
117.80	299.0
118.70	345.0
124.20	134.0
127.80	136.0
128.90	131.0
129.80	255.0
130.80	169.0
134.70	133.0
136.80	128.0
140.80	497.0
142.00	213.0
143.00	670.0
143.80	134.0
144.80	124.0
145.70	163.0
147.90	237.0
154.70	210.0
156.80	111.0
158.70	107.0
171.00	107.0
172.00	468.0
173.00	628.0
173.90	41456.0
174.90	2978.0
175.90	40568.0
176.90	2489.0
177.90	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
35.60	138.0
36.90	136.0
38.40	127.0
39.00	133.0
39.90	372.0
41.10	177.0
41.80	141.0
43.80	433.0
44.60	110.0
45.00	110.0
46.10	103.0
53.00	133.0
54.60	109.0
56.00	123.0
57.50	118.0
59.70	138.0
59.90	138.0
61.40	104.0
71.80	101.0
75.20	110.0
96.90	122.0
107.30	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80