

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021494.D
 Acq On : 04 Jun 2021 09:59
 Operator : SY/MD
 Sample : VV0604MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 05 03:57:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 05 03:34:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	483268	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	457080	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	258065	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	137617	43.252	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.500%
7) Chloroethane-d5	1.568	69	113504	47.955	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.920%
11) 1,1-Dichloroethene-d2	2.105	63	185588	34.135	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.280%
21) 2-Butanone-d5	3.886	46	239083	104.788	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.790%
24) Chloroform-d	4.346	84	295711	46.688	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.380%
26) 1,2-Dichloroethane-d4	5.031	65	177994	48.790	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.580%
32) Benzene-d6	5.047	84	600867	46.991	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.980%
36) 1,2-Dichloropropane-d6	6.069	67	188337	47.695	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.380%
41) Toluene-d8	7.314	98	569027	46.709	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.420%
43) trans-1,3-Dichloroprop...	7.622	79	98710	46.710	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.420%
47) 2-Hexanone-d5	8.085	63	174843	96.427	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.430%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	263410	48.055	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.120%
66) 1,2-Dichlorobenzene-d4	11.625	152	259342	48.344	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.680%
Target Compounds						
44) trans-1,3-Dichloropropene	7.619	75	4069	0.767	ug/L	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021494.D
Acq On : 04 Jun 2021 09:59
Operator : SY/MD
Sample : VV0604MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jun 05 03:57:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 05 03:34:55 2021
Response via : Initial Calibration

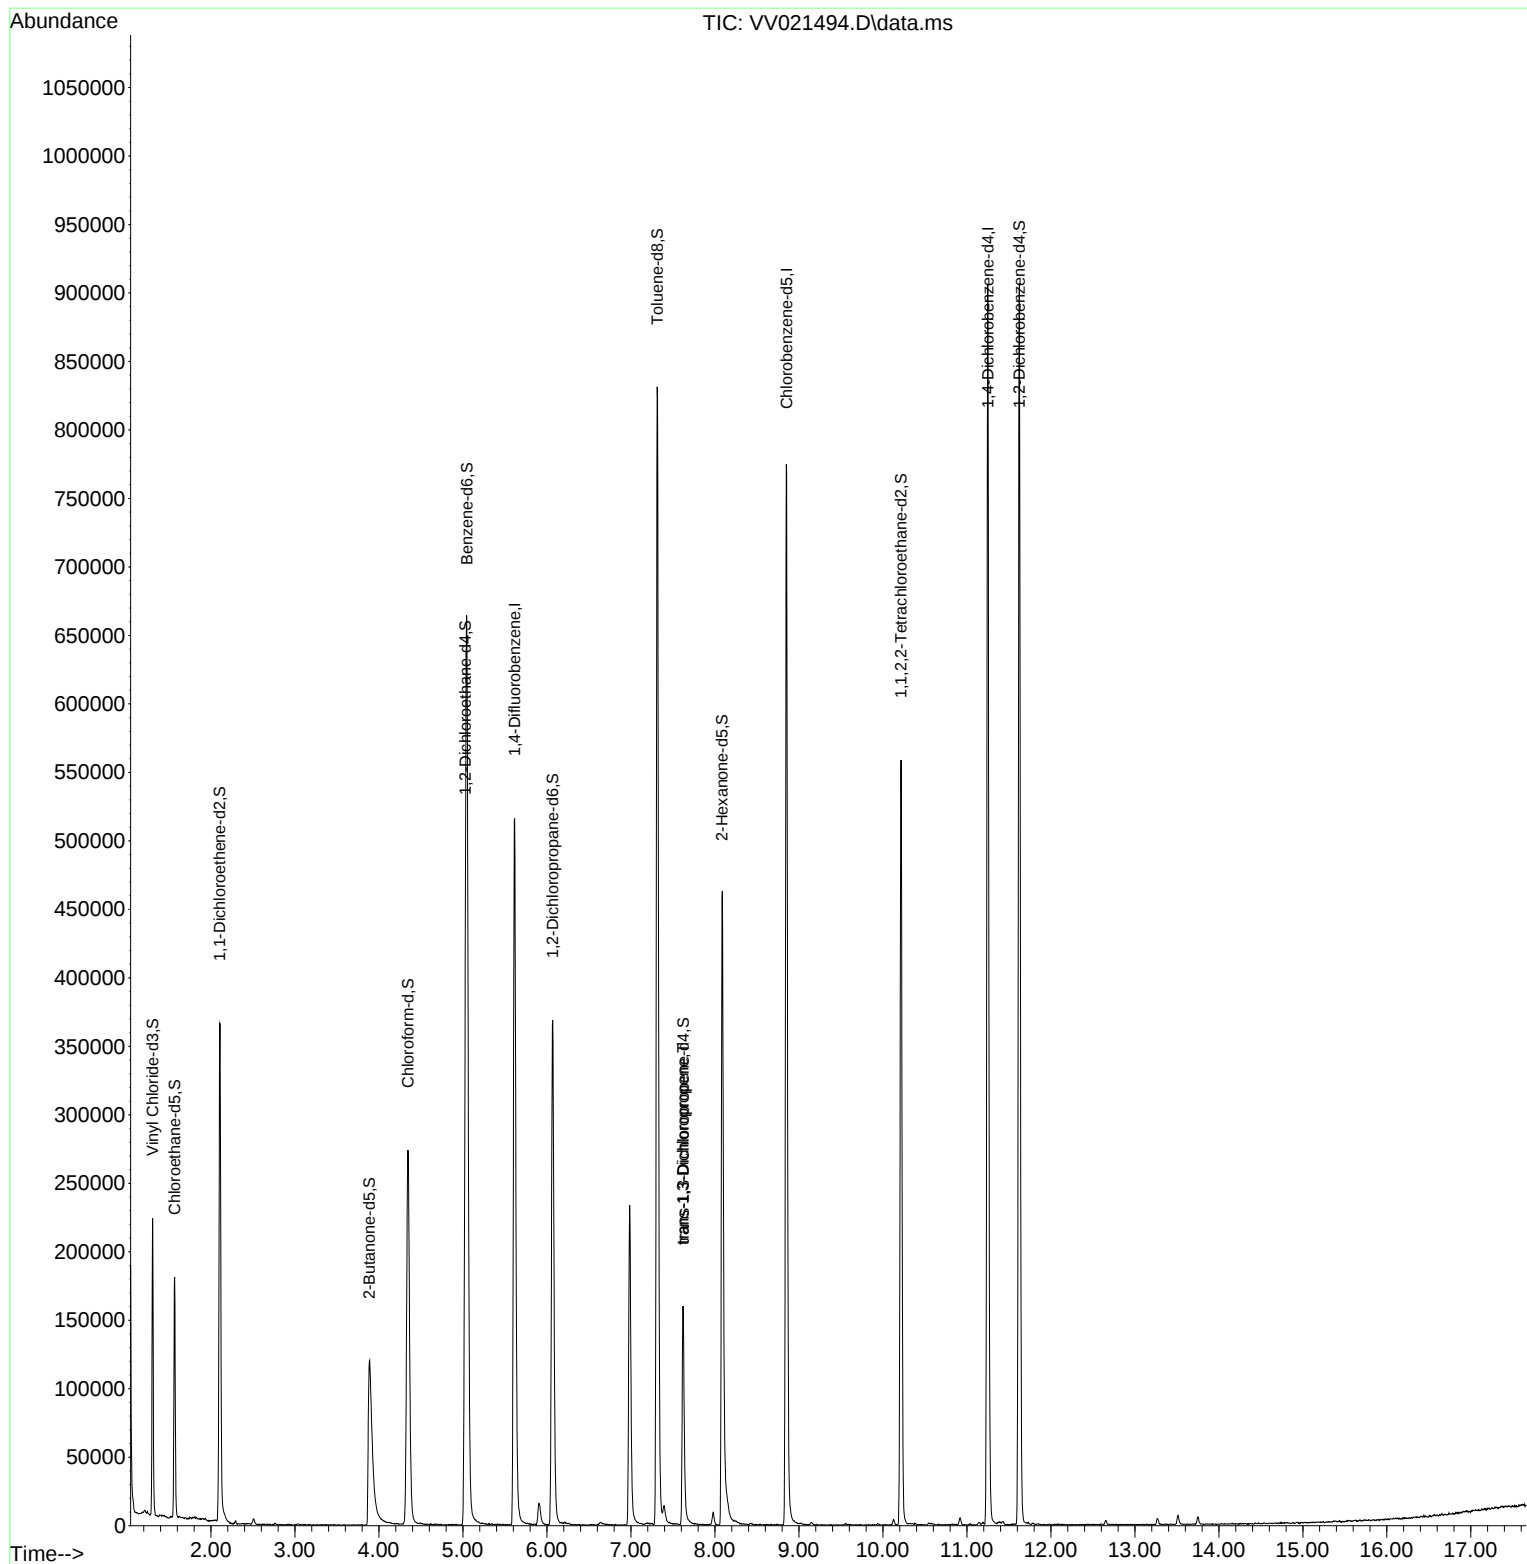

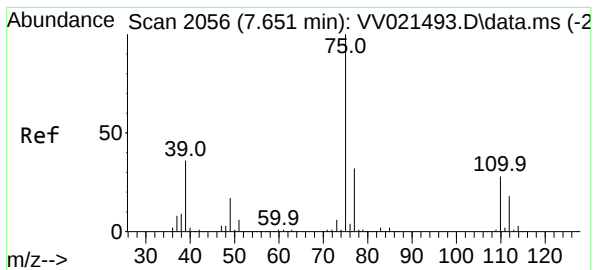

#44
 trans-1,3-Dichloropropene
 Concen: 0.767 ug/L
 RT: 7.619 min Scan# 2046
 Delta R.T. -0.032 min
 Lab File: VV021494.D
 Acq: 04 Jun 2021 09:59

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 4069
 Ion Ratio Lower Upper
 75 100
 77 41.5 22.9 42.5

