

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021514.D
 Acq On : 04 Jun 2021 18:04
 Operator : SY/MD
 Sample : M2596-09ME
 Misc : 4.61g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 05 03:59:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 05 03:34:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	501274	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	481311	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	273101	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	92547	28.042	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	56.080%#		
7) Chloroethane-d5	1.568	69	69236	28.201	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	56.400%#		
11) 1,1-Dichloroethene-d2	2.085	63	128840	22.846	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	45.700%#		
21) 2-Butanone-d5	3.905	46	175075	73.978	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	73.980%		
24) Chloroform-d	4.349	84	251632	38.302	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	76.600%		
26) 1,2-Dichloroethane-d4	5.034	65	156002	41.226	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.460%		
32) Benzene-d6	5.047	84	498200	37.000	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	74.000%		
36) 1,2-Dichloropropane-d6	6.072	67	162735	39.136	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	78.280%		
41) Toluene-d8	7.317	98	470497	36.677	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	73.360%#		
43) trans-1,3-Dichloroprop...	7.625	79	83855	37.683	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.360%		
47) 2-Hexanone-d5	8.098	63	57958	30.355	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	30.350%#		
56) 1,1,2,2-Tetrachloroeth...	10.226	84	246345	42.679	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.360%		
66) 1,2-Dichlorobenzene-d4	11.628	152	224348	39.518	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	79.040%#		
Target Compounds			Qvalue			
44) trans-1,3-Dichloropropene	7.628	75	3556	0.637	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021514.D
Acq On : 04 Jun 2021 18:04
Operator : SY/MD
Sample : M2596-09ME
Misc : 4.61g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jun 05 03:59:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 05 03:34:55 2021
Response via : Initial Calibration

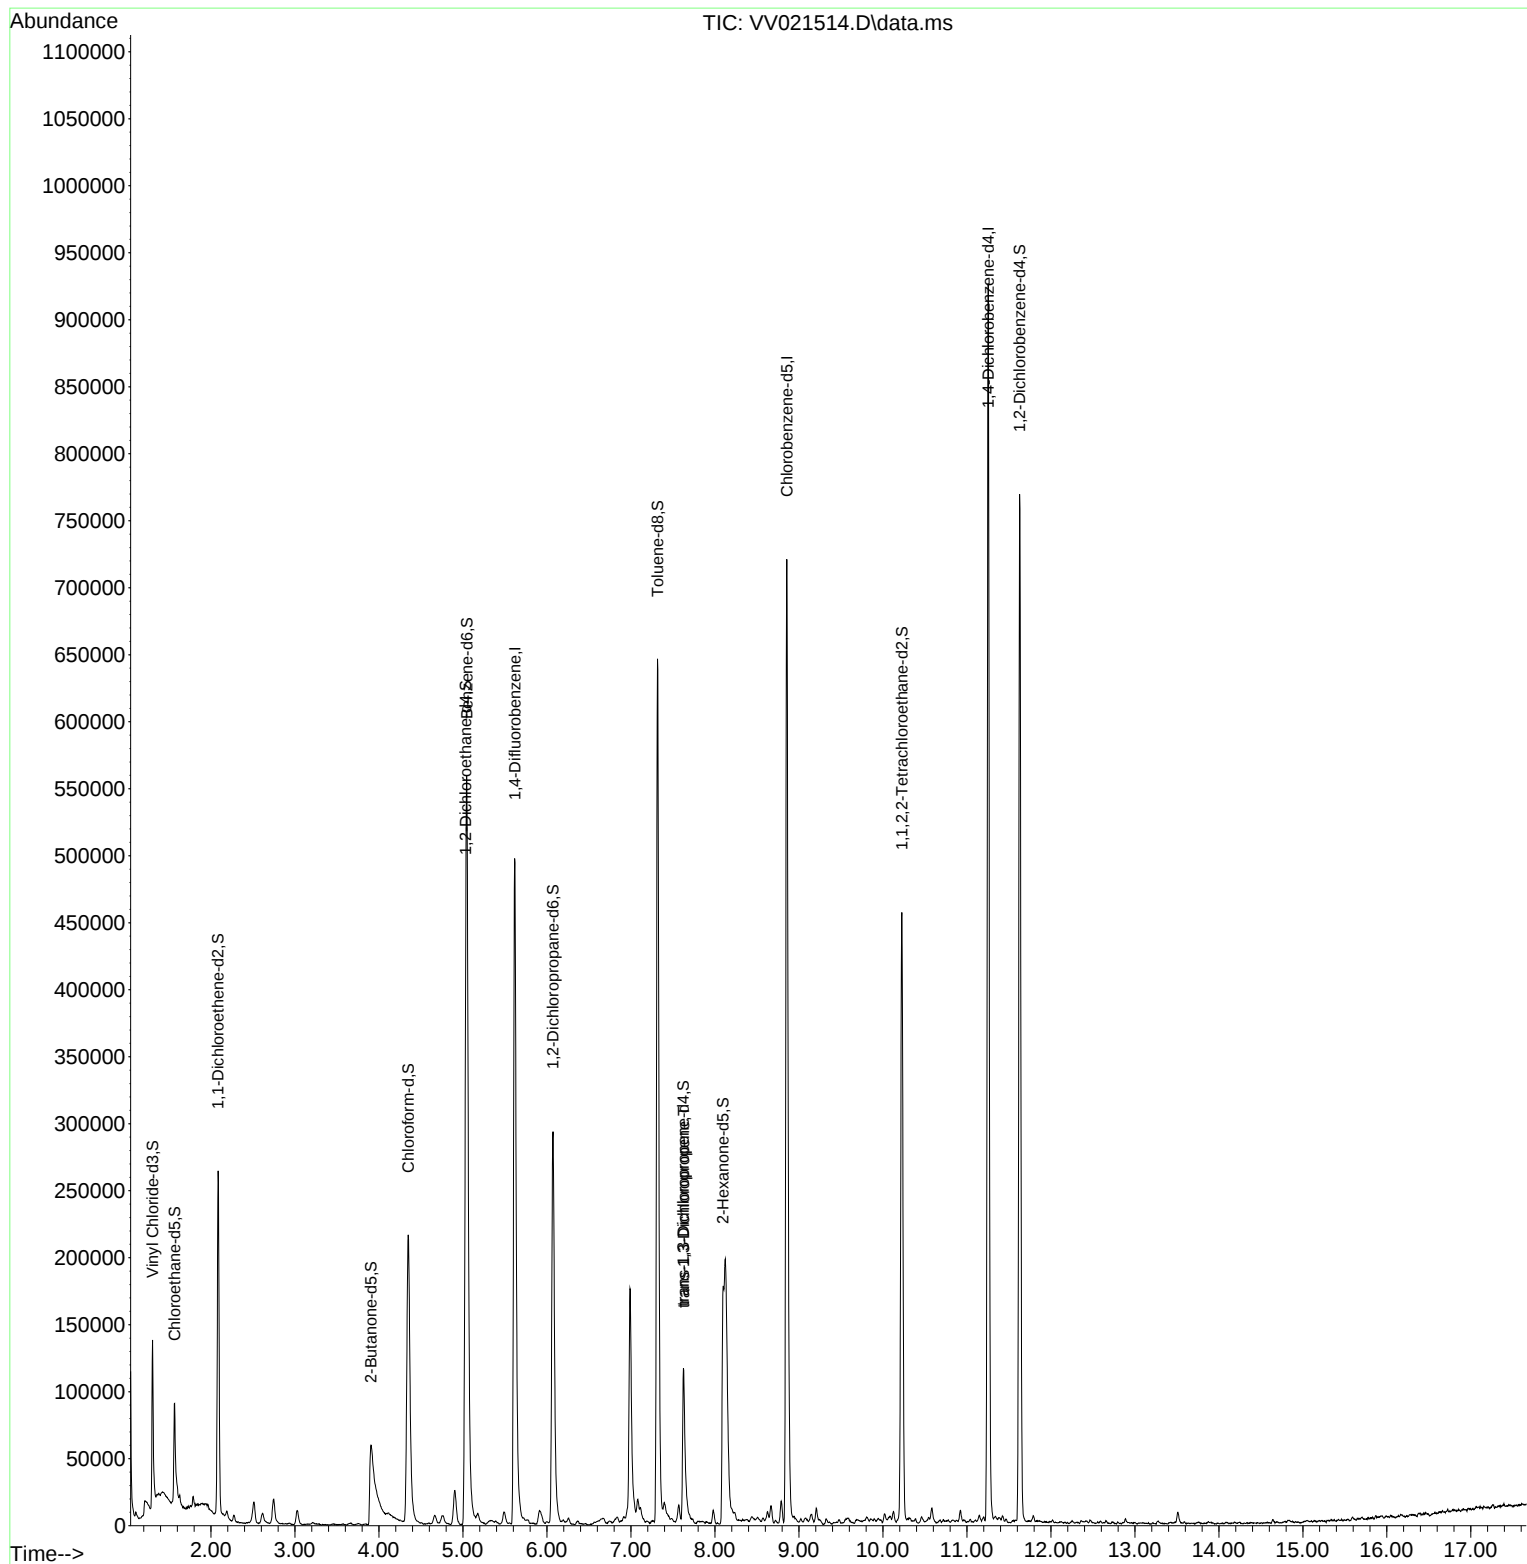

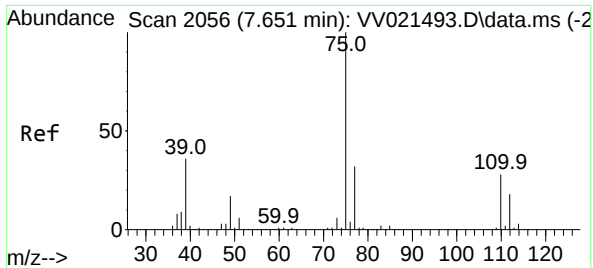

#44
 trans-1,3-Dichloropropene
 Concen: 0.637 ug/L
 RT: 7.628 min Scan# 2049
 Delta R.T. -0.023 min
 Lab File: VV021514.D
 Acq: 04 Jun 2021 18:04

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 3556
 Ion Ratio Lower Upper
 75 100
 77 52.8 22.9 42.5#

