

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021495.D
 Acq On : 04 Jun 2021 10:22
 Operator : SY/MD
 Sample : VV0604WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK186

Quant Time: Jun 05 03:57:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 05 03:34:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	470861	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	439929	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	247567	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	130212	42.003	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	84.000%		
7) Chloroethane-d5	1.568	69	108030	46.845	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.700%		
11) 1,1-Dichloroethene-d2	2.108	63	174850	33.008	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.020%		
21) 2-Butanone-d5	3.892	46	240791	108.318	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	108.320%		
24) Chloroform-d	4.352	84	285688	46.294	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.580%		
26) 1,2-Dichloroethane-d4	5.034	65	174105	48.982	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.960%		
32) Benzene-d6	5.053	84	585129	47.544	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.080%		
36) 1,2-Dichloropropane-d6	6.072	67	184990	48.673	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.340%		
41) Toluene-d8	7.317	98	553986	47.247	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.500%		
43) trans-1,3-Dichloroprop...	7.625	79	95661	47.032	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.060%		
47) 2-Hexanone-d5	8.092	63	174903	100.221	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	100.220%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	266764	50.564	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	101.120%		
66) 1,2-Dichlorobenzene-d4	11.625	152	249596	48.500	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.000%		
Target Compounds						Qvalue
46) Tetrachloroethene	7.982	164	3199	1.017	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021495.D
Acq On : 04 Jun 2021 10:22
Operator : SY/MD
Sample : VV0604WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK186

Quant Time: Jun 05 03:57:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 05 03:34:55 2021
Response via : Initial Calibration

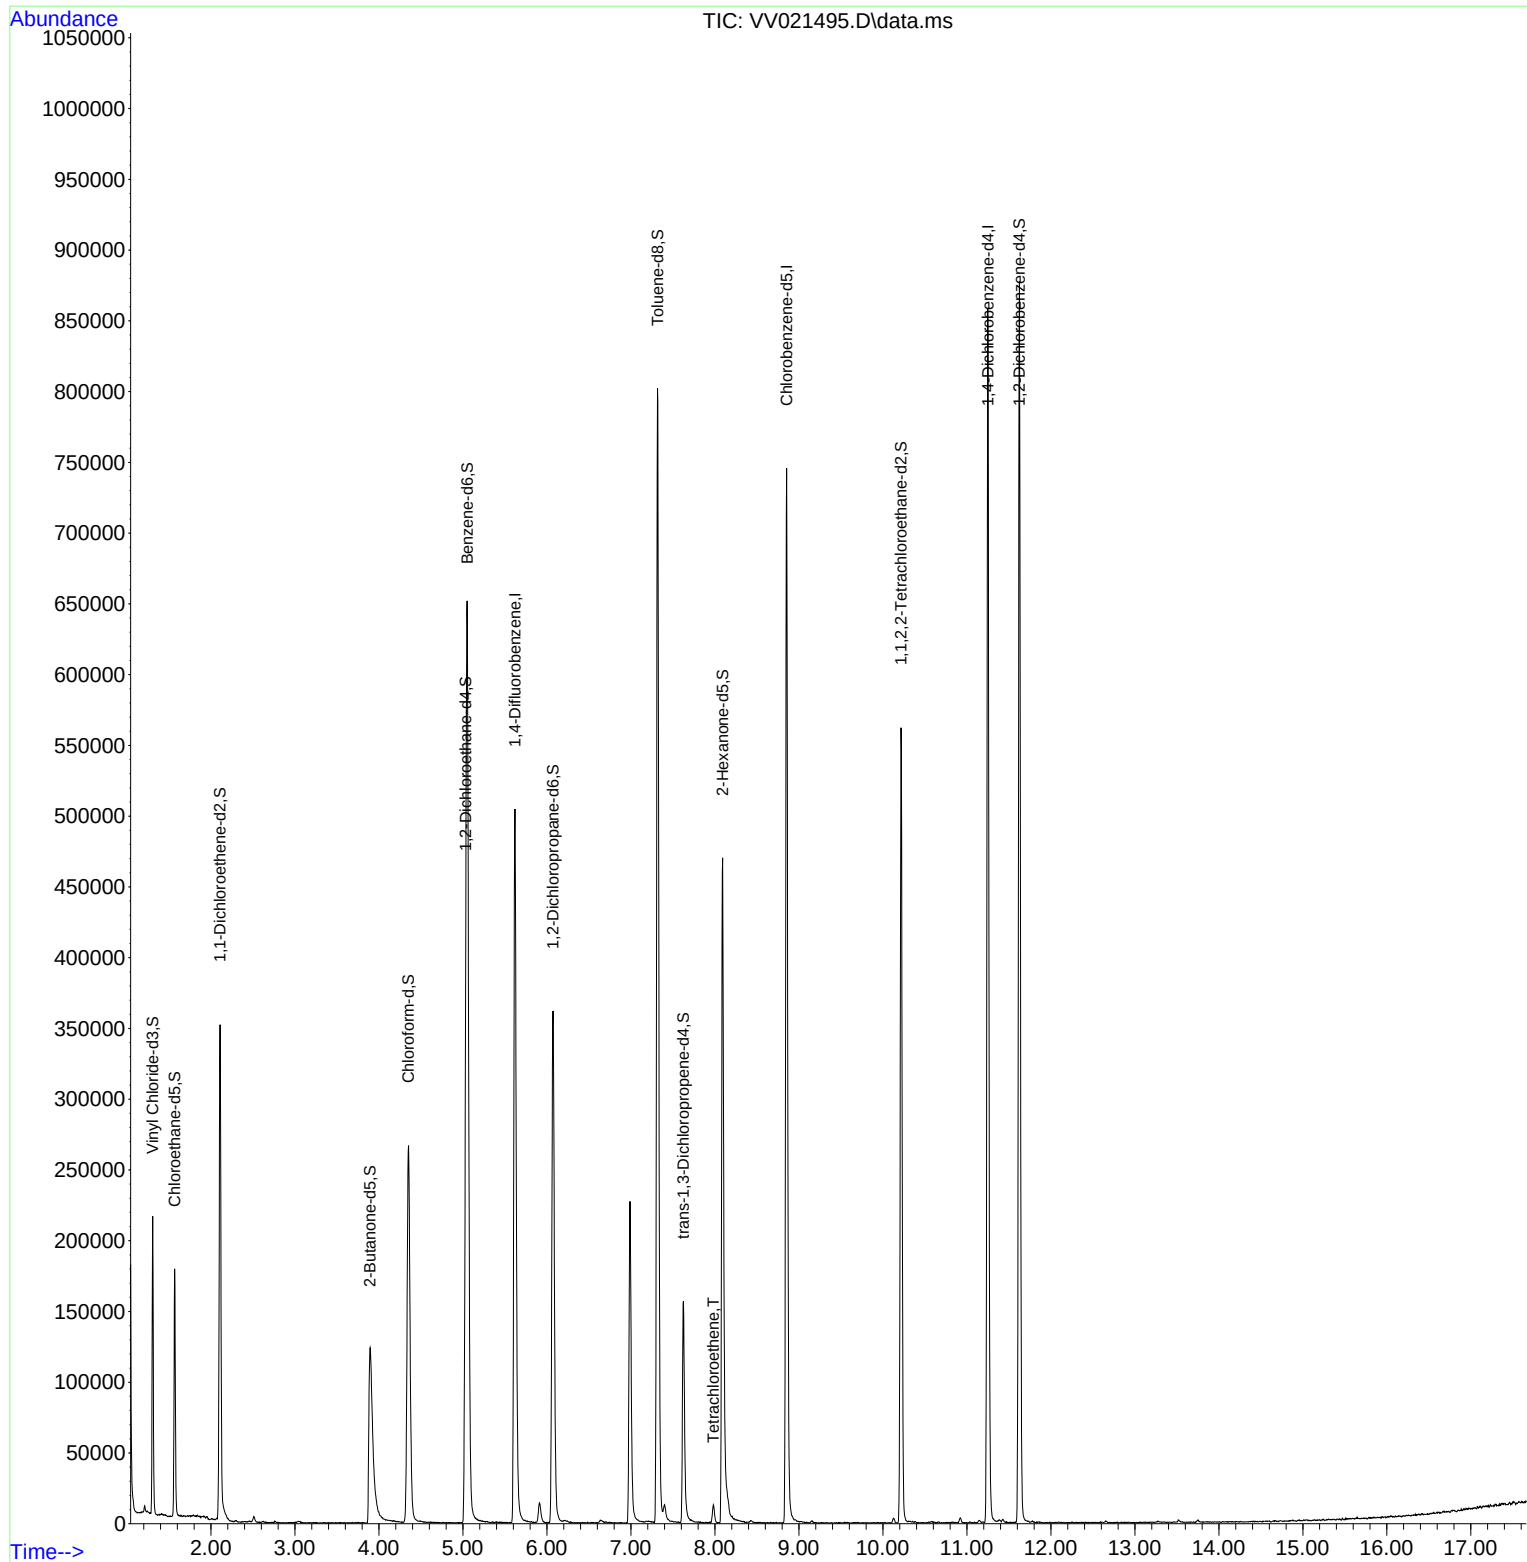

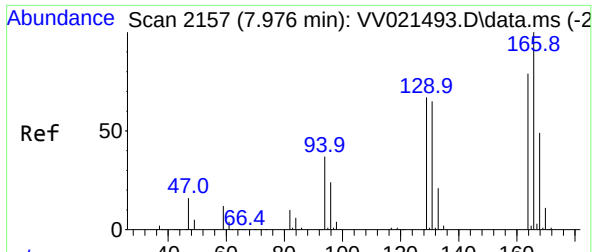

#46
Tetrachloroethene
Concen: 1.017 ug/L
RT: 7.982 min Scan# 2159
Delta R.T. 0.006 min
Lab File: VV021495.D
Acq: 04 Jun 2021 10:22

Instrument :
MSVOA_V
ClientSampleId :
VBLK186

Tgt Ion:164 Resp: 3199

Ion	Ratio	Lower	Upper
164	100		
129	85.0	60.5	112.3
131	74.2	58.7	108.9
166	123.7	88.1	163.5

