

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021495.D
 Acq On : 04 Jun 2021 10:22
 Operator : SY/MD
 Sample : VV0604WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK186

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

Signal : TIC: VV021495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	210777	208521	12.64%	1.572%
2	1.568	157	164	176	rVB	174063	189531	11.49%	1.429%
3	2.108	322	332	360	rVB	349236	520949	31.58%	3.927%
4	2.677	505	509	510	rBV3	292	179	0.01%	0.001%
5	2.761	530	535	536	rBV3	1004	591	0.04%	0.004%
6	3.002	608	610	612	rBV2	440	209	0.01%	0.002%
7	3.047	615	624	627	rBV4	1031	1760	0.11%	0.013%
8	3.236	679	683	686	rBV3	220	170	0.01%	0.001%
9	3.452	744	750	753	rBV	250	245	0.01%	0.002%
10	3.593	791	794	796	rBV	357	185	0.01%	0.001%
11	3.609	796	799	804	rVV3	321	246	0.01%	0.002%
12	3.683	820	822	825	rVV2	346	198	0.01%	0.001%
13	3.719	829	833	837	rBV	380	356	0.02%	0.003%
14	3.770	845	849	853	rVB3	405	393	0.02%	0.003%
15	3.806	857	860	864	rBV3	354	309	0.02%	0.002%
16	3.896	877	888	932	rBV	123833	422745	25.62%	3.186%
17	4.352	1012	1030	1067	rBV	266100	660687	40.05%	4.980%
18	4.725	1144	1146	1152	rVB4	308	199	0.01%	0.001%
19	4.767	1153	1159	1161	rBV4	434	455	0.03%	0.003%
20	4.831	1174	1179	1180	rBV3	396	277	0.02%	0.002%
21	4.857	1184	1187	1191	rBV3	366	299	0.02%	0.002%
22	4.941	1210	1213	1217	rVB2	296	216	0.01%	0.002%
23	5.050	1230	1247	1278	rBV2	651229	1649800	100.00%	12.435%
24	5.391	1348	1353	1355	rBV4	506	428	0.03%	0.003%
25	5.439	1365	1368	1371	rVB3	471	285	0.02%	0.002%
26	5.478	1377	1380	1381	rBV	568	307	0.02%	0.002%
27	5.619	1411	1424	1458	rBV	504460	1016226	61.60%	7.660%
28	5.912	1505	1515	1529	rBV3	13539	28028	1.70%	0.211%
29	6.072	1552	1565	1598	rVV2	361471	745648	45.20%	5.620%
30	6.355	1651	1653	1656	rVB2	307	163	0.01%	0.001%
31	6.400	1664	1667	1672	rBV4	270	291	0.02%	0.002%
32	6.420	1672	1673	1676	rVB	301	154	0.01%	0.001%
33	6.484	1689	1693	1696	rBV2	617	392	0.02%	0.003%
34	6.529	1701	1707	1708	rBV3	370	288	0.02%	0.002%
35	6.741	1769	1773	1777	rBV3	500	488	0.03%	0.004%
36	6.809	1792	1794	1799	rBV2	351	220	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021495.D
 Acq On : 04 Jun 2021 10:22
 Operator : SY/MD
 Sample : VV0604WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK186

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.883	1813	1817	1823	rBV3	374	376	0.02%	0.003%
38	6.989	1837	1850	1880	rBV	227347	419159	25.41%	3.159%
39	7.317	1940	1952	1971	rBV	801323	1394875	84.55%	10.514%
40	7.625	2037	2048	2073	rBV	156480	277961	16.85%	2.095%
41	7.857	2118	2120	2124	rBV2	403	223	0.01%	0.002%
42	7.889	2128	2130	2134	rVB3	571	383	0.02%	0.003%
43	7.934	2142	2144	2145	rBV	427	190	0.01%	0.001%
44	7.982	2150	2159	2173	rVB3	12854	22680	1.37%	0.171%
45	8.037	2173	2176	2182	rBV3	439	459	0.03%	0.003%
46	8.092	2182	2193	2227	rBV	469975	859299	52.09%	6.477%
47	8.574	2341	2343	2347	rVB2	320	219	0.01%	0.002%
48	8.600	2347	2351	2354	rVB	377	276	0.02%	0.002%
49	8.625	2354	2359	2361	rBV3	521	368	0.02%	0.003%
50	8.664	2368	2371	2373	rBV2	489	271	0.02%	0.002%
51	8.703	2380	2383	2385	rVB2	356	185	0.01%	0.001%
52	8.731	2385	2392	2394	rBV2	523	382	0.02%	0.003%
53	8.776	2403	2406	2408	rVB2	265	148	0.01%	0.001%
54	8.799	2411	2413	2416	rVB	279	159	0.01%	0.001%
55	8.854	2416	2430	2458	rBV	745247	1216962	73.76%	9.173%
56	9.069	2495	2497	2499	rVB	456	186	0.01%	0.001%
57	9.149	2514	2522	2524	rBV2	1350	1411	0.09%	0.011%
58	9.204	2536	2539	2543	rVB	382	273	0.02%	0.002%
59	9.272	2559	2560	2563	rBV	263	146	0.01%	0.001%
60	9.426	2605	2608	2611	rBV	225	172	0.01%	0.001%
61	9.452	2611	2616	2618	rVB3	341	277	0.02%	0.002%
62	9.545	2641	2645	2649	rBV3	561	534	0.03%	0.004%
63	9.899	2753	2755	2762	rVB	285	223	0.01%	0.002%
64	9.944	2762	2769	2774	rVB4	578	851	0.05%	0.006%
65	9.973	2774	2778	2782	rBV3	378	352	0.02%	0.003%
66	9.998	2782	2786	2790	rBV2	261	204	0.01%	0.002%
67	10.024	2790	2794	2801	rVB2	470	462	0.03%	0.003%
68	10.063	2802	2806	2807	rBV2	244	160	0.01%	0.001%
69	10.088	2812	2814	2817	rVB	344	152	0.01%	0.001%
70	10.124	2817	2825	2840	rBV4	3364	5780	0.35%	0.044%
71	10.217	2841	2854	2879	rBV	561916	876966	53.16%	6.610%
72	10.381	2902	2905	2912	rVB5	897	1035	0.06%	0.008%
73	10.423	2916	2918	2921	rBV2	377	200	0.01%	0.002%
74	10.526	2948	2950	2952	rBV2	288	139	0.01%	0.001%
75	10.548	2953	2957	2961	rVV3	540	443	0.03%	0.003%
76	10.638	2982	2985	2988	rBV2	311	202	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021495.D
 Acq On : 04 Jun 2021 10:22
 Operator : SY/MD
 Sample : VV0604WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK186

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

77	10.664	2988	2993	2999	rVV4	797	942	0.06%	0.007%
78	10.719	3006	3010	3015	rBV3	262	241	0.01%	0.002%
79	10.773	3025	3027	3029	rBV	338	155	0.01%	0.001%
80	10.799	3032	3035	3037	rBV3	274	189	0.01%	0.001%
81	10.834	3042	3046	3049	rBV3	562	477	0.03%	0.004%
82	10.921	3066	3073	3084	rVB6	3549	5709	0.35%	0.043%
83	10.976	3088	3090	3092	rVB	377	153	0.01%	0.001%
84	10.995	3092	3096	3099	rBV	393	287	0.02%	0.002%
85	11.091	3123	3126	3129	rBV2	499	364	0.02%	0.003%
86	11.143	3134	3142	3151	rBV3	1721	3048	0.18%	0.023%
87	11.249	3163	3175	3195	rBV	857372	1331431	80.70%	10.036%
88	11.519	3258	3259	3263	rBV2	400	282	0.02%	0.002%
89	11.571	3272	3275	3276	rBV	408	254	0.02%	0.002%
90	11.625	3280	3292	3314	rVV	876753	1383168	83.84%	10.426%
91	11.989	3403	3405	3412	rVB4	478	428	0.03%	0.003%
92	12.059	3424	3427	3430	rVB2	499	268	0.02%	0.002%
93	12.297	3499	3501	3502	rBV	333	138	0.01%	0.001%
94	12.416	3536	3538	3540	rBV2	401	232	0.01%	0.002%
95	12.577	3586	3588	3590	rBV	310	141	0.01%	0.001%
96	12.590	3590	3592	3596	rVV3	571	363	0.02%	0.003%
97	12.754	3640	3643	3644	rBV3	469	268	0.02%	0.002%
98	12.821	3662	3664	3666	rBV	341	204	0.01%	0.002%
99	13.178	3773	3775	3779	rBV	399	287	0.02%	0.002%
100	13.516	3877	3880	3890	rVB6	1511	1920	0.12%	0.014%




Sum of corrected areas: 13267130

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021495.D
Acq On : 04 Jun 2021 10:22
Operator : SY/MD
Sample : VV0604WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK186

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

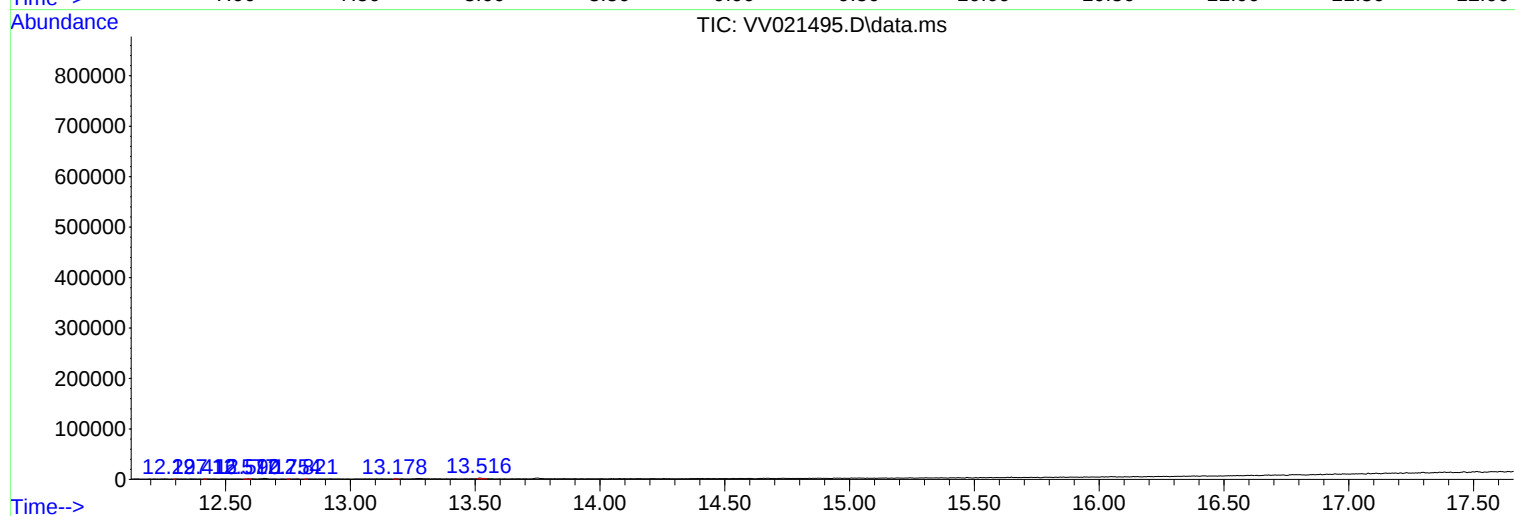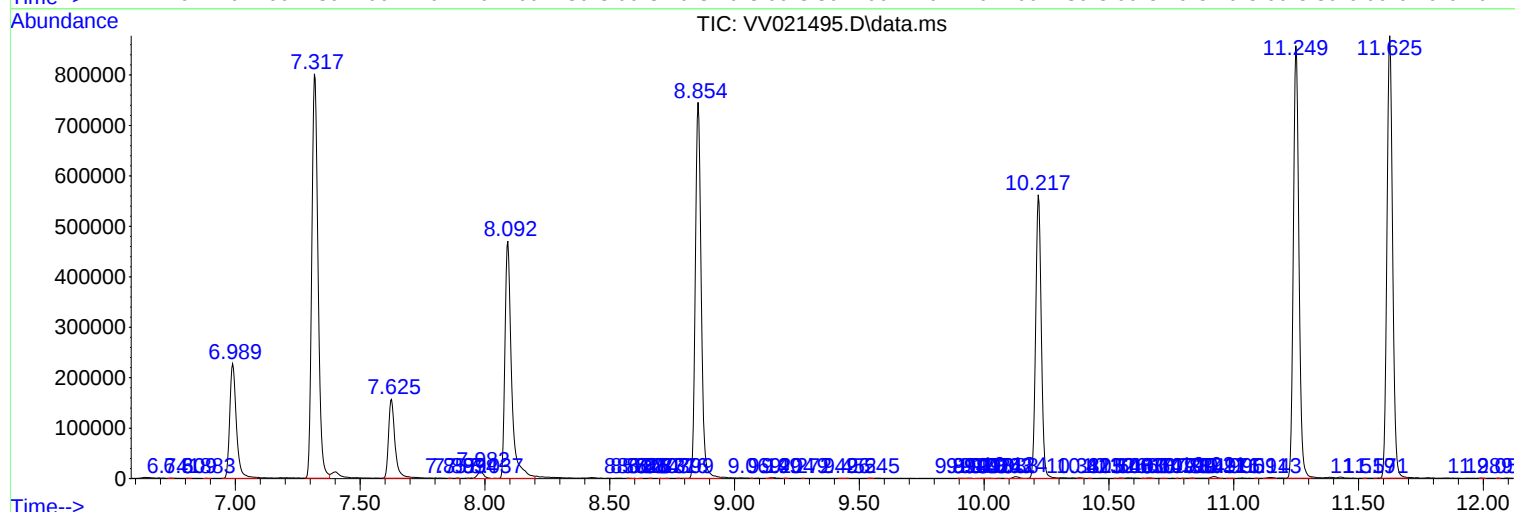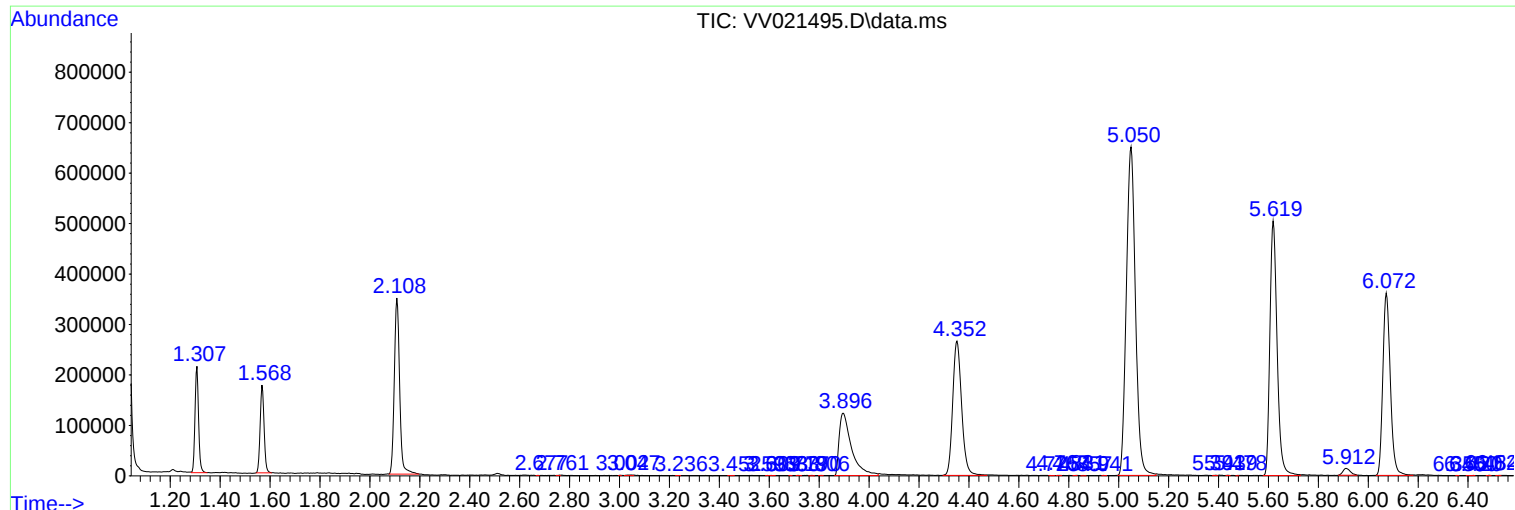

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021495.D
Acq On : 04 Jun 2021 10:22
Operator : SY/MD
Sample : VV0604WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK186

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021495.D
Acq On : 04 Jun 2021 10:22
Operator : SY/MD
Sample : VV0604WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK186

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
