

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021497.D
 Acq On : 04 Jun 2021 11:10
 Operator : SY/MD
 Sample : M2605-05DL2 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K1DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	185687	189529	7.75%	1.206%
2	1.568	157	164	176	rVB	155128	176385	7.21%	1.122%
3	2.108	322	332	370	rVB	323088	492875	20.15%	3.136%
4	2.671	505	507	512	rBV2	358	311	0.01%	0.002%
5	2.722	521	523	526	rVB	481	265	0.01%	0.002%
6	2.757	531	534	535	rBV	333	210	0.01%	0.001%
7	2.835	556	558	561	rBV2	258	192	0.01%	0.001%
8	2.960	594	597	599	rBV2	291	143	0.01%	0.001%
9	2.976	599	602	604	rBV2	313	216	0.01%	0.001%
10	3.044	618	623	625	rBV5	808	877	0.04%	0.006%
11	3.089	633	637	643	rVB3	355	300	0.01%	0.002%
12	3.317	705	708	712	rBV3	242	209	0.01%	0.001%
13	3.336	712	714	716	rBV2	269	148	0.01%	0.001%
14	3.401	730	734	736	rBV2	374	242	0.01%	0.002%
15	3.478	755	758	761	rVB2	270	158	0.01%	0.001%
16	3.658	808	814	816	rBV2	454	304	0.01%	0.002%
17	3.703	823	828	832	rBV2	227	233	0.01%	0.001%
18	3.754	842	844	846	rBV	312	169	0.01%	0.001%
19	3.790	854	855	860	rVB2	350	174	0.01%	0.001%
20	3.818	861	864	866	rBV2	302	145	0.01%	0.001%
21	3.896	876	888	936	rBV	125606	427091	17.46%	2.717%
22	4.352	1015	1030	1060	rVB	254087	627651	25.66%	3.993%
23	4.725	1144	1146	1149	rBV2	294	231	0.01%	0.001%
24	4.745	1150	1152	1156	rVV2	754	460	0.02%	0.003%
25	4.831	1177	1179	1181	rVB2	339	168	0.01%	0.001%
26	4.844	1181	1183	1185	rBV	284	132	0.01%	0.001%
27	4.989	1224	1228	1229	rBV2	303	209	0.01%	0.001%
28	5.050	1229	1247	1282	rVV2	626255	1597007	65.28%	10.161%
29	5.323	1330	1332	1338	rBV4	512	493	0.02%	0.003%
30	5.404	1355	1357	1359	rBV2	482	237	0.01%	0.002%
31	5.478	1377	1380	1381	rBV2	257	127	0.01%	0.001%
32	5.487	1381	1383	1385	rVB	415	211	0.01%	0.001%
33	5.619	1412	1424	1450	rVV	509195	1020438	41.71%	6.492%
34	5.815	1483	1485	1488	rVB2	405	118	0.00%	0.001%
35	5.918	1503	1517	1544	rBV3	175165	366418	14.98%	2.331%
36	6.072	1552	1565	1593	rBV	349995	705510	28.84%	4.489%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021497.D
 Acq On : 04 Jun 2021 11:10
 Operator : SY/MD
 Sample : M2605-05DL2 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K1DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.355	1651	1653	1656	rBV	247	137	0.01%	0.001%
38	6.381	1656	1661	1663	rBV2	374	318	0.01%	0.002%
39	6.445	1679	1681	1683	rBV	288	119	0.00%	0.001%
40	6.481	1691	1692	1695	rVV2	315	136	0.01%	0.001%
41	6.523	1703	1705	1710	rVB3	284	156	0.01%	0.001%
42	6.642	1734	1742	1744	rBV5	1610	2155	0.09%	0.014%
43	6.715	1764	1765	1769	rBV3	418	172	0.01%	0.001%
44	6.799	1788	1791	1793	rBV2	213	149	0.01%	0.001%
45	6.812	1793	1795	1799	rVB3	406	232	0.01%	0.001%
46	6.857	1807	1809	1813	rBV2	334	196	0.01%	0.001%
47	6.876	1813	1815	1819	rVB2	289	169	0.01%	0.001%
48	6.989	1839	1850	1882	rBV	220802	399869	16.34%	2.544%
49	7.317	1941	1952	1971	rBV	770965	1349638	55.17%	8.587%
50	7.625	2037	2048	2071	rBV	148900	263015	10.75%	1.673%
51	7.908	2133	2136	2139	rVB3	308	204	0.01%	0.001%
52	7.979	2139	2158	2182	rBV	1461538	2446455	100.00%	15.565%
53	8.088	2183	2192	2233	rVB	461576	839521	34.32%	5.341%
54	8.429	2292	2298	2308	rVB5	1237	1926	0.08%	0.012%
55	8.532	2328	2330	2333	rBV	319	147	0.01%	0.001%
56	8.619	2355	2357	2361	rVB	264	171	0.01%	0.001%
57	8.674	2371	2374	2376	rBV2	231	193	0.01%	0.001%
58	8.728	2389	2391	2395	rBV3	364	222	0.01%	0.001%
59	8.748	2395	2397	2398	rBV	268	131	0.01%	0.001%
60	8.799	2410	2413	2417	rVB2	289	207	0.01%	0.001%
61	8.854	2417	2430	2457	rBV	755857	1225432	50.09%	7.797%
62	9.153	2515	2523	2531	rBV7	1558	2595	0.11%	0.017%
63	9.227	2543	2546	2547	rBV	244	128	0.01%	0.001%
64	9.236	2547	2549	2551	rVB	366	119	0.00%	0.001%
65	9.256	2551	2555	2557	rBV2	190	143	0.01%	0.001%
66	9.288	2563	2565	2567	rVB	288	119	0.00%	0.001%
67	9.304	2567	2570	2572	rBV	314	195	0.01%	0.001%
68	9.645	2669	2676	2679	rBV2	227	328	0.01%	0.002%
69	9.735	2701	2704	2705	rBV2	229	127	0.01%	0.001%
70	9.796	2720	2723	2724	rBV	203	115	0.00%	0.001%
71	9.834	2731	2735	2737	rBV	227	147	0.01%	0.001%
72	9.866	2741	2745	2746	rBV	253	178	0.01%	0.001%
73	10.092	2813	2815	2818	rVV2	430	262	0.01%	0.002%
74	10.130	2818	2827	2837	rVB4	3743	5813	0.24%	0.037%
75	10.217	2842	2854	2876	rBV	543811	852747	34.86%	5.426%
76	10.413	2913	2915	2916	rBV	210	115	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021497.D
 Acq On : 04 Jun 2021 11:10
 Operator : SY/MD
 Sample : M2605-05DL2 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K1DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	10.545	2954	2956	2957	rBV	372	125	0.01%	0.001%
78	10.657	2986	2991	2996	rBV6	708	650	0.03%	0.004%
79	10.715	3006	3009	3011	rBV2	217	138	0.01%	0.001%
80	10.744	3015	3018	3020	rVV	497	282	0.01%	0.002%
81	10.805	3035	3037	3041	rBV3	390	273	0.01%	0.002%
82	10.828	3041	3044	3047	rBV4	304	266	0.01%	0.002%
83	10.921	3064	3073	3081	rVB8	3773	5405	0.22%	0.034%
84	11.079	3120	3122	3125	rBV2	258	196	0.01%	0.001%
85	11.146	3136	3143	3153	rBV5	1967	2994	0.12%	0.019%
86	11.188	3153	3156	3157	rBV	346	223	0.01%	0.001%
87	11.249	3164	3175	3196	rBV	880062	1350449	55.20%	8.592%
88	11.529	3260	3262	3264	rBV3	312	164	0.01%	0.001%
89	11.625	3279	3292	3314	rBV	848958	1348670	55.13%	8.581%
90	12.008	3408	3411	3413	rBV	549	280	0.01%	0.002%
91	12.182	3462	3465	3469	rBV2	440	320	0.01%	0.002%
92	12.201	3469	3471	3475	rVV	372	232	0.01%	0.001%
93	12.477	3556	3557	3562	rVB	656	280	0.01%	0.002%
94	12.503	3562	3565	3567	rBV	367	200	0.01%	0.001%
95	12.526	3570	3572	3576	rVB3	261	137	0.01%	0.001%
96	12.548	3576	3579	3581	rBV	447	233	0.01%	0.001%
97	12.599	3590	3595	3598	rBV2	670	692	0.03%	0.004%
98	12.699	3623	3626	3629	rBV3	300	237	0.01%	0.002%
99	12.757	3639	3644	3648	rBV2	523	363	0.01%	0.002%
100	12.921	3689	3695	3698	rBV2	626	624	0.03%	0.004%




Sum of corrected areas: 15717220

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021497.D
Acq On : 04 Jun 2021 11:10
Operator : SY/MD
Sample : M2605-05DL2 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K1DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

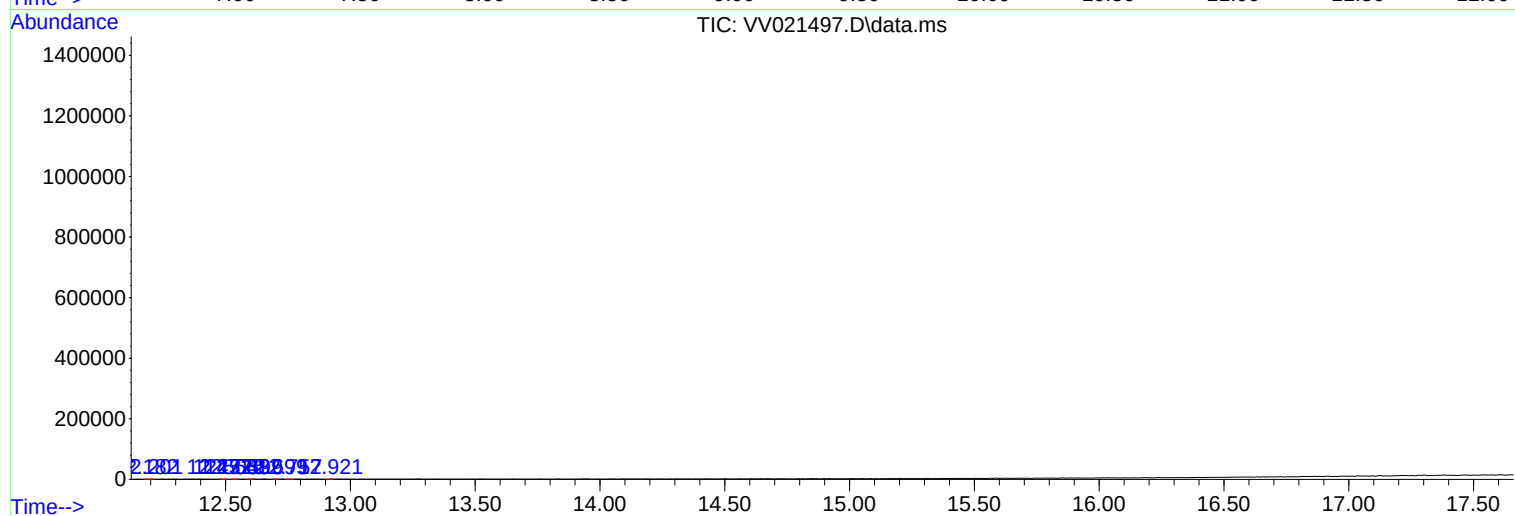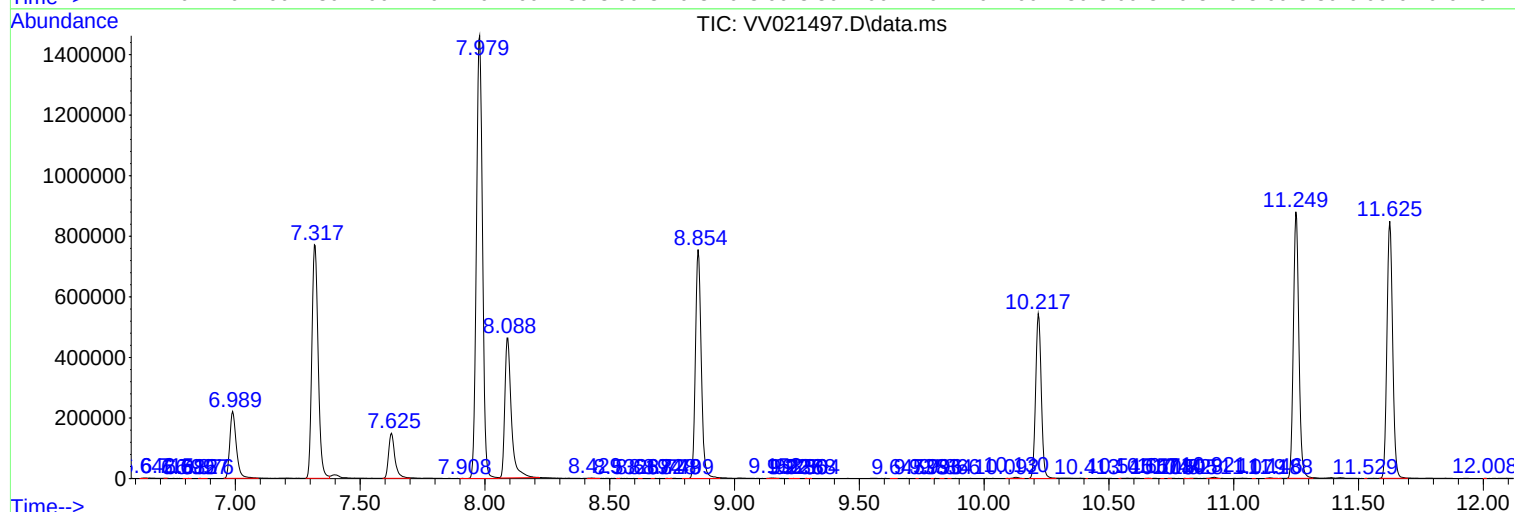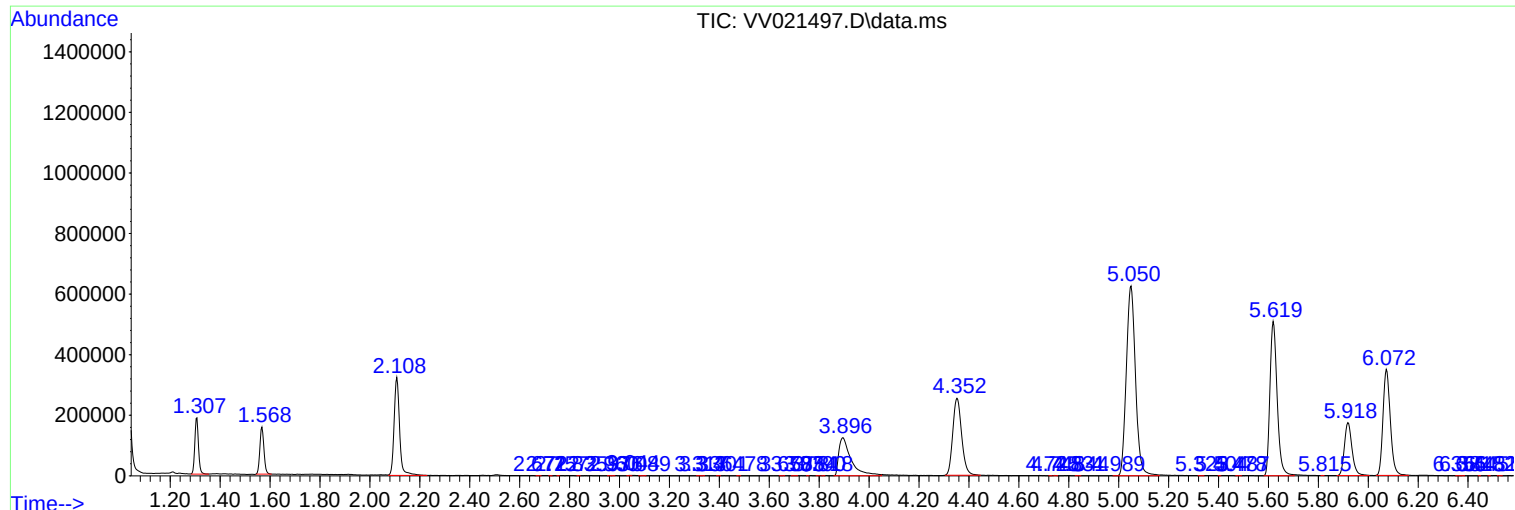

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021497.D
Acq On : 04 Jun 2021 11:10
Operator : SY/MD
Sample : M2605-05DL2 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K1DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021497.D
Acq On : 04 Jun 2021 11:10
Operator : SY/MD
Sample : M2605-05DL2 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K1DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
