

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021500.D
 Acq On : 04 Jun 2021 12:33
 Operator : SY/MD
 Sample : M2605-05DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

Signal : TIC: VV021500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	182068	183543	1.46%	0.676%
2	1.568	157	164	177	rVB	156574	176118	1.40%	0.649%
3	2.105	321	331	352	rBV	318999	477851	3.80%	1.761%
4	2.577	476	478	483	rVB4	455	214	0.00%	0.001%
5	2.613	483	489	493	rBV4	848	1139	0.01%	0.004%
6	2.661	501	504	507	rBV3	318	226	0.00%	0.001%
7	2.716	519	521	524	rVB2	395	192	0.00%	0.001%
8	2.841	557	560	564	rVB	587	330	0.00%	0.001%
9	2.921	582	585	588	rBV3	629	444	0.00%	0.002%
10	2.998	605	609	611	rBV2	274	193	0.00%	0.001%
11	3.037	611	621	635	rVV6	5721	12859	0.10%	0.047%
12	3.127	646	649	651	rBV	290	158	0.00%	0.001%
13	3.153	654	657	661	rVV3	385	269	0.00%	0.001%
14	3.175	661	664	666	rVB2	289	168	0.00%	0.001%
15	3.259	688	690	693	rVB2	498	257	0.00%	0.001%
16	3.330	711	712	717	rVB2	247	206	0.00%	0.001%
17	3.365	721	723	728	rBV2	220	136	0.00%	0.001%
18	3.429	738	743	747	rVB3	280	331	0.00%	0.001%
19	3.462	750	753	755	rBV3	225	179	0.00%	0.001%
20	3.593	789	794	795	rBV	286	219	0.00%	0.001%
21	3.661	811	815	817	rVV2	191	126	0.00%	0.000%
22	3.818	861	864	866	rBV	252	160	0.00%	0.001%
23	3.831	866	868	872	rVB2	281	131	0.00%	0.000%
24	3.892	876	887	909	rBV	112371	370815	2.95%	1.366%
25	4.349	1014	1029	1055	rBV	255019	627001	4.99%	2.310%
26	4.757	1153	1156	1159	rBV3	341	287	0.00%	0.001%
27	4.867	1188	1190	1196	rBV2	296	221	0.00%	0.001%
28	4.960	1215	1219	1223	rBV2	393	301	0.00%	0.001%
29	4.979	1223	1225	1228	rBV	309	243	0.00%	0.001%
30	5.047	1228	1246	1280	rBV2	606741	1569948	12.49%	5.785%
31	5.484	1379	1382	1386	rBV2	550	455	0.00%	0.002%
32	5.532	1395	1397	1400	rVB	512	193	0.00%	0.001%
33	5.551	1400	1403	1406	rBV2	228	162	0.00%	0.001%
34	5.616	1410	1423	1453	rBV	521444	1054156	8.39%	3.884%
35	5.912	1501	1515	1549	rBV	893783	1760223	14.00%	6.486%
36	6.069	1552	1564	1590	rVB	343784	696996	5.54%	2.568%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021500.D
 Acq On : 04 Jun 2021 12:33
 Operator : SY/MD
 Sample : M2605-05DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

37	6.307	1636	1638	1641	rVB	297	127	0.00%	0.000%
38	6.449	1680	1682	1685	rBV2	299	177	0.00%	0.001%
39	6.519	1700	1704	1705	rBV2	197	174	0.00%	0.001%
40	6.551	1712	1714	1720	rBV3	296	285	0.00%	0.001%
41	6.584	1723	1724	1728	rVB2	420	133	0.00%	0.000%
42	6.641	1733	1742	1744	rBV5	1407	2128	0.02%	0.008%
43	6.709	1762	1763	1767	rVB2	654	330	0.00%	0.001%
44	6.741	1771	1773	1775	rVB	302	137	0.00%	0.001%
45	6.764	1778	1780	1783	rBV	331	175	0.00%	0.001%
46	6.783	1783	1786	1787	rBV2	312	161	0.00%	0.001%
47	6.838	1800	1803	1804	rVB	296	146	0.00%	0.001%
48	6.924	1825	1830	1833	rBV2	263	180	0.00%	0.001%
49	6.985	1838	1849	1883	rBV	218508	399832	3.18%	1.473%
50	7.317	1940	1952	1970	rBV	758817	1325128	10.54%	4.883%
51	7.622	2036	2047	2080	rBV	147977	263982	2.10%	0.973%
52	7.863	2119	2122	2123	rBV	354	183	0.00%	0.001%
53	7.976	2139	2157	2183	rVV	7505690	12569949	100.00%	46.316%
54	8.088	2183	2192	2233	rVB	429396	786171	6.25%	2.897%
55	8.442	2300	2302	2303	rBV	293	151	0.00%	0.001%
56	8.503	2320	2321	2326	rVB	411	185	0.00%	0.001%
57	8.622	2355	2358	2362	rBV	545	496	0.00%	0.002%
58	8.661	2368	2370	2374	rBV2	400	290	0.00%	0.001%
59	8.712	2385	2386	2388	rBV	339	124	0.00%	0.000%
60	8.741	2393	2395	2399	rVB2	325	212	0.00%	0.001%
61	8.854	2417	2430	2458	rBV	761861	1256797	10.00%	4.631%
62	9.088	2501	2503	2504	rVB	460	134	0.00%	0.000%
63	9.146	2513	2521	2525	rBV5	2280	3141	0.02%	0.012%
64	9.220	2536	2544	2546	rBV3	456	496	0.00%	0.002%
65	9.426	2605	2608	2611	rBV	342	206	0.00%	0.001%
66	9.442	2611	2613	2616	rVB2	265	157	0.00%	0.001%
67	9.545	2640	2645	2648	rBV3	460	498	0.00%	0.002%
68	9.680	2682	2687	2690	rBV2	615	424	0.00%	0.002%
69	9.696	2690	2692	2698	rVB2	223	169	0.00%	0.001%
70	9.767	2707	2714	2715	rBV2	299	279	0.00%	0.001%
71	10.001	2783	2787	2789	rBV	309	208	0.00%	0.001%
72	10.018	2789	2792	2793	rBV2	402	207	0.00%	0.001%
73	10.030	2793	2796	2799	rVV2	425	322	0.00%	0.001%
74	10.072	2808	2809	2816	rVB	291	177	0.00%	0.001%
75	10.127	2816	2826	2835	rBV6	2873	5148	0.04%	0.019%
76	10.217	2841	2854	2875	rBV	512066	814134	6.48%	3.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021500.D
 Acq On : 04 Jun 2021 12:33
 Operator : SY/MD
 Sample : M2605-05DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	10.529	2948	2951	2952	rBV	341	174	0.00%	0.001%
78	10.571	2960	2964	2965	rBV2	794	595	0.00%	0.002%
79	10.696	2999	3003	3008	rBV3	308	377	0.00%	0.001%
80	10.731	3012	3014	3017	rBV	453	308	0.00%	0.001%
81	10.792	3030	3033	3034	rBV	258	144	0.00%	0.001%
82	10.876	3058	3059	3063	rBV3	476	315	0.00%	0.001%
83	10.918	3063	3072	3083	rVB5	3511	5894	0.05%	0.022%
84	11.034	3105	3108	3110	rBV3	505	420	0.00%	0.002%
85	11.198	3157	3159	3163	rBV	336	162	0.00%	0.001%
86	11.249	3163	3175	3204	rBV	919595	1418401	11.28%	5.226%
87	11.500	3251	3253	3256	rVB3	768	352	0.00%	0.001%
88	11.625	3279	3292	3315	rBV	834771	1339468	10.66%	4.935%
89	11.995	3404	3407	3409	rBV	208	131	0.00%	0.000%
90	12.053	3422	3425	3430	rBV3	338	381	0.00%	0.001%
91	12.082	3432	3434	3436	rBV2	656	270	0.00%	0.001%
92	12.162	3456	3459	3464	rVB2	240	160	0.00%	0.001%
93	12.355	3517	3519	3521	rBV2	344	194	0.00%	0.001%
94	12.545	3575	3578	3579	rBV	548	340	0.00%	0.001%
95	12.593	3590	3593	3595	rBV	606	359	0.00%	0.001%
96	12.664	3614	3615	3618	rBV2	284	167	0.00%	0.001%
97	12.779	3648	3651	3653	rBV2	322	218	0.00%	0.001%
98	12.969	3707	3710	3711	rBV	276	132	0.00%	0.000%
99	13.214	3782	3786	3790	rBV2	537	544	0.00%	0.002%
100	13.837	3976	3980	3985	rBV3	514	509	0.00%	0.002%




Sum of corrected areas: 27139818

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021500.D
Acq On : 04 Jun 2021 12:33
Operator : SY/MD
Sample : M2605-05DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

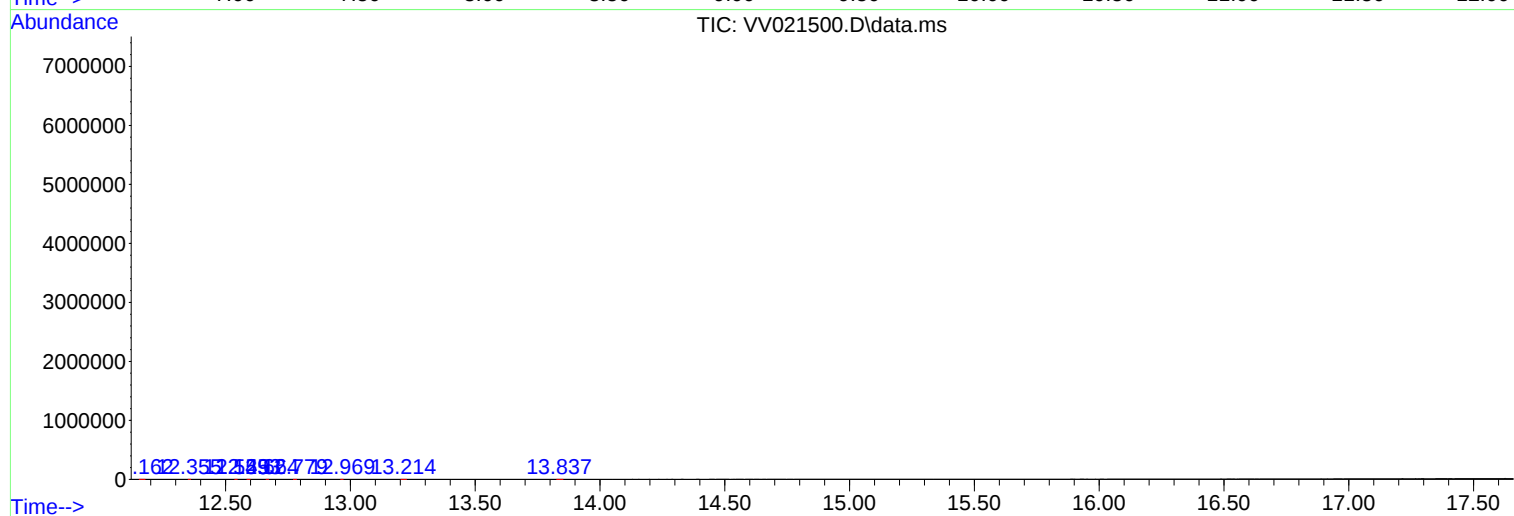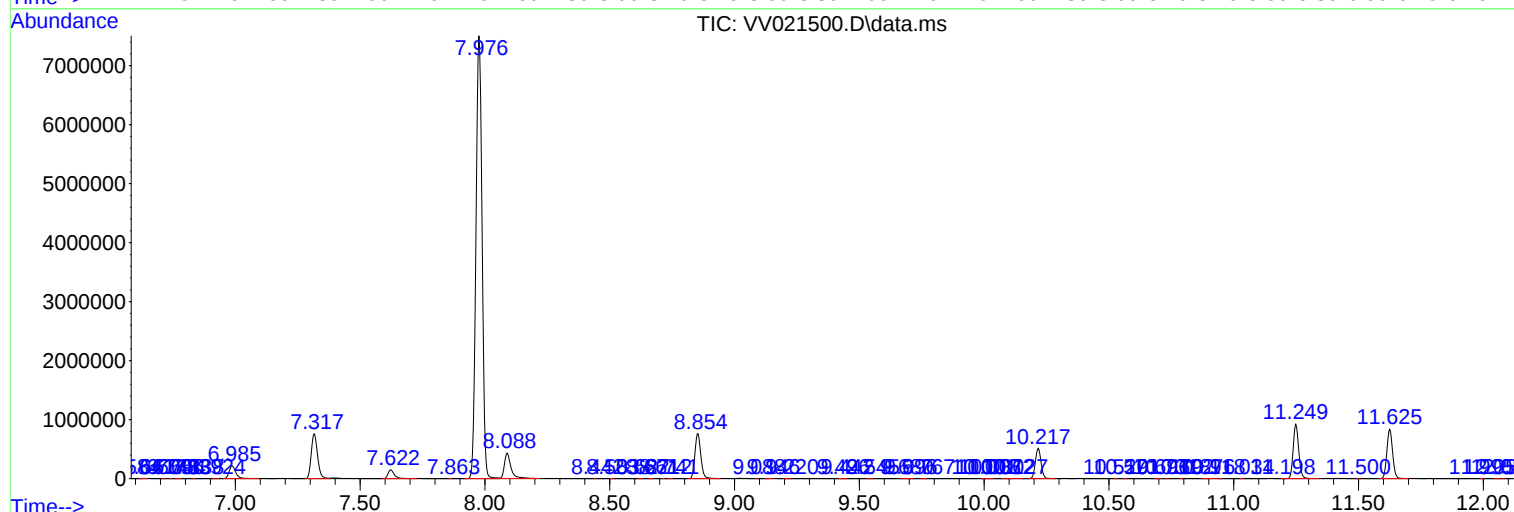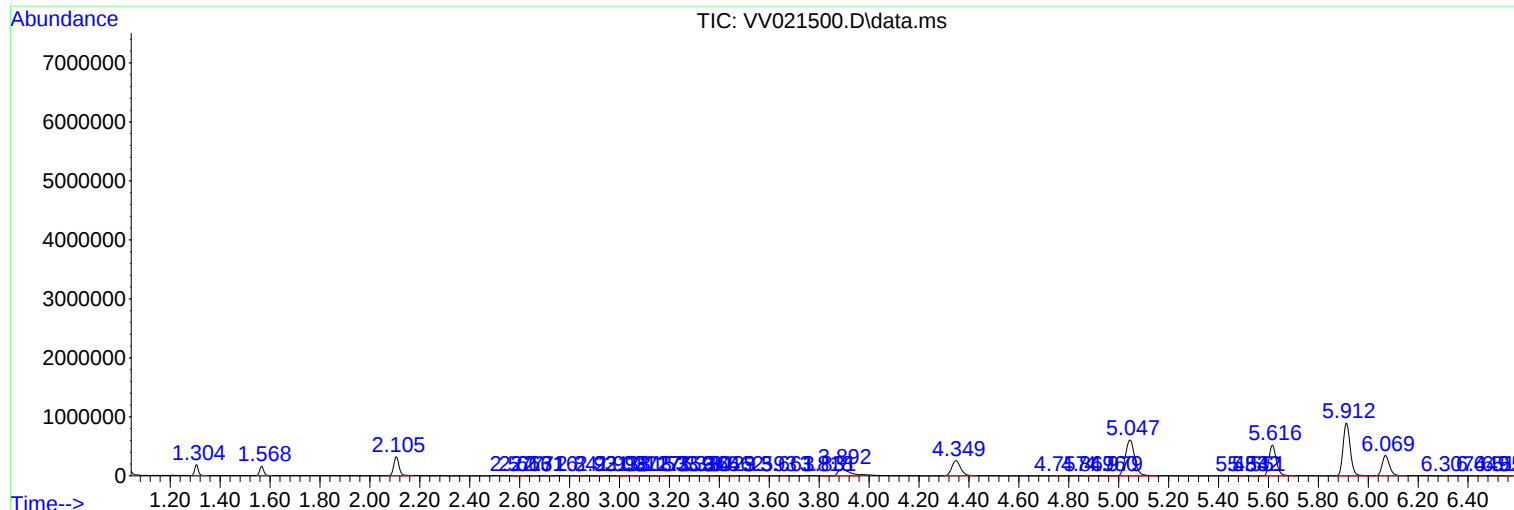

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021500.D
Acq On : 04 Jun 2021 12:33
Operator : SY/MD
Sample : M2605-05DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021500.D
Acq On : 04 Jun 2021 12:33
Operator : SY/MD
Sample : M2605-05DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
