

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021509.D
 Acq On : 04 Jun 2021 16:06
 Operator : SY/MD
 Sample : M2605-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021509.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	88	rBV	161341	161930	10.80%	1.222%
2	2.108	324	332	350	rVB	302416	446704	29.81%	3.370%
3	2.989	604	606	608	rBV	530	258	0.02%	0.002%
4	3.047	612	624	636	rBV7	4105	8811	0.59%	0.066%
5	3.166	657	661	664	rBV2	437	410	0.03%	0.003%
6	3.211	672	675	676	rBV	399	229	0.02%	0.002%
7	3.259	687	690	695	rVB2	574	347	0.02%	0.003%
8	3.285	695	698	700	rBV	443	263	0.02%	0.002%
9	3.343	714	716	719	rVB	441	219	0.01%	0.002%
10	3.368	722	724	729	rVB3	416	294	0.02%	0.002%
11	3.529	773	774	778	rBV2	250	159	0.01%	0.001%
12	3.593	790	794	797	rBV2	245	182	0.01%	0.001%
13	3.654	810	813	817	rVB2	444	309	0.02%	0.002%
14	3.677	817	820	823	rBV2	438	334	0.02%	0.003%
15	3.696	823	826	830	rBV2	276	159	0.01%	0.001%
16	3.716	830	832	833	rBV2	327	120	0.01%	0.001%
17	3.738	836	839	840	rBV3	571	311	0.02%	0.002%
18	3.892	875	887	907	rBV2	120846	378419	25.25%	2.855%
19	4.352	1015	1030	1054	rBV	247490	616961	41.17%	4.654%
20	4.696	1133	1137	1138	rBV	592	341	0.02%	0.003%
21	4.738	1142	1150	1152	rBV5	641	665	0.04%	0.005%
22	4.854	1183	1186	1189	rVB2	529	308	0.02%	0.002%
23	4.873	1189	1192	1193	rBV2	453	245	0.02%	0.002%
24	4.908	1202	1203	1204	rBV2	460	152	0.01%	0.001%
25	5.050	1228	1247	1285	rBV2	574505	1498660	100.00%	11.306%
26	5.526	1394	1395	1400	rBV3	464	347	0.02%	0.003%
27	5.619	1411	1424	1457	rVV	492957	997017	66.53%	7.522%
28	5.825	1486	1488	1491	rBV2	443	262	0.02%	0.002%
29	5.918	1504	1517	1545	rBV	239858	483558	32.27%	3.648%
30	6.072	1553	1565	1597	rVB	327168	664090	44.31%	5.010%
31	6.358	1652	1654	1656	rBV2	377	222	0.01%	0.002%
32	6.407	1664	1669	1670	rBV2	612	318	0.02%	0.002%
33	6.442	1677	1680	1681	rVB	442	189	0.01%	0.001%
34	6.632	1734	1739	1740	rBV4	1170	989	0.07%	0.007%
35	6.796	1788	1790	1794	rVB3	458	256	0.02%	0.002%
36	6.854	1805	1808	1810	rVB2	375	212	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060421\
 Data File : VW021509.D
 Acq On : 04 Jun 2021 16:06
 Operator : SY/MD
 Sample : M2605-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.876	1812	1815	1817	rBV	499	278	0.02%	0.002%
38	6.915	1825	1827	1831	rVB2	293	219	0.01%	0.002%
39	6.989	1837	1850	1874	rBV	198466	364484	24.32%	2.750%
40	7.317	1941	1952	1970	rBV	720614	1242975	82.94%	9.377%
41	7.625	2038	2048	2089	rVB	136219	239591	15.99%	1.808%
42	7.780	2094	2096	2100	rVB3	673	356	0.02%	0.003%
43	7.815	2104	2107	2109	rBV2	526	287	0.02%	0.002%
44	7.886	2127	2129	2132	rVB2	269	122	0.01%	0.001%
45	7.928	2140	2142	2145	rBV	361	244	0.02%	0.002%
46	7.979	2145	2158	2182	rVV	432800	734293	49.00%	5.540%
47	8.088	2183	2192	2237	rVV	432226	778552	51.95%	5.874%
48	8.410	2289	2292	2295	rBV3	610	584	0.04%	0.004%
49	8.426	2295	2297	2299	rBV4	862	410	0.03%	0.003%
50	8.465	2305	2309	2312	rBV3	413	316	0.02%	0.002%
51	8.619	2353	2357	2358	rBV2	295	182	0.01%	0.001%
52	8.680	2373	2376	2378	rBV3	531	389	0.03%	0.003%
53	8.706	2383	2384	2388	rVV	424	239	0.02%	0.002%
54	8.735	2392	2393	2399	rVB3	568	398	0.03%	0.003%
55	8.764	2399	2402	2404	rBV	265	136	0.01%	0.001%
56	8.854	2418	2430	2458	rBV	733226	1195422	79.77%	9.019%
57	9.281	2560	2563	2568	rBV2	316	279	0.02%	0.002%
58	9.310	2568	2572	2578	rVB2	304	280	0.02%	0.002%
59	9.346	2580	2583	2585	rBV	354	252	0.02%	0.002%
60	9.378	2590	2593	2597	rVB2	401	299	0.02%	0.002%
61	9.442	2611	2613	2615	rBV	271	158	0.01%	0.001%
62	9.487	2625	2627	2630	rVB	375	130	0.01%	0.001%
63	9.532	2637	2641	2642	rBV	275	143	0.01%	0.001%
64	9.735	2700	2704	2706	rBV2	245	158	0.01%	0.001%
65	9.744	2706	2707	2711	rVB2	359	168	0.01%	0.001%
66	9.776	2711	2717	2721	rBV2	340	510	0.03%	0.004%
67	9.828	2730	2733	2737	rVB2	428	248	0.02%	0.002%
68	9.873	2741	2747	2748	rBV3	302	198	0.01%	0.001%
69	9.989	2781	2783	2786	rVB	286	136	0.01%	0.001%
70	10.027	2790	2795	2802	rBV4	1419	1873	0.12%	0.014%
71	10.130	2819	2827	2836	rVB3	3147	4667	0.31%	0.035%
72	10.217	2842	2854	2875	rBV	519450	814565	54.35%	6.145%
73	10.458	2926	2929	2930	rBV	339	178	0.01%	0.001%
74	10.641	2983	2986	2988	rBV2	319	159	0.01%	0.001%
75	10.690	2999	3001	3007	rVB2	393	273	0.02%	0.002%
76	10.725	3007	3012	3013	rBV2	353	283	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021509.D
 Acq On : 04 Jun 2021 16:06
 Operator : SY/MD
 Sample : M2605-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	10.860	3050	3054	3056	rBV2	818	489	0.03%	0.004%
78	10.886	3059	3062	3063	rVV2	288	149	0.01%	0.001%
79	10.918	3065	3072	3084	rVB5	3501	5220	0.35%	0.039%
80	11.146	3137	3143	3150	rBV6	1732	2640	0.18%	0.020%
81	11.249	3164	3175	3203	rBV	878918	1325916	88.47%	10.003%
82	11.519	3257	3259	3262	rVB2	379	133	0.01%	0.001%
83	11.538	3262	3265	3266	rBV2	327	201	0.01%	0.002%
84	11.625	3280	3292	3311	rBV	814132	1264439	84.37%	9.539%
85	11.847	3358	3361	3363	rBV2	590	437	0.03%	0.003%
86	11.905	3373	3379	3383	rVB3	311	369	0.02%	0.003%
87	11.927	3383	3386	3387	rBV2	362	178	0.01%	0.001%
88	12.021	3412	3415	3417	rBV2	433	216	0.01%	0.002%
89	12.040	3417	3421	3425	rBV2	418	339	0.02%	0.003%
90	12.124	3444	3447	3448	rVB	364	144	0.01%	0.001%
91	12.136	3448	3451	3455	rBV4	444	372	0.02%	0.003%
92	12.214	3472	3475	3477	rBV2	343	214	0.01%	0.002%
93	12.316	3503	3507	3510	rBV2	373	279	0.02%	0.002%
94	12.374	3523	3525	3529	rBV2	364	275	0.02%	0.002%
95	12.493	3559	3562	3566	rBV2	452	342	0.02%	0.003%
96	12.516	3566	3569	3571	rBV2	266	213	0.01%	0.002%
97	12.715	3625	3631	3633	rBV2	534	476	0.03%	0.004%
98	12.892	3685	3686	3688	rVB2	363	128	0.01%	0.001%
99	13.069	3739	3741	3745	rBV2	479	333	0.02%	0.003%
100	13.513	3874	3879	3887	rBV6	2247	3022	0.20%	0.023%




Sum of corrected areas: 13255208

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021509.D
Acq On : 04 Jun 2021 16:06
Operator : SY/MD
Sample : M2605-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

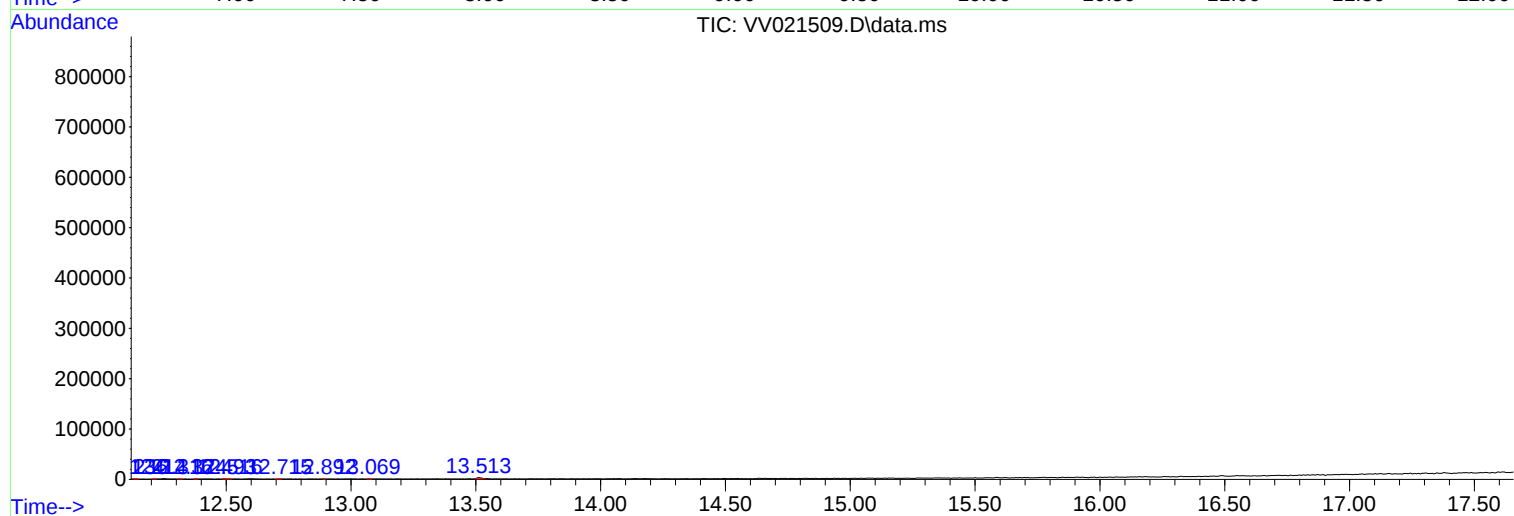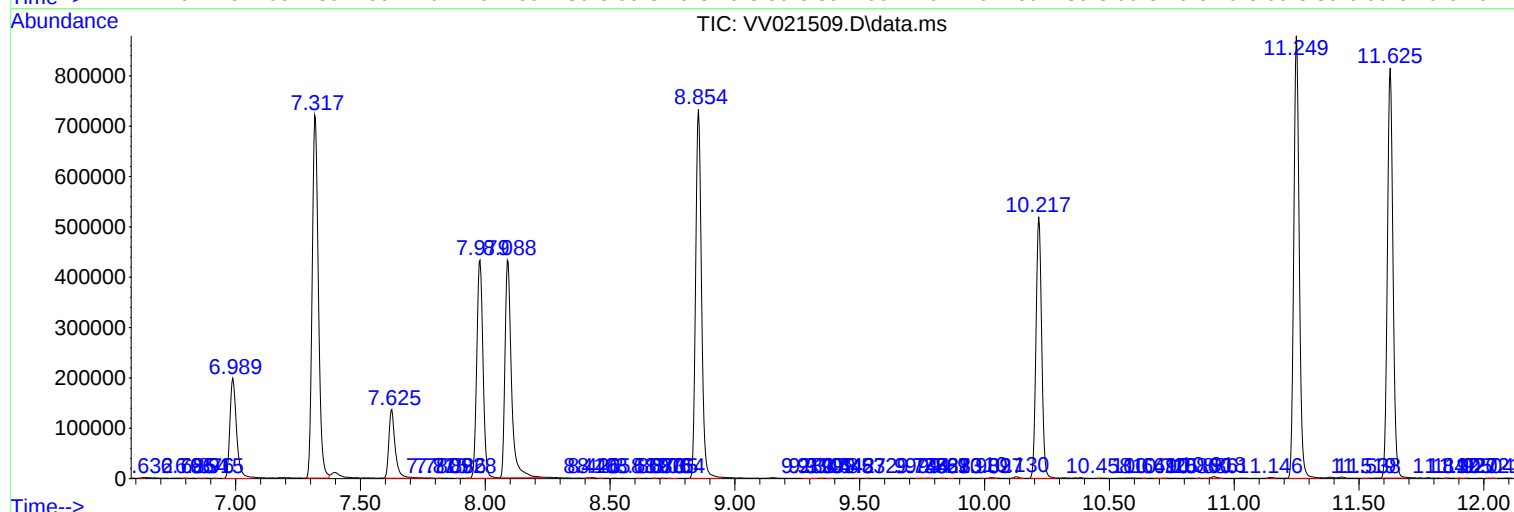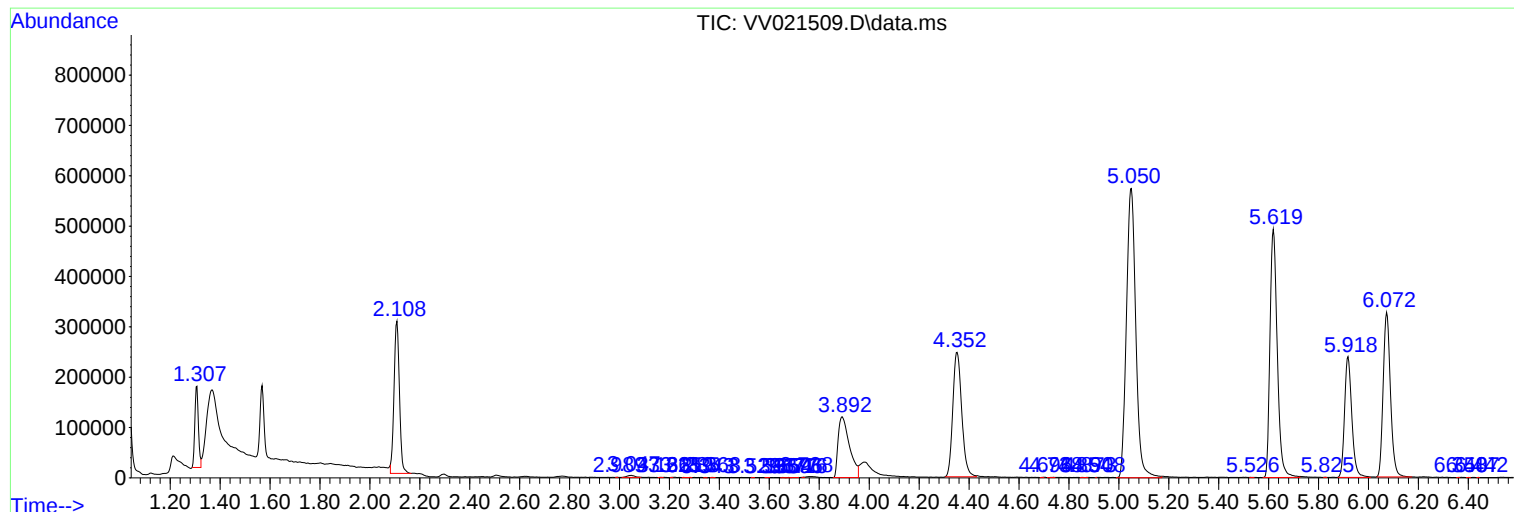

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021509.D
Acq On : 04 Jun 2021 16:06
Operator : SY/MD
Sample : M2605-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021509.D
Acq On : 04 Jun 2021 16:06
Operator : SY/MD
Sample : M2605-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
