

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021511.D
 Acq On : 04 Jun 2021 16:54
 Operator : SY/MD
 Sample : M2605-12 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	92	rVB	149254	151198	2.38%	0.820%
2	1.568	158	164	175	rVB	132514	147078	2.31%	0.798%
3	2.108	324	332	352	rVB	277582	416894	6.56%	2.261%
4	2.767	528	537	553	rVB2	16376	33448	0.53%	0.181%
5	2.963	595	598	599	rVB	415	223	0.00%	0.001%
6	2.979	599	603	607	rBV3	366	423	0.01%	0.002%
7	3.143	650	654	656	rBV	345	254	0.00%	0.001%
8	3.175	661	664	667	rBV2	428	269	0.00%	0.001%
9	3.294	697	701	704	rBV2	403	413	0.01%	0.002%
10	3.442	746	747	750	rBV2	342	188	0.00%	0.001%
11	3.487	758	761	766	rBV	314	185	0.00%	0.001%
12	3.590	791	793	796	rVB	373	147	0.00%	0.001%
13	3.619	798	802	804	rBV	175	148	0.00%	0.001%
14	3.696	821	826	830	rBV4	500	409	0.01%	0.002%
15	3.822	861	865	869	rVB2	293	279	0.00%	0.002%
16	3.850	869	874	875	rBV	186	175	0.00%	0.001%
17	3.889	875	886	927	rBV	119943	383979	6.04%	2.083%
18	4.352	1012	1030	1059	rBV	228563	568391	8.95%	3.083%
19	4.645	1118	1121	1124	rBV2	558	344	0.01%	0.002%
20	4.664	1124	1127	1129	rBV2	438	308	0.00%	0.002%
21	4.706	1138	1140	1143	rVB	419	193	0.00%	0.001%
22	4.731	1145	1148	1150	rBV2	284	156	0.00%	0.001%
23	4.764	1156	1158	1167	rVB3	461	505	0.01%	0.003%
24	4.802	1167	1170	1172	rBV	526	358	0.01%	0.002%
25	4.831	1178	1179	1184	rVB2	310	164	0.00%	0.001%
26	4.854	1184	1186	1189	rBV2	601	365	0.01%	0.002%
27	4.918	1204	1206	1208	rBV	348	163	0.00%	0.001%
28	4.982	1223	1226	1229	rBV2	363	302	0.00%	0.002%
29	5.050	1229	1247	1288	rBV2	537863	1424060	22.41%	7.724%
30	5.384	1349	1351	1354	rBV2	366	180	0.00%	0.001%
31	5.420	1358	1362	1371	rVB5	637	754	0.01%	0.004%
32	5.458	1371	1374	1376	rBV2	251	151	0.00%	0.001%
33	5.516	1390	1392	1396	rVB4	429	221	0.00%	0.001%
34	5.619	1411	1424	1457	rBV	478678	966701	15.21%	5.244%
35	5.918	1504	1517	1548	rBV	201651	410166	6.46%	2.225%
36	6.072	1551	1565	1594	rVV	310146	630587	9.92%	3.420%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021511.D
 Acq On : 04 Jun 2021 16:54
 Operator : SY/MD
 Sample : M2605-12 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.214	1605	1609	1610	rBV4	824	602	0.01%	0.003%
38	6.326	1639	1644	1647	rBV3	482	469	0.01%	0.003%
39	6.471	1686	1689	1691	rBV	344	201	0.00%	0.001%
40	6.506	1697	1700	1701	rBV	274	165	0.00%	0.001%
41	6.731	1767	1770	1771	rBV3	743	450	0.01%	0.002%
42	6.780	1783	1785	1786	rBV	475	174	0.00%	0.001%
43	6.924	1827	1830	1832	rBV	247	170	0.00%	0.001%
44	6.944	1832	1836	1839	rBV4	249	206	0.00%	0.001%
45	6.989	1839	1850	1871	rBV	188363	342888	5.40%	1.860%
46	7.320	1940	1953	1970	rBV	660344	1145685	18.03%	6.214%
47	7.625	2037	2048	2070	rBV	131177	229411	3.61%	1.244%
48	7.834	2111	2113	2115	rVB	360	146	0.00%	0.001%
49	7.866	2120	2123	2126	rVB3	548	324	0.01%	0.002%
50	7.979	2144	2158	2182	rBV	3830317	6354075	100.00%	34.465%
51	8.088	2183	2192	2222	rVB	426583	754492	11.87%	4.092%
52	8.436	2298	2300	2303	rVB	366	176	0.00%	0.001%
53	8.455	2303	2306	2308	rBV	270	184	0.00%	0.001%
54	8.677	2372	2375	2378	rBV3	289	225	0.00%	0.001%
55	8.728	2387	2391	2393	rBV	332	160	0.00%	0.001%
56	8.802	2411	2414	2415	rBV2	319	141	0.00%	0.001%
57	8.854	2418	2430	2456	rBV	710533	1151039	18.11%	6.243%
58	9.133	2513	2517	2518	rBV3	345	231	0.00%	0.001%
59	9.149	2518	2522	2525	rBV3	937	849	0.01%	0.005%
60	9.217	2537	2543	2544	rVV	275	200	0.00%	0.001%
61	9.304	2566	2570	2575	rBV	371	327	0.01%	0.002%
62	9.358	2580	2587	2588	rBV2	283	218	0.00%	0.001%
63	9.403	2599	2601	2608	rVB2	305	258	0.00%	0.001%
64	9.484	2624	2626	2630	rVB	283	156	0.00%	0.001%
65	9.545	2642	2645	2646	rBV	506	303	0.00%	0.002%
66	9.632	2671	2672	2676	rBV	362	174	0.00%	0.001%
67	9.722	2696	2700	2703	rBV2	246	196	0.00%	0.001%
68	9.763	2710	2713	2717	rBV2	163	161	0.00%	0.001%
69	9.940	2765	2768	2769	rVB2	349	155	0.00%	0.001%
70	10.079	2807	2811	2813	rBV2	187	170	0.00%	0.001%
71	10.217	2841	2854	2878	rVV	512526	799484	12.58%	4.336%
72	10.358	2897	2898	2901	rVB2	386	186	0.00%	0.001%
73	10.384	2904	2906	2908	rBV2	416	229	0.00%	0.001%
74	10.751	3017	3020	3025	rVB2	267	256	0.00%	0.001%
75	10.796	3031	3034	3037	rBV2	303	229	0.00%	0.001%
76	10.860	3049	3054	3064	rBV5	487	809	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021511.D
 Acq On : 04 Jun 2021 16:54
 Operator : SY/MD
 Sample : M2605-12 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

77	10.921	3064	3073	3083	rVV6	2739	4607	0.07%	0.025%
78	11.098	3124	3128	3130	rBV2	341	288	0.00%	0.002%
79	11.149	3137	3144	3152	rVB5	1554	2100	0.03%	0.011%
80	11.249	3163	3175	3204	rBV	837162	1292059	20.33%	7.008%
81	11.487	3247	3249	3252	rBV	256	141	0.00%	0.001%
82	11.506	3252	3255	3257	rBV2	258	153	0.00%	0.001%
83	11.548	3266	3268	3271	rVB2	505	190	0.00%	0.001%
84	11.625	3279	3292	3316	rBV	769535	1205969	18.98%	6.541%
85	11.770	3334	3337	3340	rBV5	505	448	0.01%	0.002%
86	11.847	3357	3361	3364	rBV3	725	545	0.01%	0.003%
87	12.027	3415	3417	3421	rVB2	305	150	0.00%	0.001%
88	12.078	3430	3433	3435	rBV2	300	207	0.00%	0.001%
89	12.143	3451	3453	3458	rVB2	461	226	0.00%	0.001%
90	12.332	3509	3512	3513	rBV2	352	182	0.00%	0.001%
91	12.516	3566	3569	3570	rBV2	353	145	0.00%	0.001%
92	12.545	3576	3578	3581	rVB2	342	155	0.00%	0.001%
93	12.606	3595	3597	3601	rBV3	347	231	0.00%	0.001%
94	12.628	3602	3604	3609	rVB2	583	361	0.01%	0.002%
95	12.702	3620	3627	3629	rBV3	547	467	0.01%	0.003%
96	12.767	3644	3647	3648	rBV	230	150	0.00%	0.001%
97	12.773	3648	3649	3652	rBV	302	198	0.00%	0.001%
98	13.027	3724	3728	3732	rBV2	408	460	0.01%	0.002%
99	14.075	4051	4054	4061	rBV4	541	558	0.01%	0.003%
100	14.435	4164	4166	4171	rBV4	567	423	0.01%	0.002%




Sum of corrected areas: 18436166

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021511.D
Acq On : 04 Jun 2021 16:54
Operator : SY/MD
Sample : M2605-12 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

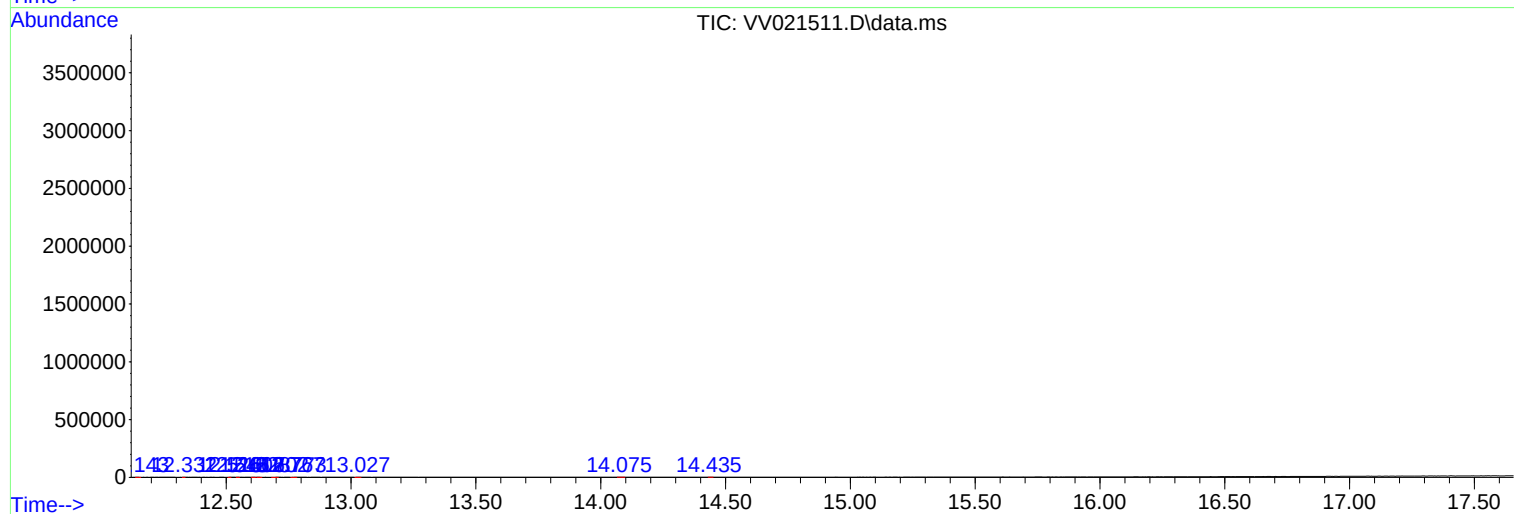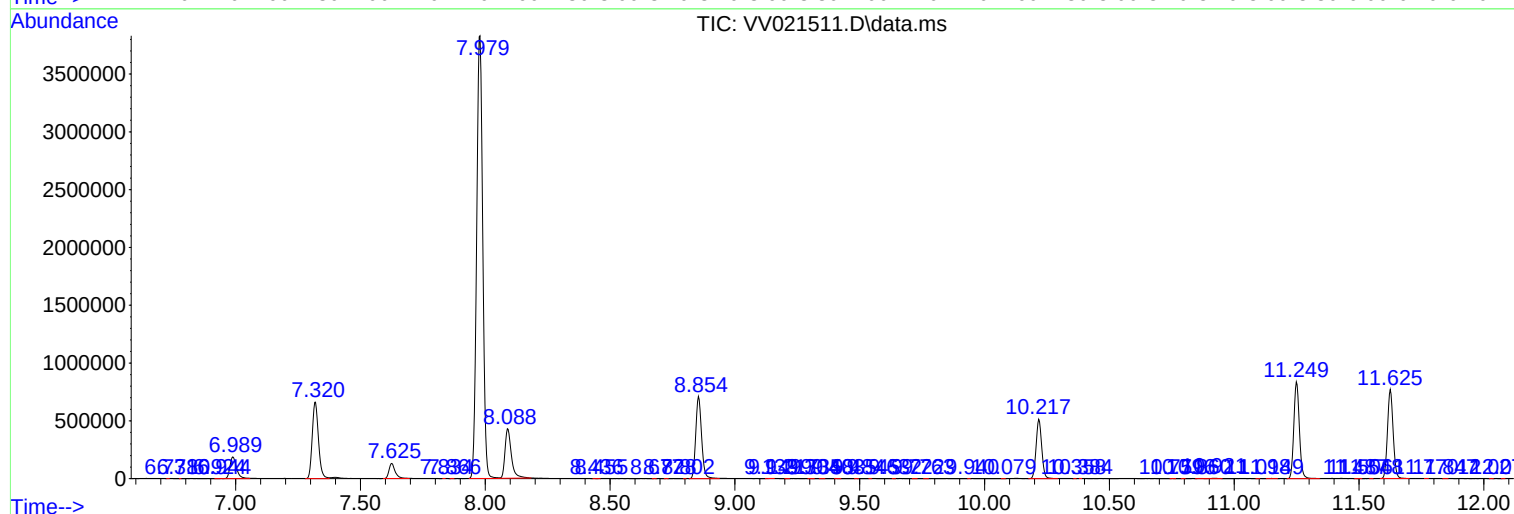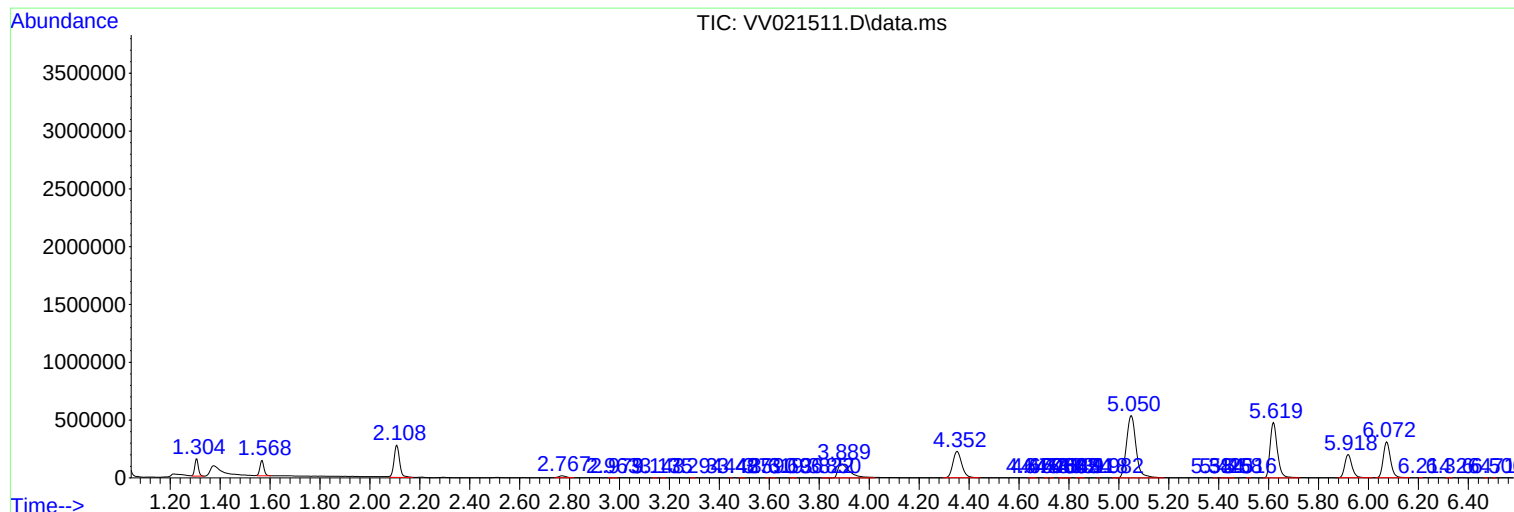

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021511.D
Acq On : 04 Jun 2021 16:54
Operator : SY/MD
Sample : M2605-12 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021511.D
Acq On : 04 Jun 2021 16:54
Operator : SY/MD
Sample : M2605-12 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
