

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021512.D
 Acq On : 04 Jun 2021 17:17
 Operator : SY/MD
 Sample : M2605-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	94	rVB	154828	160048	11.52%	1.359%
2	1.568	158	164	179	rVB	132602	149619	10.77%	1.270%
3	2.108	323	332	357	rVB	271338	410136	29.53%	3.482%
4	2.761	530	535	537	rBV2	1021	851	0.06%	0.007%
5	2.873	567	570	573	rBV2	494	272	0.02%	0.002%
6	2.947	590	593	596	rBV2	269	185	0.01%	0.002%
7	2.970	597	600	603	rVV2	623	432	0.03%	0.004%
8	3.044	616	623	628	rBV6	1345	1791	0.13%	0.015%
9	3.098	637	640	642	rVV	268	159	0.01%	0.001%
10	3.134	649	651	653	rVB	435	186	0.01%	0.002%
11	3.214	674	676	678	rBV	390	182	0.01%	0.002%
12	3.230	678	681	683	rVB2	340	163	0.01%	0.001%
13	3.375	724	726	729	rBV	333	182	0.01%	0.002%
14	3.394	729	732	733	rBV	374	206	0.01%	0.002%
15	3.442	744	747	750	rBV	279	207	0.01%	0.002%
16	3.484	757	760	766	rBV2	279	252	0.02%	0.002%
17	3.548	777	780	784	rBV2	334	212	0.02%	0.002%
18	3.712	828	831	835	rVB3	350	176	0.01%	0.001%
19	3.773	849	850	854	rVB	413	183	0.01%	0.002%
20	3.812	857	862	865	rVB3	208	175	0.01%	0.001%
21	3.838	865	870	876	rBV2	212	242	0.02%	0.002%
22	3.892	876	887	924	rBV	116951	372686	26.83%	3.164%
23	4.352	1013	1030	1062	rBV	225947	563828	40.60%	4.787%
24	4.600	1103	1107	1110	rBV3	395	310	0.02%	0.003%
25	4.626	1114	1115	1118	rBV2	343	204	0.01%	0.002%
26	4.783	1160	1164	1165	rBV	264	169	0.01%	0.001%
27	4.793	1165	1167	1171	rVV2	301	188	0.01%	0.002%
28	4.825	1175	1177	1182	rVB2	291	246	0.02%	0.002%
29	5.050	1229	1247	1275	rBV2	541517	1388873	100.00%	11.792%
30	5.307	1326	1327	1329	rBV	340	157	0.01%	0.001%
31	5.339	1333	1337	1338	rBV2	455	340	0.02%	0.003%
32	5.481	1379	1381	1385	rBV2	553	468	0.03%	0.004%
33	5.571	1406	1409	1410	rBV2	372	186	0.01%	0.002%
34	5.619	1412	1424	1457	rVV	496854	997549	71.82%	8.469%
35	5.815	1481	1485	1489	rBV4	542	459	0.03%	0.004%
36	5.915	1506	1516	1535	rVB8	7535	17352	1.25%	0.147%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021512.D
 Acq On : 04 Jun 2021 17:17
 Operator : SY/MD
 Sample : M2605-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.072	1551	1565	1598	rBV	310091	638387	45.96%	5.420%
38	6.285	1628	1631	1632	rBV	500	284	0.02%	0.002%
39	6.388	1659	1663	1667	rBV2	392	274	0.02%	0.002%
40	6.513	1698	1702	1704	rBV3	475	364	0.03%	0.003%
41	6.532	1706	1708	1711	rBV2	386	233	0.02%	0.002%
42	6.597	1723	1728	1731	rBV2	423	380	0.03%	0.003%
43	6.806	1789	1793	1799	rBV3	431	441	0.03%	0.004%
44	6.896	1816	1821	1822	rBV	443	257	0.02%	0.002%
45	6.989	1837	1850	1872	rBV	189978	345335	24.86%	2.932%
46	7.256	1928	1933	1937	rBV4	726	779	0.06%	0.007%
47	7.317	1941	1952	1972	rBV	656773	1141984	82.22%	9.696%
48	7.625	2037	2048	2079	rBV	129235	230442	16.59%	1.956%
49	7.847	2115	2117	2122	rVB2	409	277	0.02%	0.002%
50	7.870	2122	2124	2127	rVB	361	168	0.01%	0.001%
51	7.905	2133	2135	2138	rVB	296	158	0.01%	0.001%
52	7.921	2138	2140	2142	rBV2	340	163	0.01%	0.001%
53	7.979	2149	2158	2173	rVB2	16790	29162	2.10%	0.248%
54	8.088	2181	2192	2229	rBV	429989	785265	56.54%	6.667%
55	8.400	2287	2289	2291	rBV2	553	231	0.02%	0.002%
56	8.542	2331	2333	2334	rBV2	467	198	0.01%	0.002%
57	8.616	2354	2356	2360	rBV	445	220	0.02%	0.002%
58	8.741	2393	2395	2399	rVB2	405	244	0.02%	0.002%
59	8.767	2399	2403	2405	rBV	218	162	0.01%	0.001%
60	8.783	2405	2408	2412	rVB3	429	252	0.02%	0.002%
61	8.812	2412	2417	2418	rBV2	246	162	0.01%	0.001%
62	8.854	2418	2430	2450	rBV	743729	1199432	86.36%	10.183%
63	9.175	2529	2530	2536	rVB	806	483	0.03%	0.004%
64	9.207	2536	2540	2541	rBV2	255	172	0.01%	0.001%
65	9.294	2565	2567	2571	rVB2	308	220	0.02%	0.002%
66	9.420	2602	2606	2608	rBV2	317	180	0.01%	0.002%
67	9.680	2684	2687	2689	rBV2	382	184	0.01%	0.002%
68	9.725	2696	2701	2703	rBV2	398	277	0.02%	0.002%
69	9.793	2717	2722	2725	rBV	222	184	0.01%	0.002%
70	9.844	2731	2738	2739	rBV2	277	231	0.02%	0.002%
71	9.873	2742	2747	2749	rVB2	304	257	0.02%	0.002%
72	9.895	2749	2754	2756	rBV2	360	255	0.02%	0.002%
73	9.934	2763	2766	2768	rBV2	262	153	0.01%	0.001%
74	10.085	2811	2813	2818	rVB2	342	172	0.01%	0.001%
75	10.130	2818	2827	2836	rBV4	2237	3545	0.26%	0.030%
76	10.217	2841	2854	2880	rBV	514109	797946	57.45%	6.775%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021512.D
 Acq On : 04 Jun 2021 17:17
 Operator : SY/MD
 Sample : M2605-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	10.352	2894	2896	2898	rVB2	484	221	0.02%	0.002%
78	10.538	2950	2954	2957	rBV2	277	257	0.02%	0.002%
79	10.564	2960	2962	2965	rBV2	464	268	0.02%	0.002%
80	10.857	3048	3053	3057	rBV	532	457	0.03%	0.004%
81	11.043	3105	3111	3116	rVB2	551	583	0.04%	0.005%
82	11.114	3131	3133	3137	rBV2	251	179	0.01%	0.002%
83	11.149	3137	3144	3152	rBV4	1222	1524	0.11%	0.013%
84	11.204	3158	3161	3163	rVB	362	239	0.02%	0.002%
85	11.249	3163	3175	3194	rBV	864016	1324894	95.39%	11.248%
86	11.493	3247	3251	3253	rBV2	313	219	0.02%	0.002%
87	11.625	3279	3292	3314	rBV	768323	1198293	86.28%	10.174%
88	11.841	3355	3359	3363	rBV3	527	442	0.03%	0.004%
89	11.860	3363	3365	3369	rVV2	456	250	0.02%	0.002%
90	11.879	3369	3371	3374	rVB2	353	162	0.01%	0.001%
91	11.937	3386	3389	3390	rBV2	340	227	0.02%	0.002%
92	12.043	3420	3422	3425	rBV	272	188	0.01%	0.002%
93	12.056	3425	3426	3429	rVB	333	165	0.01%	0.001%
94	12.088	3434	3436	3440	rBV2	229	174	0.01%	0.001%
95	12.239	3481	3483	3484	rBV	346	173	0.01%	0.001%
96	12.413	3534	3537	3539	rBV	295	171	0.01%	0.001%
97	12.429	3539	3542	3547	rVV	320	209	0.02%	0.002%
98	12.526	3569	3572	3574	rBV	326	200	0.01%	0.002%
99	12.561	3580	3583	3587	rVB3	282	254	0.02%	0.002%
100	13.387	3838	3840	3843	rBV2	428	272	0.02%	0.002%




Sum of corrected areas: 11778408

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021512.D
Acq On : 04 Jun 2021 17:17
Operator : SY/MD
Sample : M2605-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

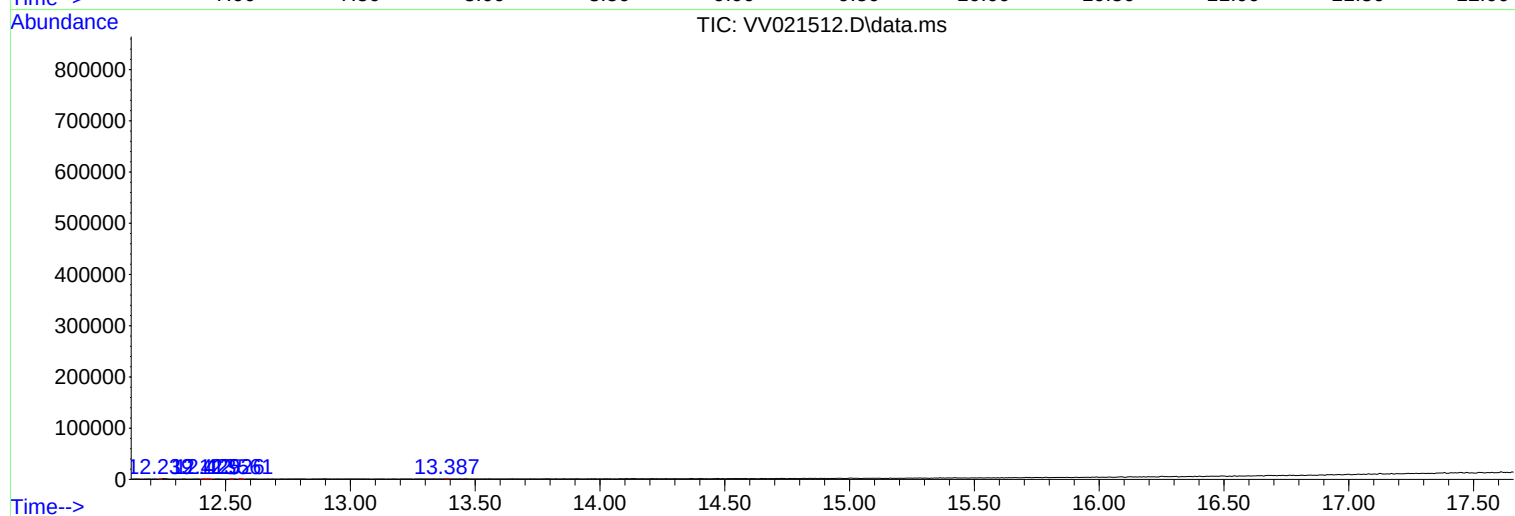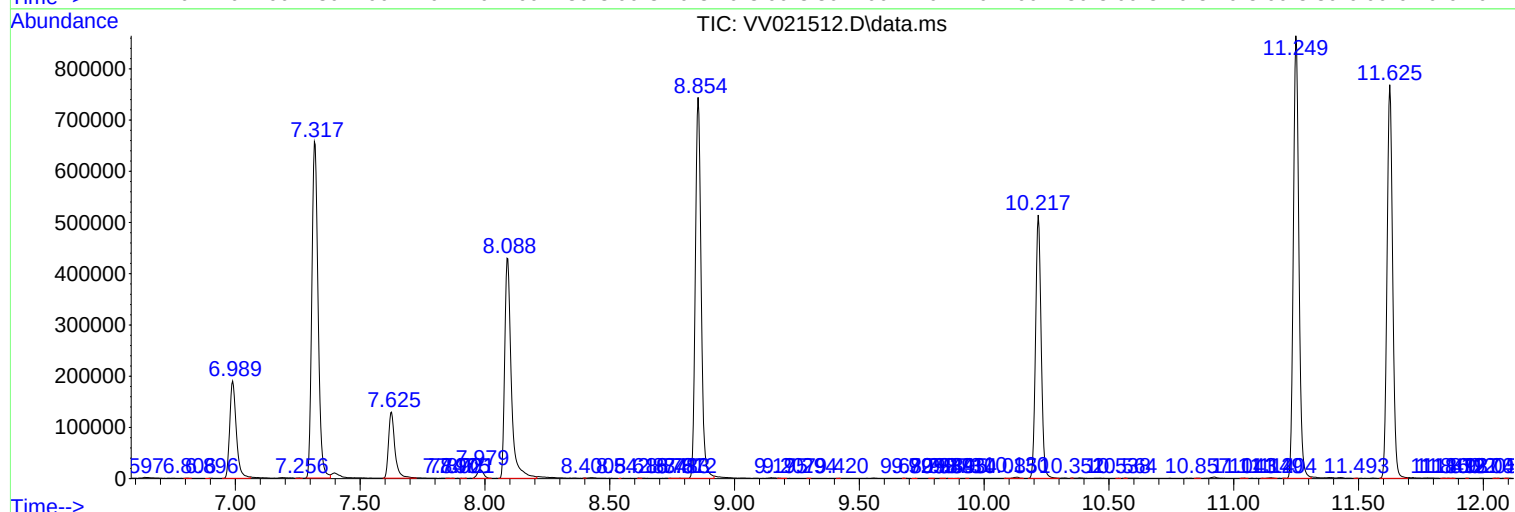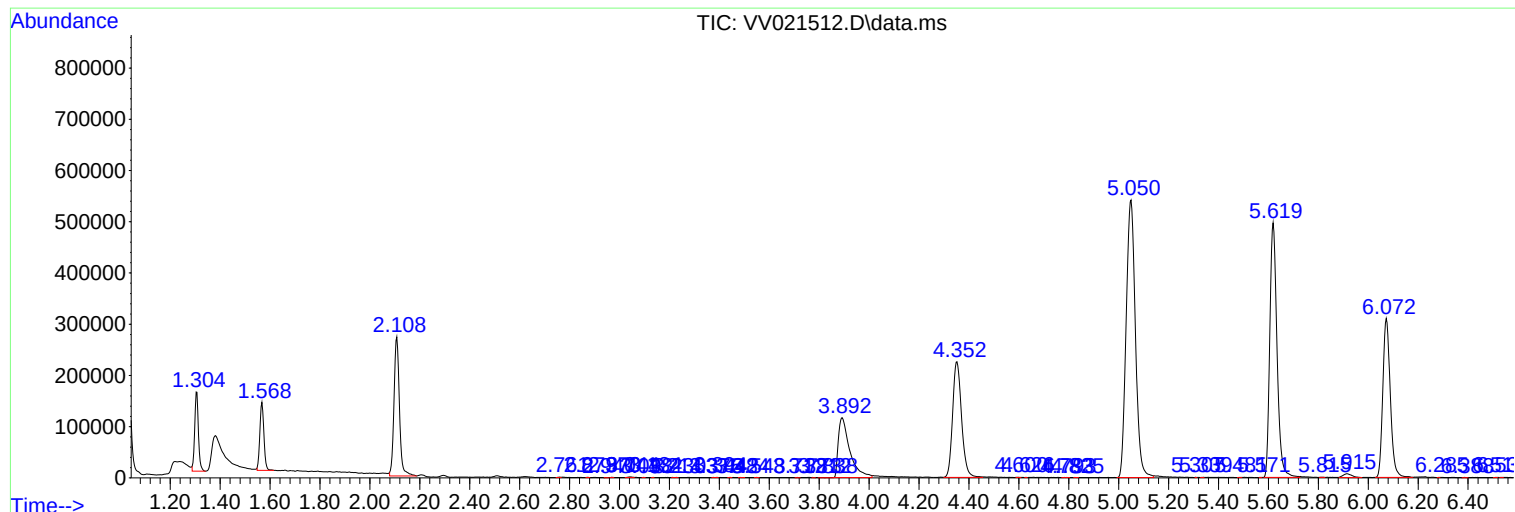

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021512.D
Acq On : 04 Jun 2021 17:17
Operator : SY/MD
Sample : M2605-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021512.D
Acq On : 04 Jun 2021 17:17
Operator : SY/MD
Sample : M2605-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
