

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021513.D
 Acq On : 04 Jun 2021 17:41
 Operator : SY/MD
 Sample : VIBLK182
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK182

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rVB	156947	159899	11.40%	1.351%
2	1.568	158	164	174	rVB	136153	147234	10.50%	1.244%
3	2.108	323	332	356	rVB	277087	418332	29.83%	3.534%
4	2.471	443	445	447	rBV2	563	303	0.02%	0.003%
5	2.561	471	473	478	rBV	382	246	0.02%	0.002%
6	2.703	516	517	521	rVB2	401	218	0.02%	0.002%
7	2.767	530	537	542	rBV5	571	767	0.05%	0.006%
8	2.838	555	559	561	rVB2	287	166	0.01%	0.001%
9	2.870	566	569	571	rBV	327	220	0.02%	0.002%
10	3.008	609	612	614	rBV	267	168	0.01%	0.001%
11	3.050	617	625	630	rBV4	1131	1829	0.13%	0.015%
12	3.124	645	648	652	rBV3	225	226	0.02%	0.002%
13	3.275	692	695	697	rBV	313	187	0.01%	0.002%
14	3.297	700	702	707	rVB	234	189	0.01%	0.002%
15	3.384	726	729	731	rBV	280	136	0.01%	0.001%
16	3.432	742	744	747	rBV2	330	167	0.01%	0.001%
17	3.494	762	763	766	rBV	247	112	0.01%	0.001%
18	3.584	788	791	796	rBV2	252	150	0.01%	0.001%
19	3.703	826	828	831	rVB2	271	155	0.01%	0.001%
20	3.731	834	837	841	rVB	307	161	0.01%	0.001%
21	3.764	844	847	848	rBV	281	167	0.01%	0.001%
22	3.825	864	866	872	rVB2	356	230	0.02%	0.002%
23	3.889	876	886	923	rBV	119306	364236	25.97%	3.077%
24	4.352	1014	1030	1058	rBV	227237	567187	40.44%	4.792%
25	4.538	1085	1088	1091	rBV3	527	286	0.02%	0.002%
26	4.738	1148	1150	1153	rBV	239	123	0.01%	0.001%
27	4.754	1153	1155	1158	rVB3	355	195	0.01%	0.002%
28	4.792	1162	1167	1170	rBV3	353	347	0.02%	0.003%
29	4.895	1197	1199	1203	rVB2	285	163	0.01%	0.001%
30	4.918	1203	1206	1209	rBV2	312	187	0.01%	0.002%
31	4.969	1220	1222	1227	rBV	266	181	0.01%	0.002%
32	5.050	1230	1247	1278	rBV2	542355	1402567	100.00%	11.850%
33	5.394	1352	1354	1355	rVB	422	116	0.01%	0.001%
34	5.461	1373	1375	1379	rBV3	359	233	0.02%	0.002%
35	5.490	1380	1384	1386	rBV2	445	249	0.02%	0.002%
36	5.564	1404	1407	1408	rBV	488	287	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021513.D
 Acq On : 04 Jun 2021 17:41
 Operator : SY/MD
 Sample : VIBLK182
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK182

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	5.619	1411	1424	1456	rBV	493508	998958	71.22%	8.440%
38	5.915	1506	1516	1529	rBV7	7383	16307	1.16%	0.138%
39	5.976	1534	1535	1537	rBV	407	166	0.01%	0.001%
40	6.072	1551	1565	1595	rBV	314669	639886	45.62%	5.406%
41	6.365	1653	1656	1659	rVB3	451	261	0.02%	0.002%
42	6.384	1661	1662	1666	rVB3	472	176	0.01%	0.001%
43	6.407	1666	1669	1671	rBV2	258	129	0.01%	0.001%
44	6.509	1699	1701	1704	rBV	408	289	0.02%	0.002%
45	6.593	1722	1727	1731	rBV4	463	515	0.04%	0.004%
46	6.738	1770	1772	1773	rBV	342	121	0.01%	0.001%
47	6.796	1789	1790	1792	rVB	315	102	0.01%	0.001%
48	6.812	1792	1795	1798	rBV2	478	285	0.02%	0.002%
49	6.892	1817	1820	1821	rBV2	291	131	0.01%	0.001%
50	6.989	1835	1850	1871	rBV	190197	347704	24.79%	2.938%
51	7.320	1940	1953	1971	rBV	665514	1159670	82.68%	9.797%
52	7.625	2037	2048	2073	rBV2	128115	230629	16.44%	1.948%
53	7.895	2130	2132	2134	rVB	310	141	0.01%	0.001%
54	7.915	2134	2138	2143	rVB3	428	325	0.02%	0.003%
55	7.940	2143	2146	2147	rBV3	375	210	0.01%	0.002%
56	7.982	2151	2159	2169	rVB3	7941	12806	0.91%	0.108%
57	8.088	2180	2192	2226	rBV	438559	791117	56.40%	6.684%
58	8.416	2291	2294	2296	rBV2	801	516	0.04%	0.004%
59	8.567	2337	2341	2343	rBV2	236	167	0.01%	0.001%
60	8.619	2354	2357	2358	rBV2	244	139	0.01%	0.001%
61	8.657	2364	2369	2371	rBV	380	293	0.02%	0.002%
62	8.734	2391	2393	2398	rVB3	201	106	0.01%	0.001%
63	8.792	2409	2411	2414	rBV2	190	103	0.01%	0.001%
64	8.853	2418	2430	2450	rBV	733908	1193024	85.06%	10.079%
65	9.117	2510	2512	2517	rBV	221	244	0.02%	0.002%
66	9.149	2518	2522	2532	rVB3	1115	1392	0.10%	0.012%
67	9.291	2563	2566	2567	rBV	211	101	0.01%	0.001%
68	9.361	2585	2588	2591	rVB2	331	197	0.01%	0.002%
69	9.394	2595	2598	2600	rBV2	209	110	0.01%	0.001%
70	9.477	2621	2624	2630	rBV2	227	155	0.01%	0.001%
71	9.522	2636	2638	2642	rVB2	292	162	0.01%	0.001%
72	9.554	2642	2648	2649	rBV3	465	391	0.03%	0.003%
73	9.725	2699	2701	2704	rVV2	207	111	0.01%	0.001%
74	9.940	2765	2768	2772	rVB2	273	215	0.02%	0.002%
75	10.027	2790	2795	2797	rBV2	358	287	0.02%	0.002%
76	10.133	2815	2828	2837	rVB7	2326	3907	0.28%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021513.D
 Acq On : 04 Jun 2021 17:41
 Operator : SY/MD
 Sample : VIBLK182
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK182

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

77	10.217	2841	2854	2877	rBV	517144	807382	57.56%	6.821%
78	10.458	2926	2929	2931	rBV2	257	201	0.01%	0.002%
79	10.519	2946	2948	2952	rBV2	207	118	0.01%	0.001%
80	10.654	2986	2990	2991	rBV	257	171	0.01%	0.001%
81	10.741	3013	3017	3019	rBV2	187	168	0.01%	0.001%
82	10.795	3031	3034	3036	rBV	258	165	0.01%	0.001%
83	10.831	3044	3045	3049	rVB2	458	236	0.02%	0.002%
84	10.921	3066	3073	3081	rBV5	2581	3554	0.25%	0.030%
85	11.001	3097	3098	3102	rBV	248	131	0.01%	0.001%
86	11.037	3103	3109	3116	rVV2	748	700	0.05%	0.006%
87	11.140	3136	3141	3142	rBV2	1000	683	0.05%	0.006%
88	11.188	3152	3156	3162	rBV3	419	392	0.03%	0.003%
89	11.249	3163	3175	3194	rBV	876135	1331108	94.91%	11.246%
90	11.625	3280	3292	3318	rBV	769455	1219711	86.96%	10.305%
91	11.940	3388	3390	3391	rBV	235	123	0.01%	0.001%
92	12.014	3410	3413	3418	rVB2	256	222	0.02%	0.002%
93	12.037	3418	3420	3421	rBV	327	119	0.01%	0.001%
94	12.159	3457	3458	3461	rBV	274	142	0.01%	0.001%
95	12.246	3480	3485	3486	rBV2	498	372	0.03%	0.003%
96	12.406	3531	3535	3537	rBV2	366	311	0.02%	0.003%
97	12.525	3570	3572	3575	rVB	383	169	0.01%	0.001%
98	12.609	3594	3598	3601	rBV2	706	661	0.05%	0.006%
99	13.011	3720	3723	3726	rBV2	460	279	0.02%	0.002%
100	13.101	3749	3751	3754	rBV2	335	123	0.01%	0.001%




Sum of corrected areas: 11836408

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021513.D
Acq On : 04 Jun 2021 17:41
Operator : SY/MD
Sample : VIBLK182
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK182

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

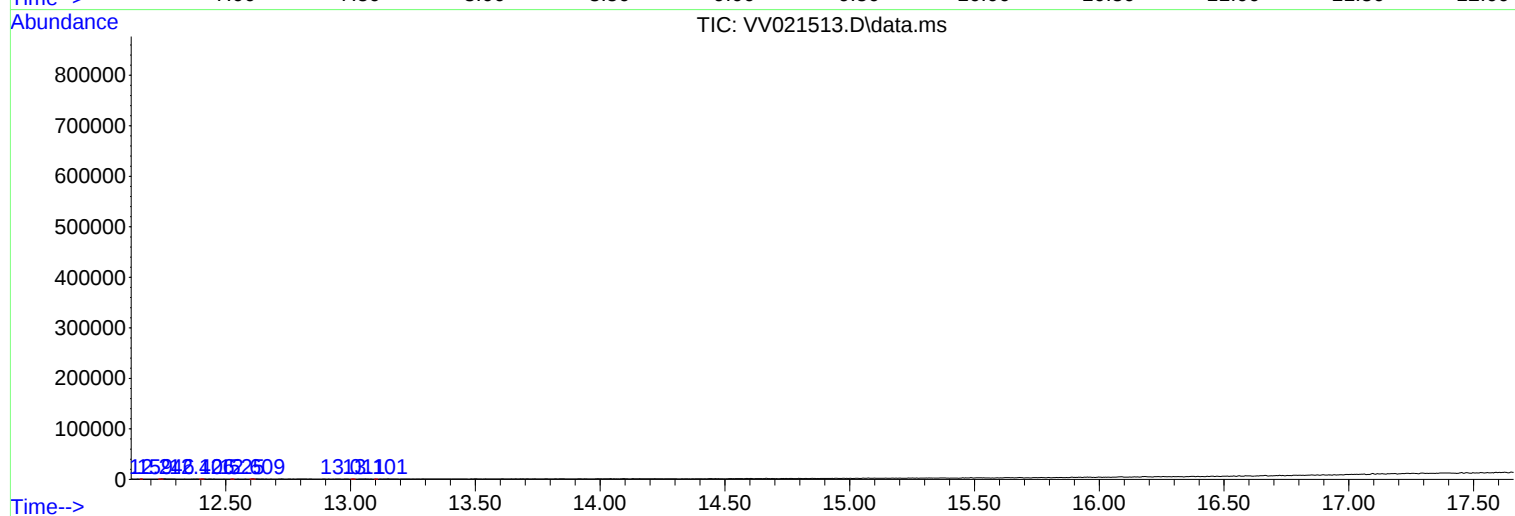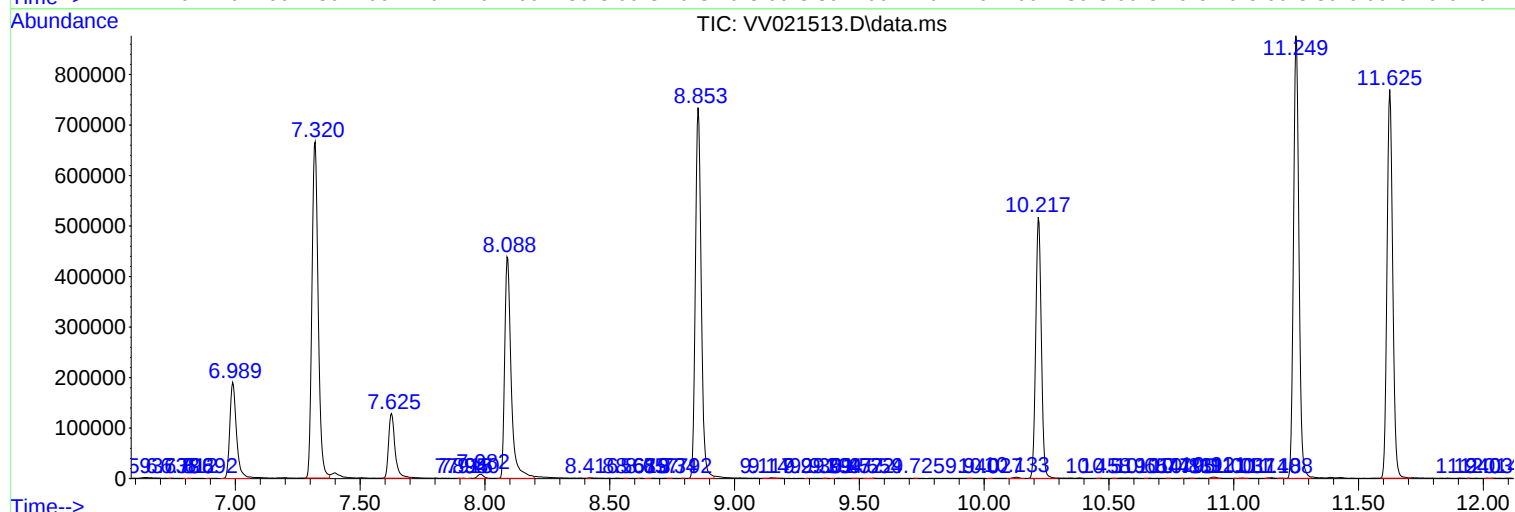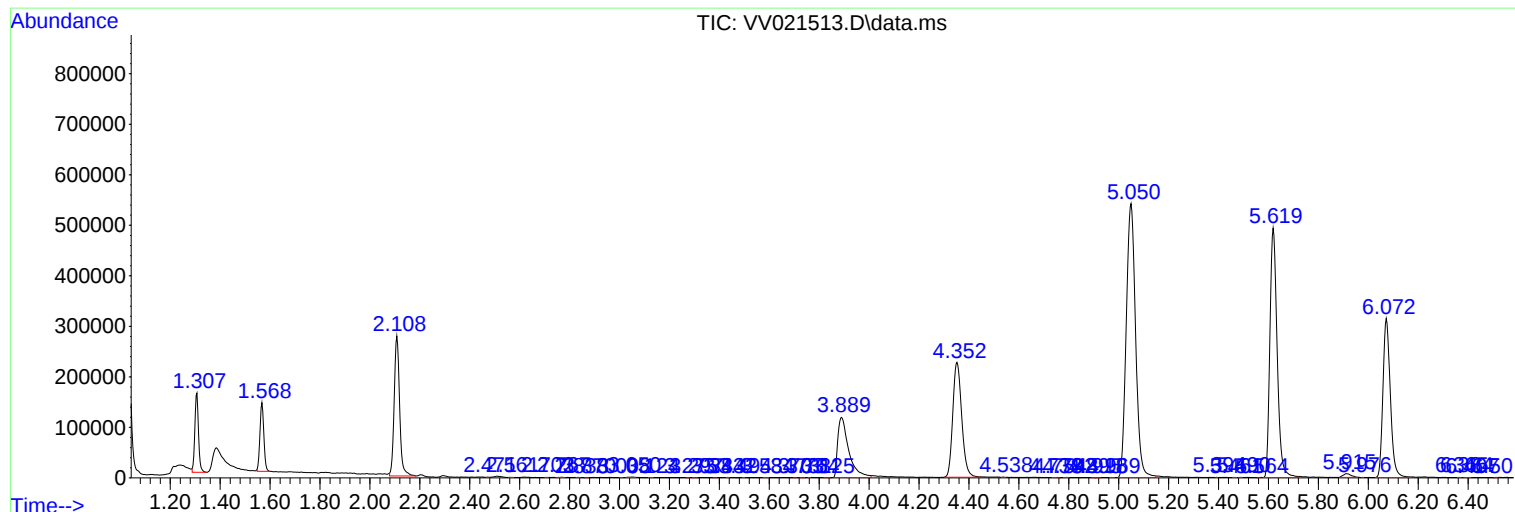

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021513.D
Acq On : 04 Jun 2021 17:41
Operator : SY/MD
Sample : VIBLK182
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK182

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
Data File : VV021513.D
Acq On : 04 Jun 2021 17:41
Operator : SY/MD
Sample : VIBLK182
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK182

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------