


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060421\
 Data File : VV021492.D
 Acq On : 04 Jun 2021 08:51
 Operator : SY/MD
 Sample : BFB67
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB167

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis
 Last Update : Tue Jun 08 03:17:01 2021

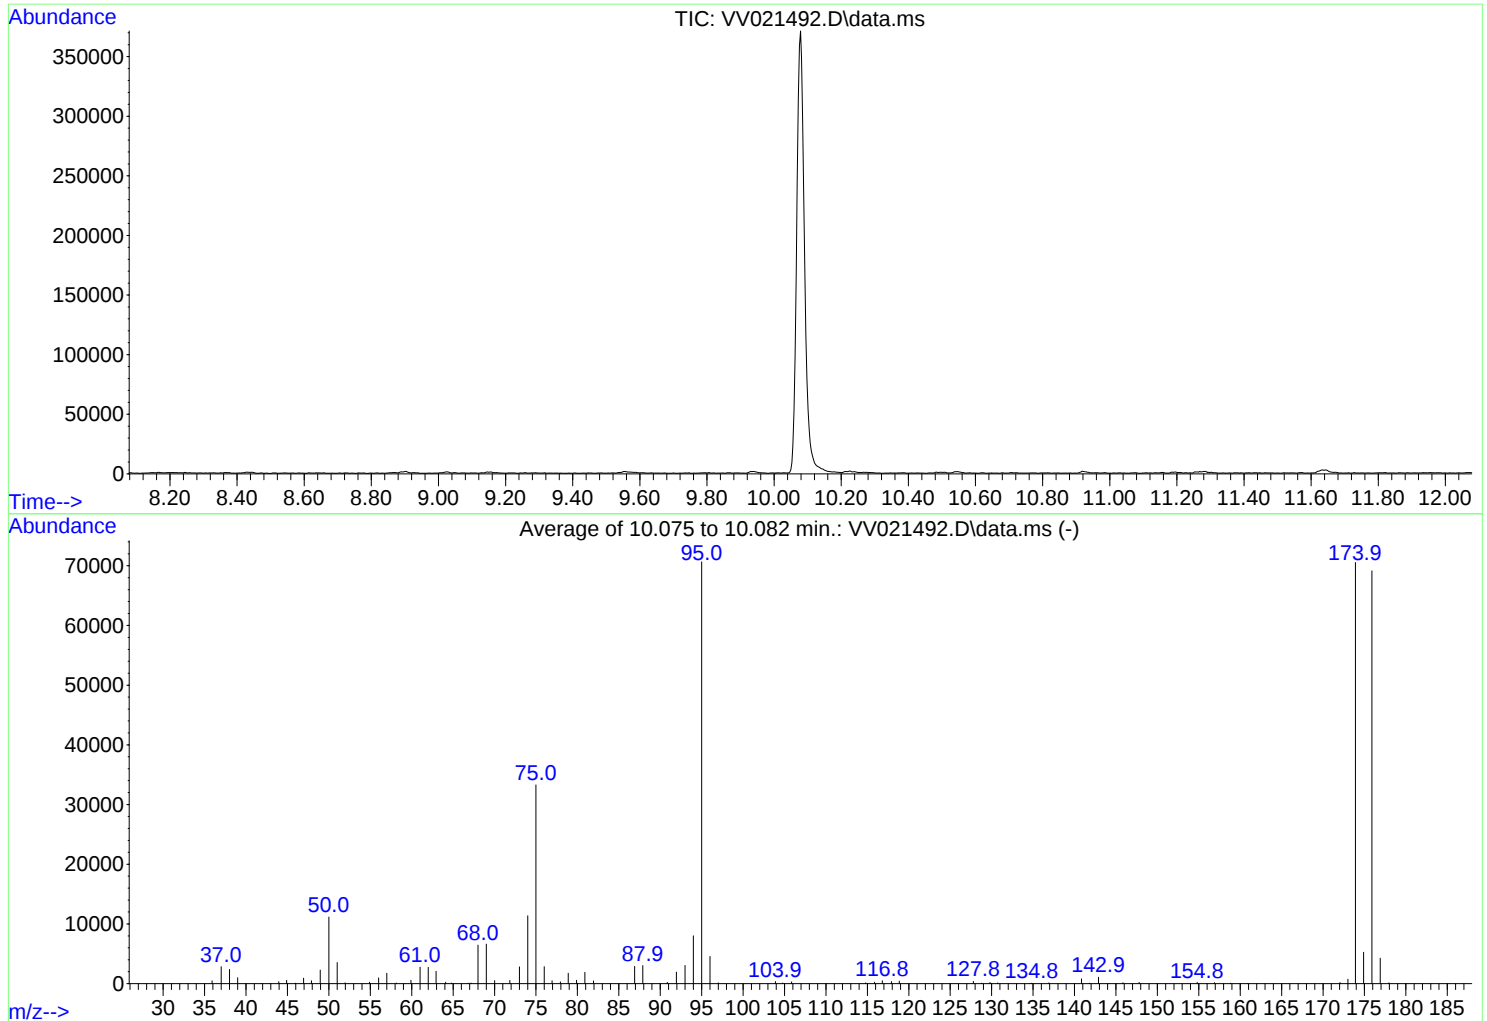

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	11160	PASS
75	95	30	80	47.1	33293	PASS
95	95	100	100	100.0	70656	PASS
96	95	5	9	6.5	4560	PASS
173	174	0.00	2	1.1	757	PASS
174	95	50	120	99.8	70541	PASS
175	174	5	9	7.4	5245	PASS
176	174	95	105	98.0	69155	PASS
177	176	5	10	6.2	4266	PASS

m/z	Abundance
35.90	536.0
37.00	3037.0
38.00	2500.0
39.00	995.0
39.90	175.0
41.00	134.0
42.90	108.0
44.00	784.0
44.90	553.0
46.00	141.0
47.00	908.0
47.90	475.0
49.00	2456.0
50.00	11597.0
51.00	3743.0
52.00	135.0
54.90	230.0
56.00	842.0
57.00	1742.0
58.20	112.0
59.90	607.0
61.00	2884.0
62.00	2775.0
63.00	2065.0
64.00	243.0
64.80	119.0
66.80	125.0
68.00	6341.0
69.00	6791.0
70.00	511.0
71.80	500.0
73.00	2761.0
74.00	11359.0
75.00	33464.0
76.00	2999.0
77.00	553.0
77.90	354.0
78.90	1831.0
79.90	583.0
80.90	1868.0
82.00	424.0
86.90	2895.0
87.90	3152.0
90.90	237.0
92.00	1926.0
93.00	3031.0
94.00	7983.0
95.00	70912.0
96.00	4675.0
97.00	172.0
103.90	319.0
104.80	127.0
105.90	326.0
114.70	132.0
115.80	244.0
116.80	471.0
117.90	374.0
118.80	457.0
127.80	372.0
128.80	137.0
129.80	215.0
130.70	160.0
134.60	121.0
136.90	131.0
140.90	827.0
142.90	1000.0
145.80	186.0
147.80	197.0
154.80	198.0
156.90	134.0
158.80	113.0
172.00	181.0
173.00	786.0
173.90	68864.0
174.90	5221.0
175.90	67888.0
176.90	4245.0
178.00	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB167

m/z	Abundance
39.90	177.0
40.90	127.0
44.00	473.0

Instrument :
MSVOA_V
ClientSampleId :
BFB167

m/z	Abundance
35.90	497.0
37.00	2947.0
38.00	2465.0
39.00	1009.0
39.90	177.0
40.90	119.0
41.80	102.0
43.90	801.0
44.90	585.0
45.90	127.0
47.00	963.0
47.90	516.0
48.90	2300.0
50.00	11461.0
51.00	3645.0
51.90	151.0
54.90	242.0
56.00	1012.0
57.00	1816.0
58.20	123.0
59.90	577.0
61.00	2790.0
62.00	2799.0
62.90	2111.0
64.10	260.0
64.80	119.0
66.80	135.0
67.20	143.0
68.00	6643.0
69.00	6903.0
70.00	505.0
71.90	574.0
73.00	2925.0
74.00	11783.0
75.00	34360.0
76.00	2982.0
77.00	472.0
78.00	298.0
78.90	1797.0
79.90	585.0
80.90	1945.0
81.90	480.0
86.90	2975.0
87.90	3129.0
90.90	231.0
91.90	1993.0
93.00	3240.0
94.00	8209.0
95.00	72856.0
96.00	4693.0
97.00	148.0
103.90	352.0
104.80	112.0
105.90	304.0
114.80	133.0
115.90	246.0
116.80	499.0
117.90	376.0
118.80	446.0
127.80	394.0
128.70	104.0
129.80	216.0
130.70	150.0
134.80	128.0
136.90	134.0
140.80	809.0
141.80	112.0
142.90	1143.0
145.80	160.0
147.80	209.0
154.80	219.0
156.90	163.0
158.90	106.0
172.00	216.0
173.00	805.0
173.90	72752.0
174.90	5444.0
175.90	71496.0
176.90	4387.0
178.00	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB167

m/z	Abundance
35.90	403.0
37.00	2520.0
38.00	2196.0
39.00	976.0
39.90	174.0
43.90	781.0
44.90	547.0
46.90	857.0
47.90	447.0
48.90	2070.0
50.00	10421.0
51.00	3217.0
51.90	159.0
54.90	224.0
56.00	1050.0
57.00	1698.0
58.10	110.0
59.90	502.0
61.00	2651.0
62.00	2615.0
62.90	1999.0
64.20	230.0
64.80	107.0
67.10	151.0
68.00	6421.0
69.00	6208.0
70.00	524.0
71.90	519.0
73.00	2803.0
74.00	10974.0
75.00	32056.0
76.00	2555.0
76.90	428.0
78.00	263.0
78.90	1591.0
79.90	561.0
80.90	1878.0
81.90	498.0
86.90	2836.0
87.90	2815.0
90.80	225.0
91.90	1853.0
93.00	2883.0
94.00	7863.0
95.00	68200.0
96.00	4312.0
97.00	122.0
103.90	337.0
104.80	102.0
105.80	251.0
114.90	121.0
115.80	215.0
116.80	455.0
117.90	291.0
118.90	404.0
127.80	387.0
129.80	227.0
130.80	119.0
134.90	133.0
136.90	123.0
140.90	760.0
141.80	135.0
142.90	1105.0
145.90	128.0
147.80	206.0
154.80	217.0
156.90	176.0
160.90	106.0
172.10	193.0
173.00	680.0
173.90	70008.0
174.90	5070.0
175.90	68080.0
176.90	4166.0
177.90	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB167