




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038747.D
Acq On : 04 Jun 2025 15:21
Operator : SY/MD
Sample : VSTD00142
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001242

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 08:29:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 08:29:01 2025
Response via : Initial Calibration

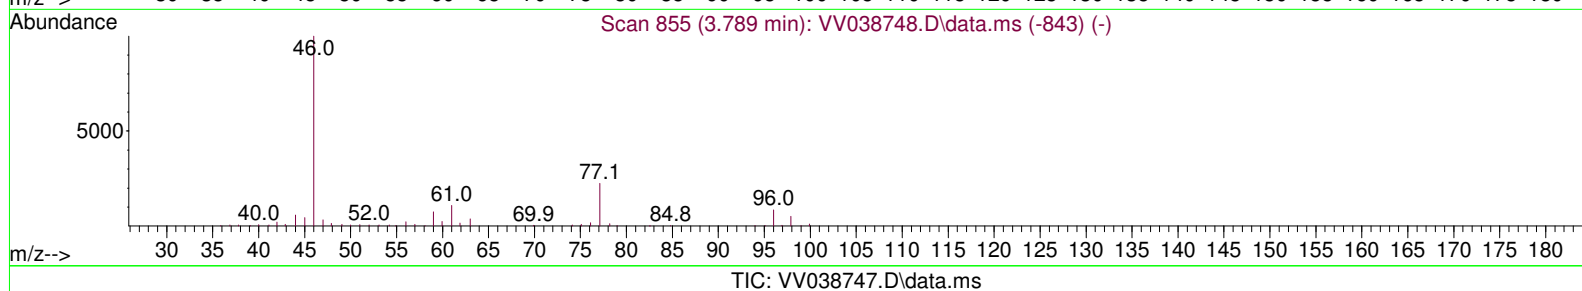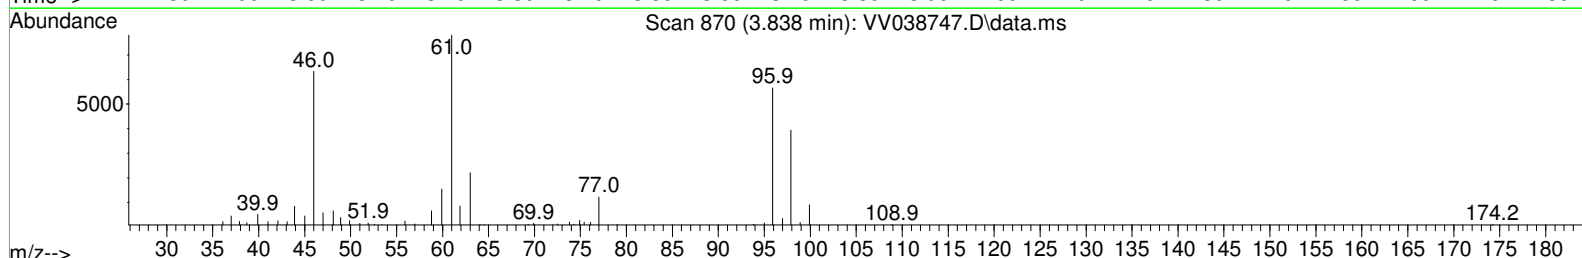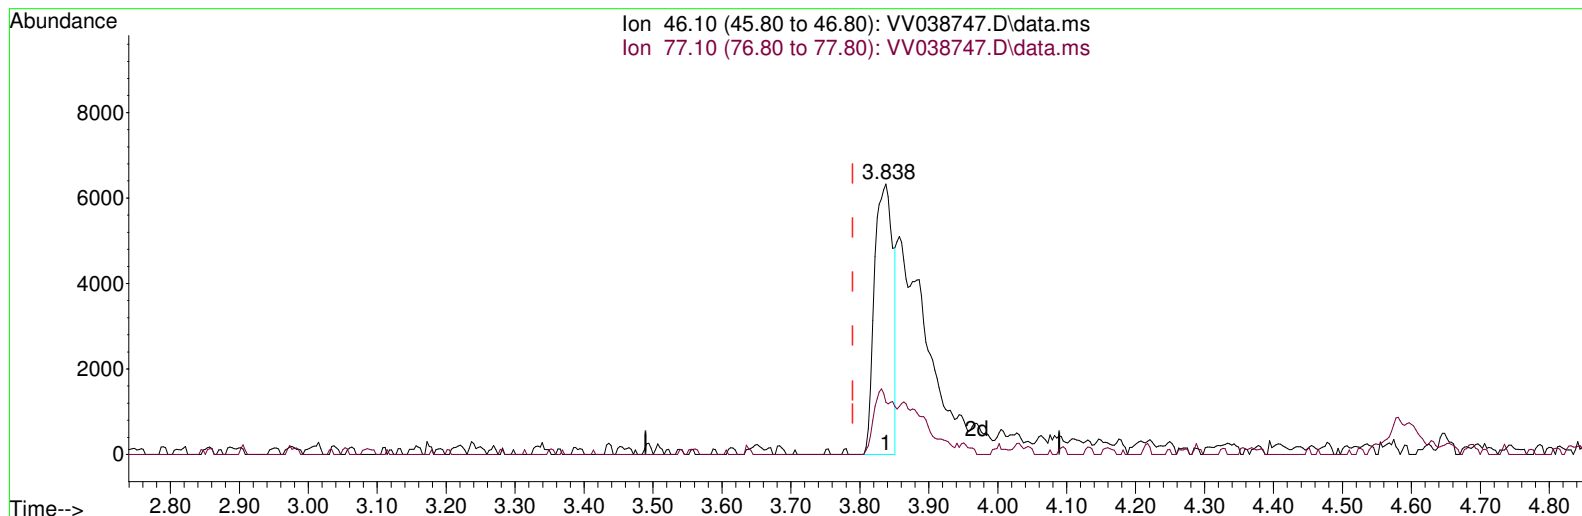

(20) 2-Butanone-d5 (S)

3.838min (+ 0.048) 3.10 ug/L

response 11784

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	23.70	17.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038747.D
Acq On : 04 Jun 2025 15:21
Operator : SY/MD
Sample : VSTD00142
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001242

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 08:29:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 08:29:01 2025
Response via : Initial Calibration

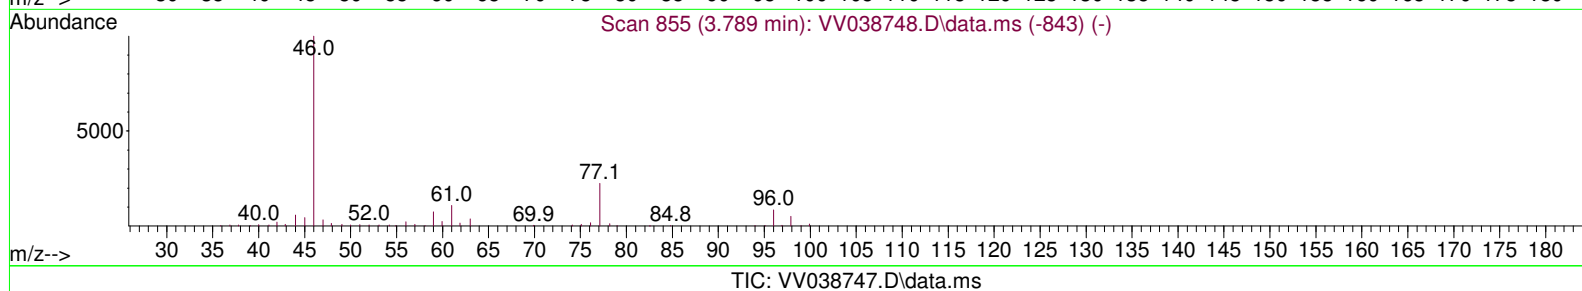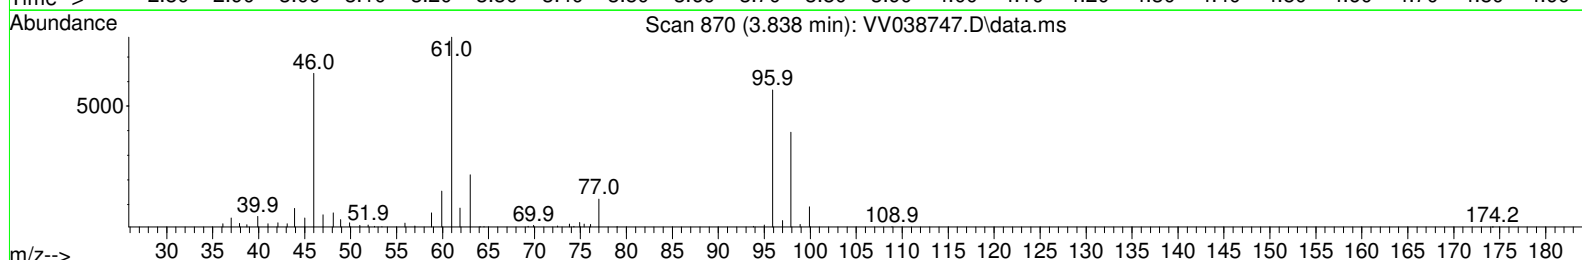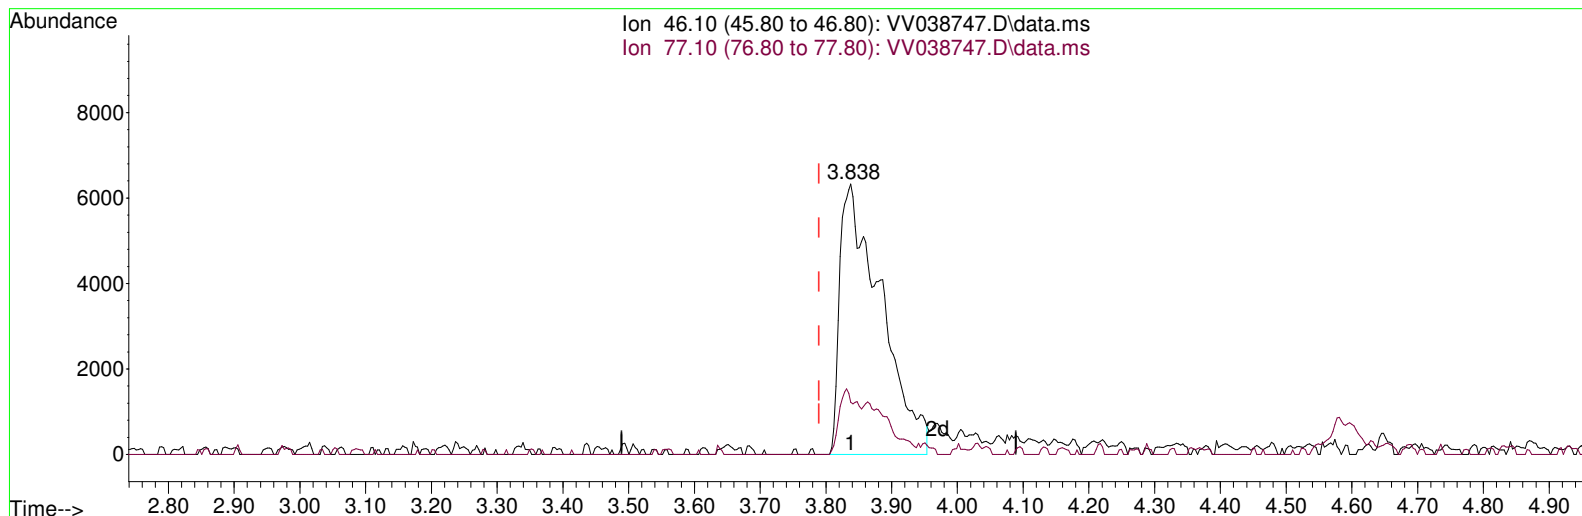

(20) 2-Butanone-d5 (S)

3.838min (+ 0.048) 7.21 ug/L m

response 27407

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	23.70	7.61#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038747.D
Acq On : 04 Jun 2025 15:21
Operator : SY/MD
Sample : VSTD00142
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001242

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 08:29:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 08:29:01 2025
Response via : Initial Calibration

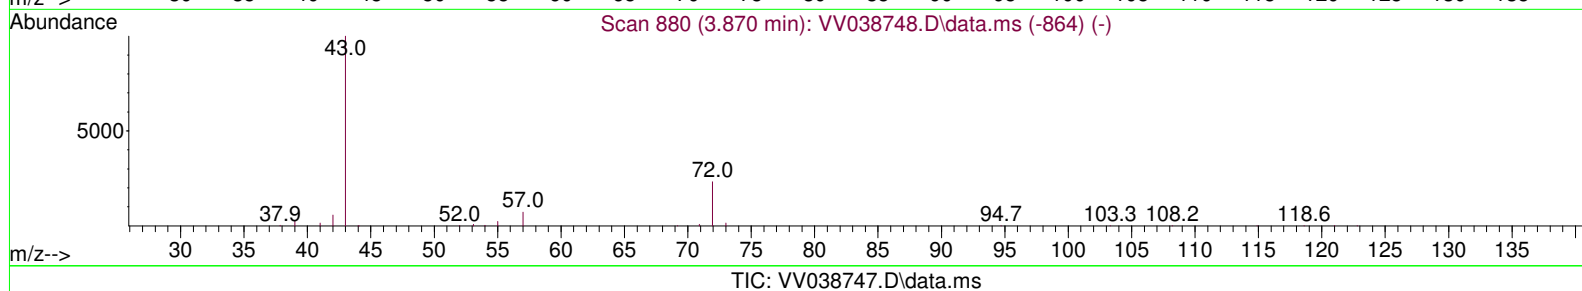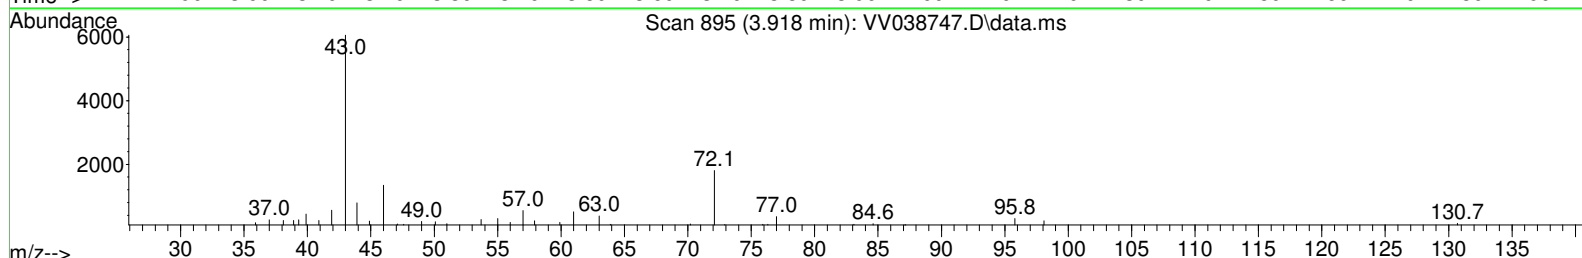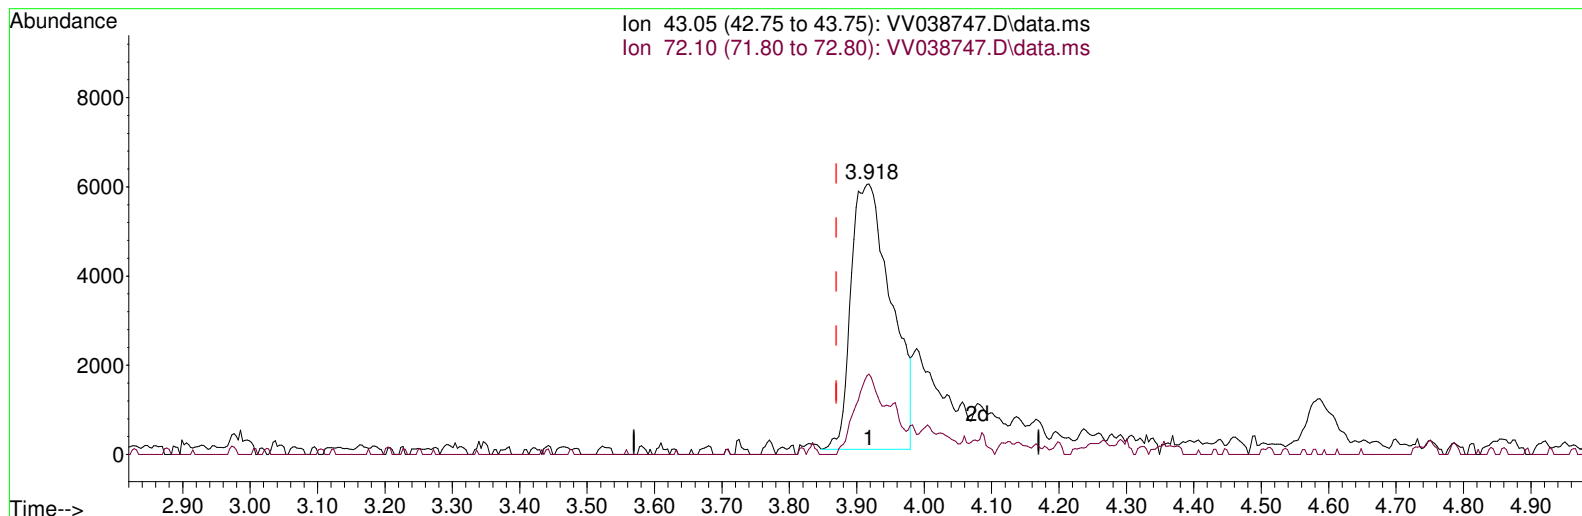

(21) 2-Butanone (T)

3.918min (+ 0.048) 5.78 ug/L

response 24534

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.70	18.68
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038747.D
Acq On : 04 Jun 2025 15:21
Operator : SY/MD
Sample : VSTD00142
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001242

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 08:29:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 08:29:01 2025
Response via : Initial Calibration

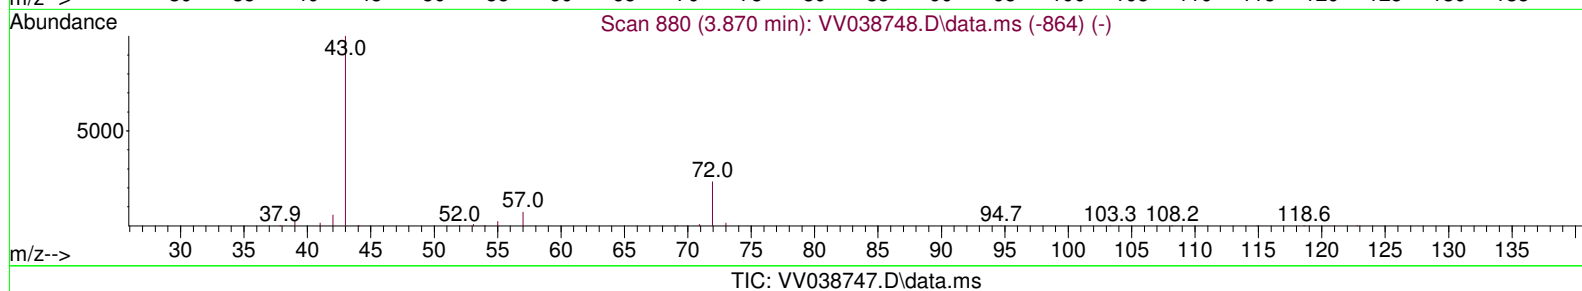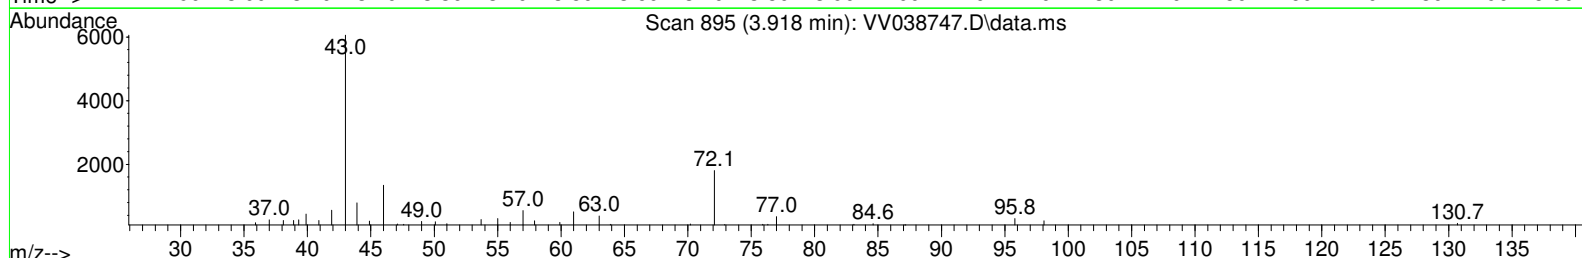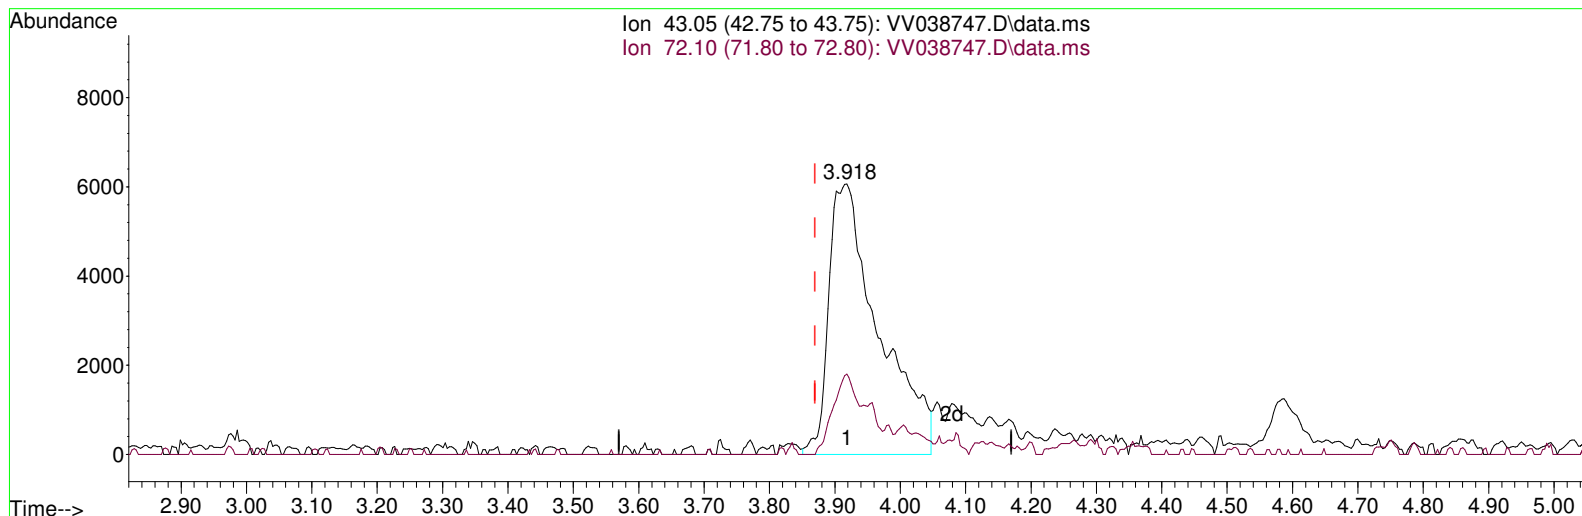

(21) 2-Butanone (T)

3.918min (+ 0.048) 7.57 ug/L m

response 32120

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.70	14.27
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038747.D
Acq On : 04 Jun 2025 15:21
Operator : SY/MD
Sample : VSTD00142
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001242

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 08:29:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 08:29:01 2025
Response via : Initial Calibration

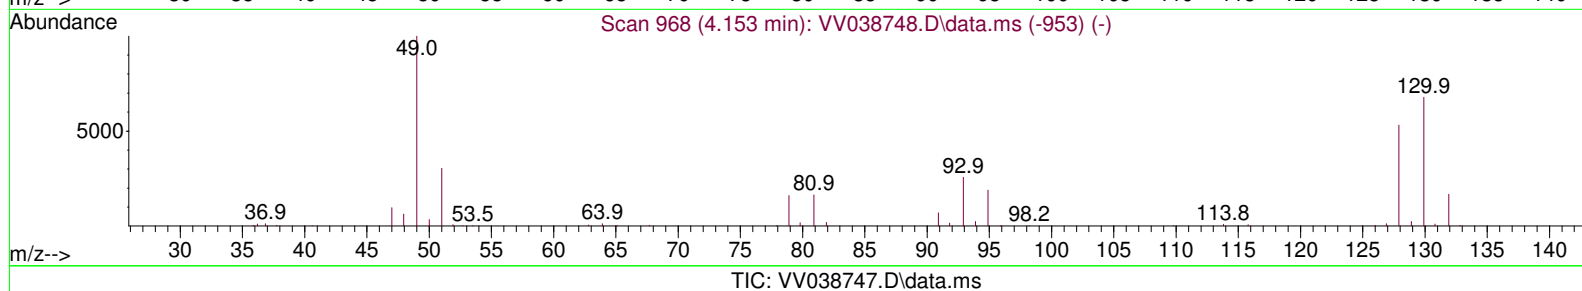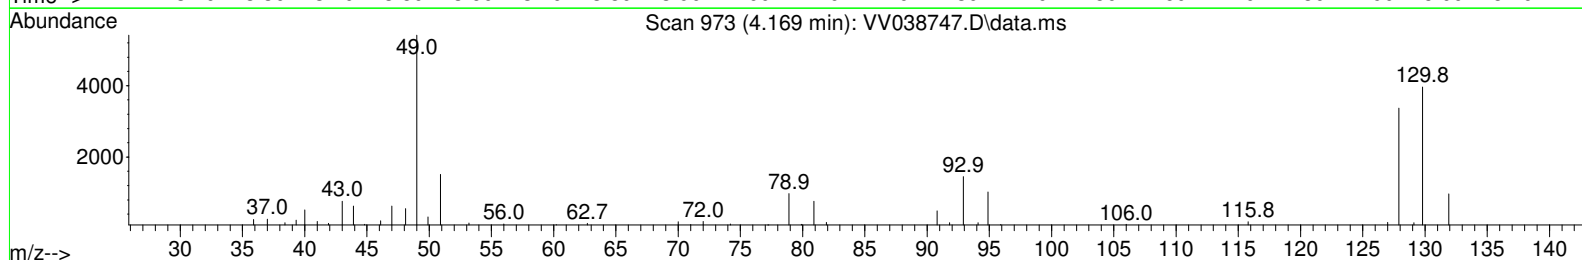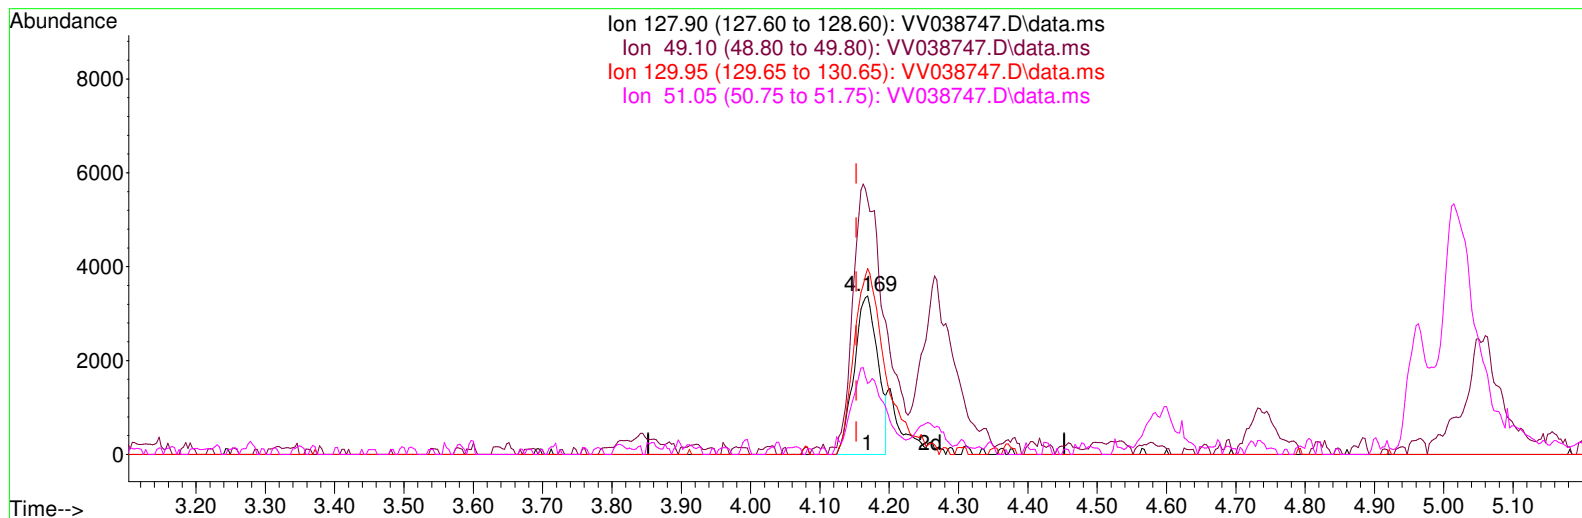

(23) Bromochloromethane (T)

4.169min (+ 0.016) 0.84 ug/L

response 8072

Ion	Exp%	Act%
127.90	100.00	100.00
49.10	165.70	160.74
129.95	128.90	117.44
51.05	54.30	44.90




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038747.D
Acq On : 04 Jun 2025 15:21
Operator : SY/MD
Sample : VSTD00142
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001242

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 08:29:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 08:29:01 2025
Response via : Initial Calibration

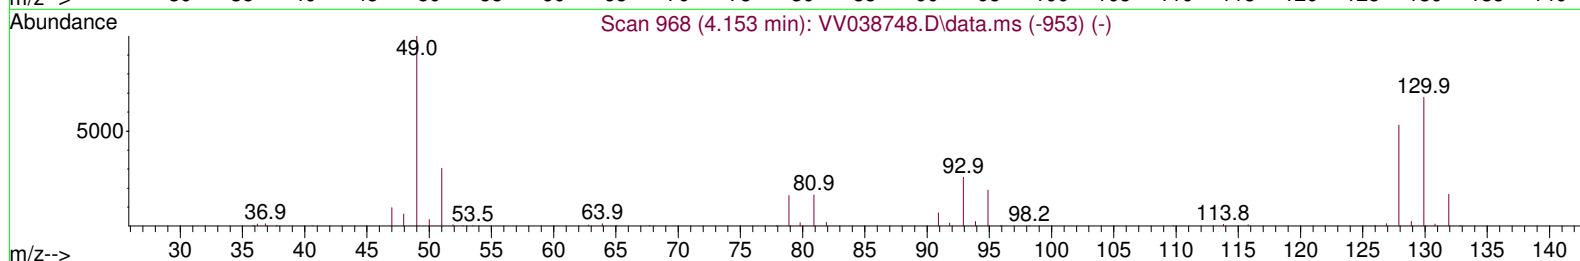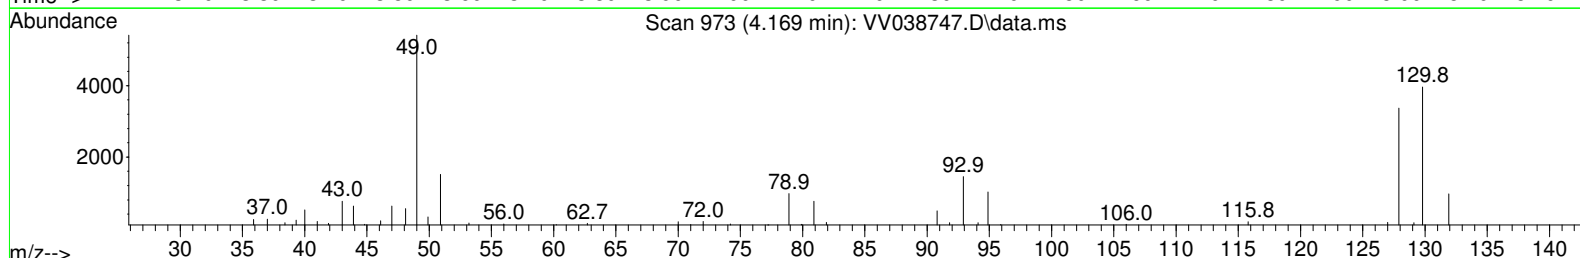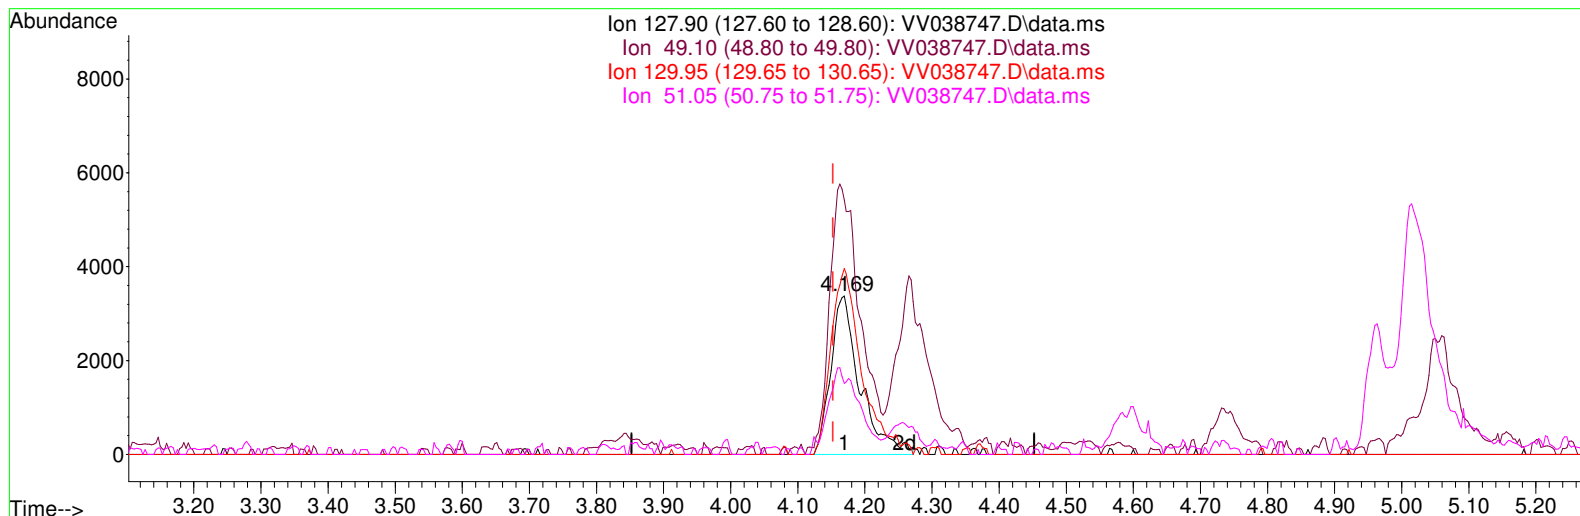

TIC: VV038747.D\data.ms

(23) Bromochloromethane (T)

4.169min (+ 0.016) 1.07 ug/L m

response 10245

Ion	Exp%	Act%
127.90	100.00	100.00
49.10	165.70	160.74
129.95	128.90	117.44
51.05	54.30	44.90




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038747.D
Acq On : 04 Jun 2025 15:21
Operator : SY/MD
Sample : VSTD00142
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001242

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 08:29:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 08:29:01 2025
Response via : Initial Calibration

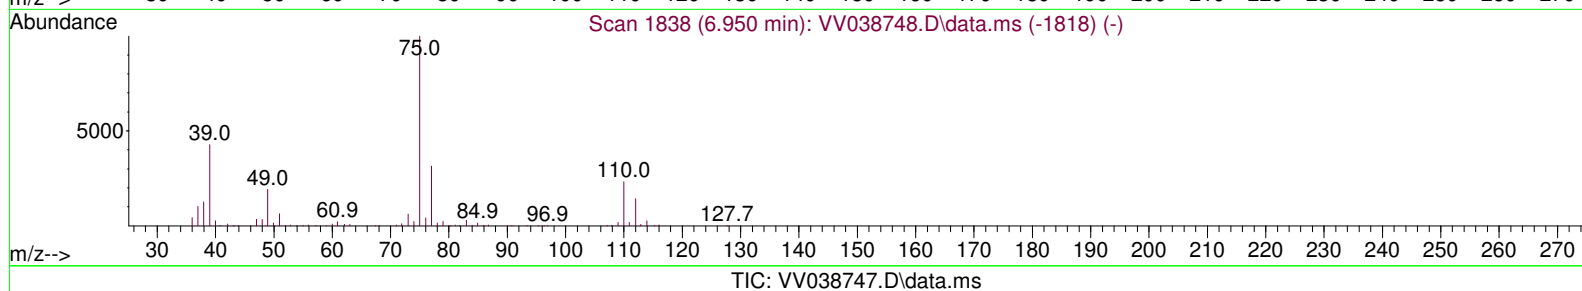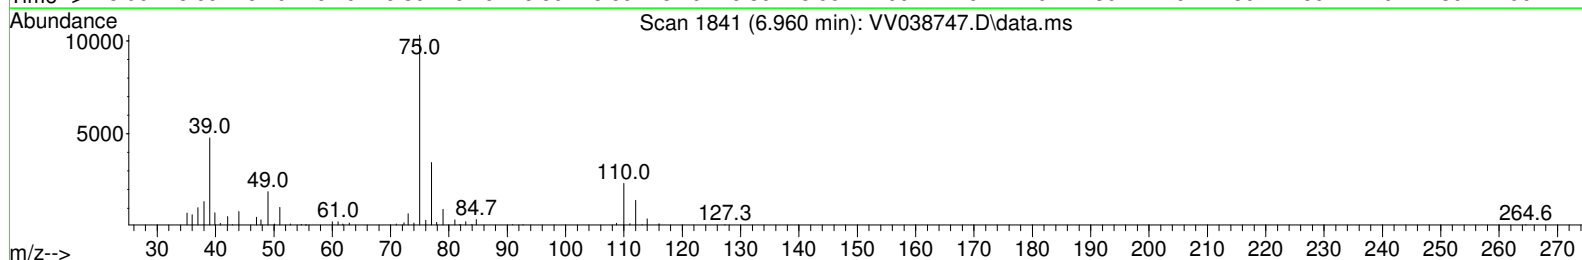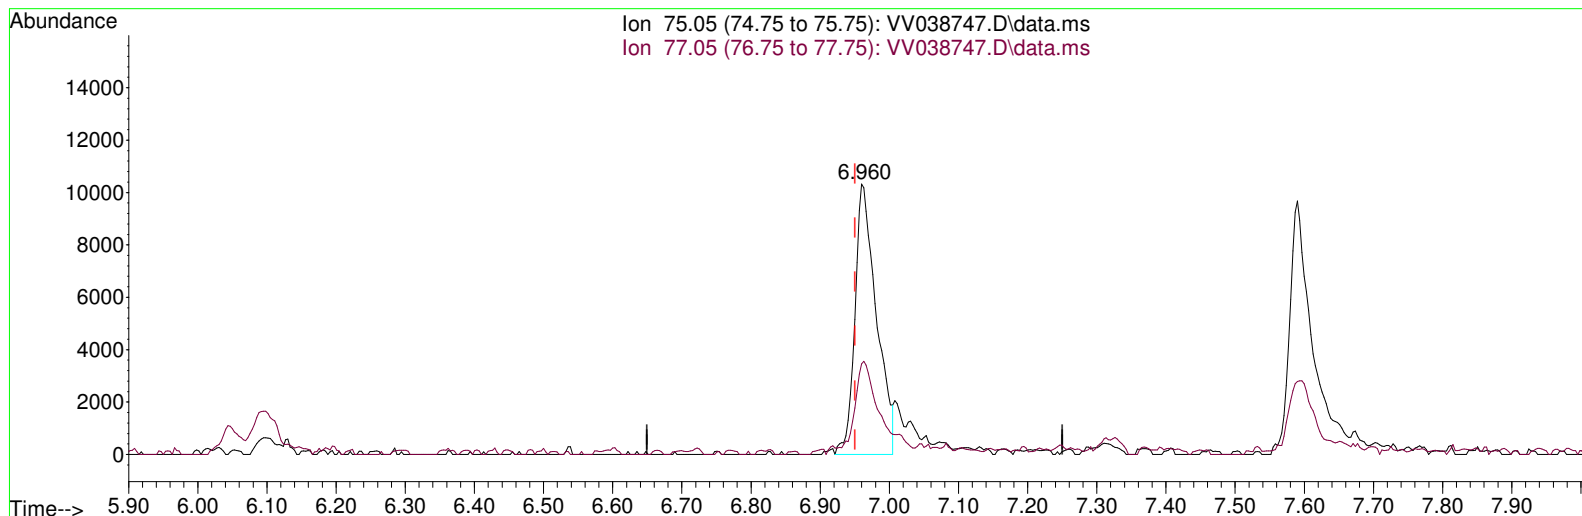

(39) cis-1,3-Dichloropropene (T)

6.960min (+ 0.010) 0.75 ug/L

response 22226

Ion	Exp%	Act%
75.05	100.00	100.00
77.05	30.40	33.49
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038747.D
Acq On : 04 Jun 2025 15:21
Operator : SY/MD
Sample : VSTD00142
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001242

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 08:29:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 08:29:01 2025
Response via : Initial Calibration

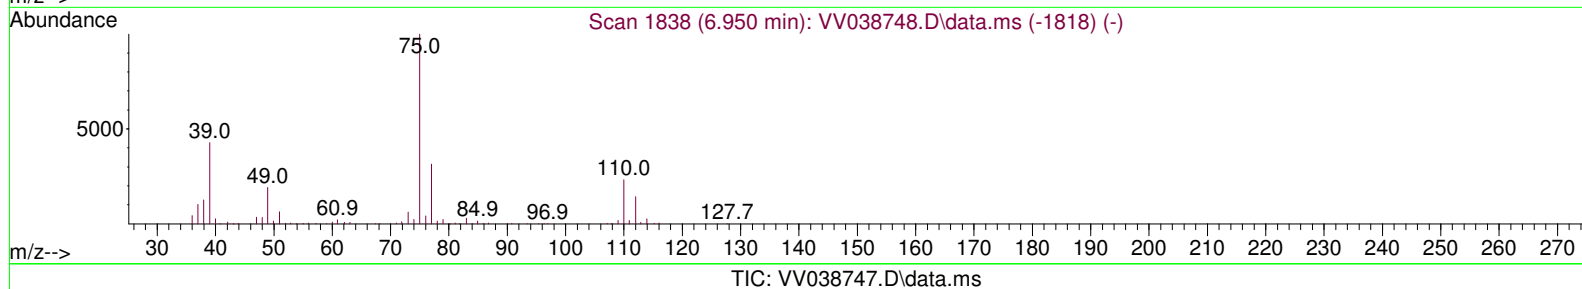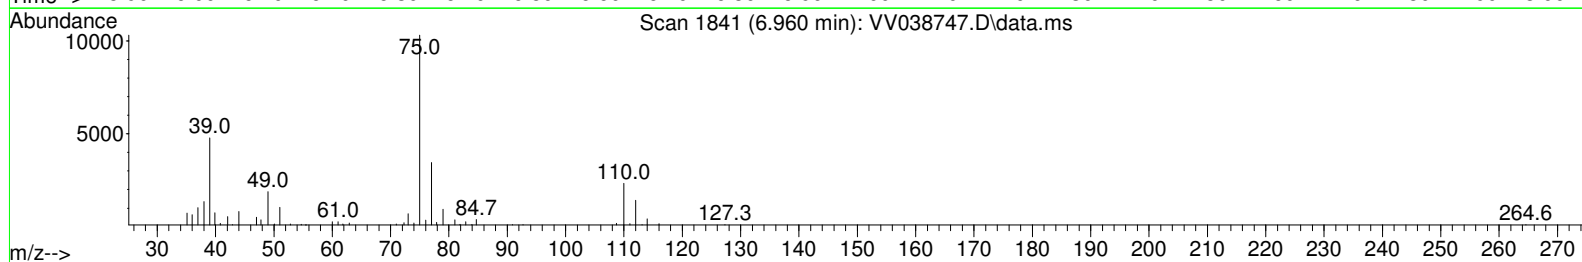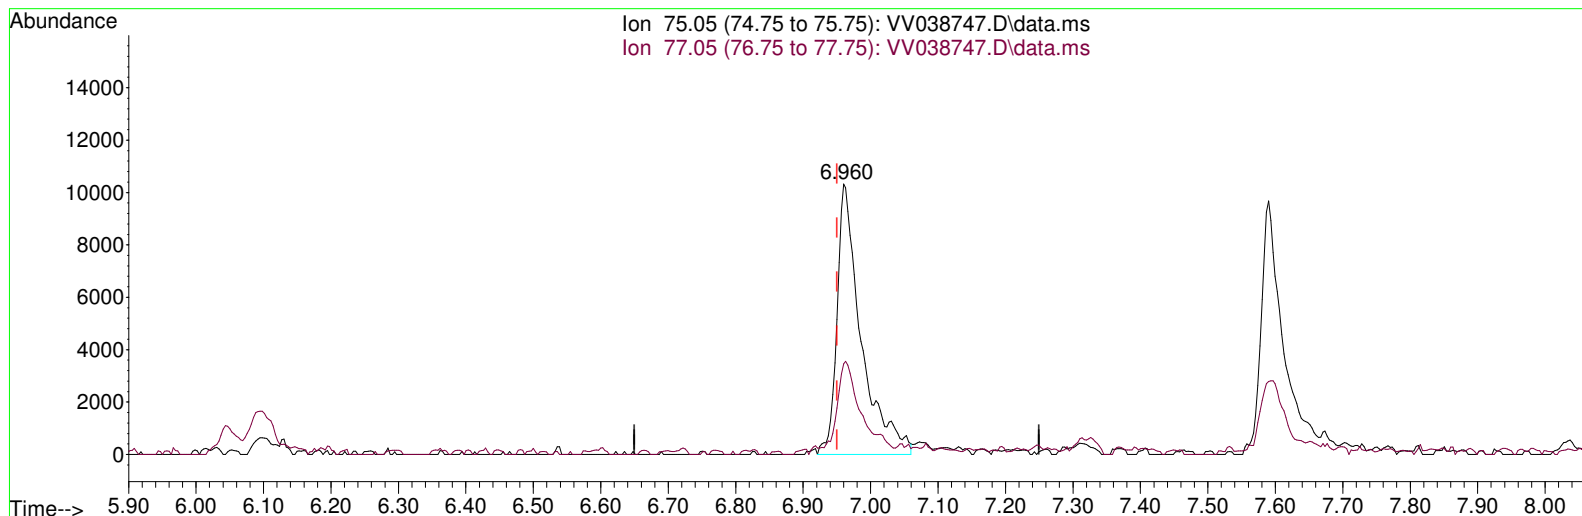

(39) cis-1,3-Dichloropropene (T)

6.960min (+ 0.010) 0.87 ug/L m

response 25681

Ion	Exp%	Act%
75.05	100.00	100.00
77.05	30.40	33.49
0.00	0.00	0.00
0.00	0.00	0.00