




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038748.D
Acq On : 04 Jun 2025 15:57
Operator : SY/MD
Sample : VSTD00543
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD005243

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/06/2025

Quant Time: Jun 06 12:40:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 05 08:49:01 2025
Response via : Initial Calibration

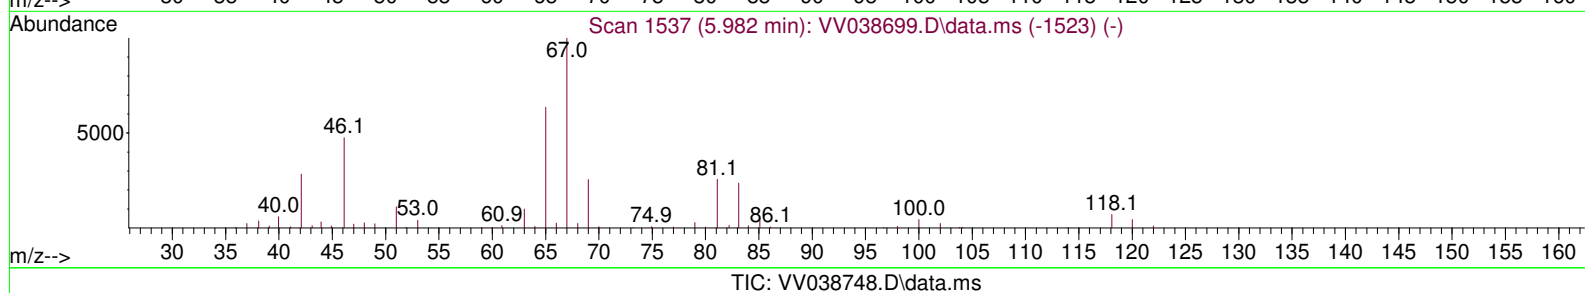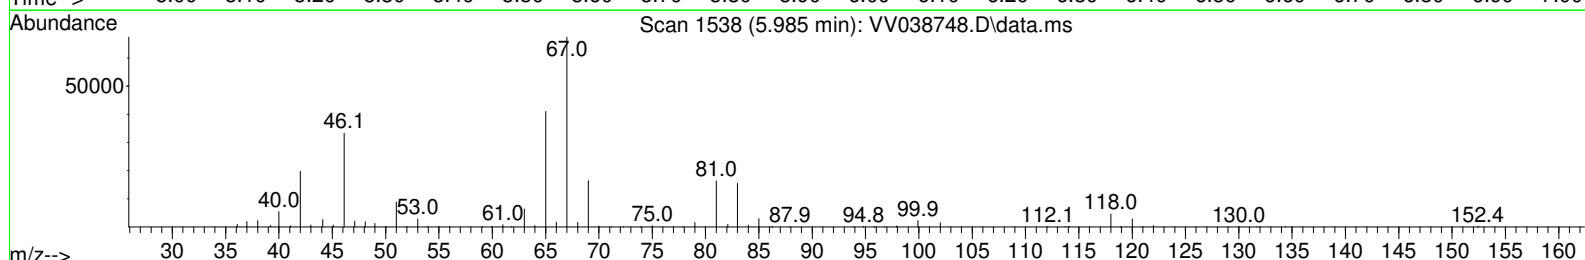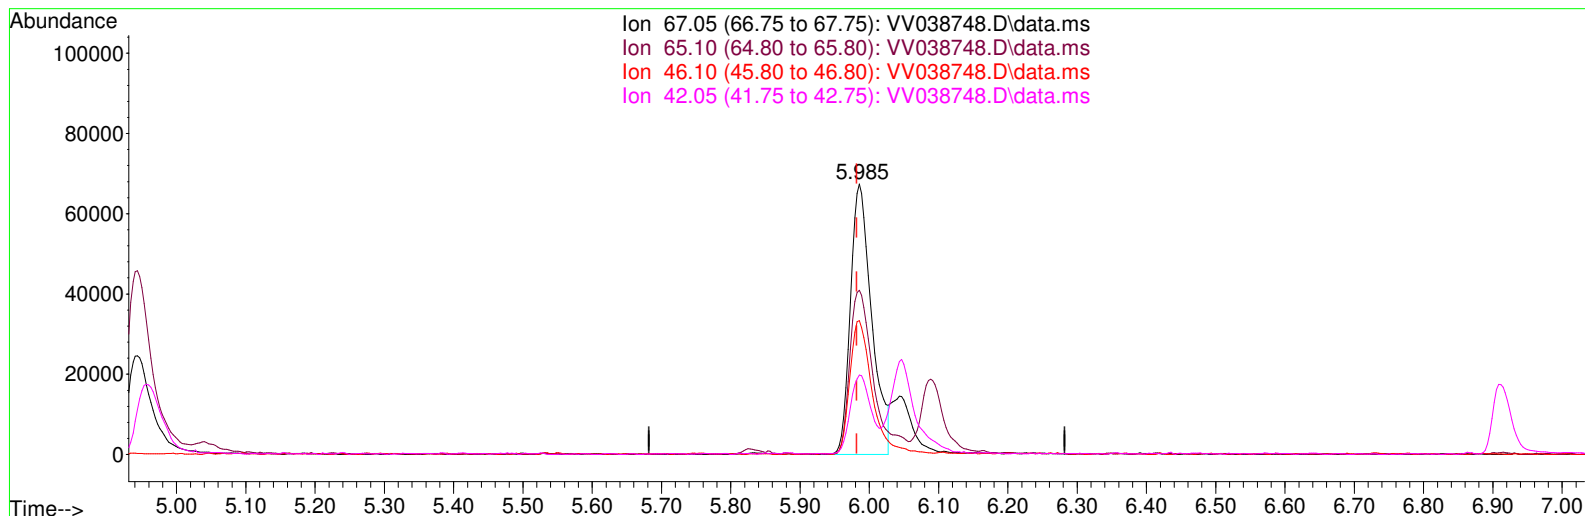

(36) 1,2-Dichloropropane-d6 (S)

5.985min (+ 0.003) 7.07 ug/L

response 143819

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	69.80	68.14
46.10	50.70	52.36
42.05	27.70	28.44




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038748.D
Acq On : 04 Jun 2025 15:57
Operator : SY/MD
Sample : VSTD00543
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD005243

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/06/2025

Quant Time: Jun 06 12:40:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 05 08:49:01 2025
Response via : Initial Calibration

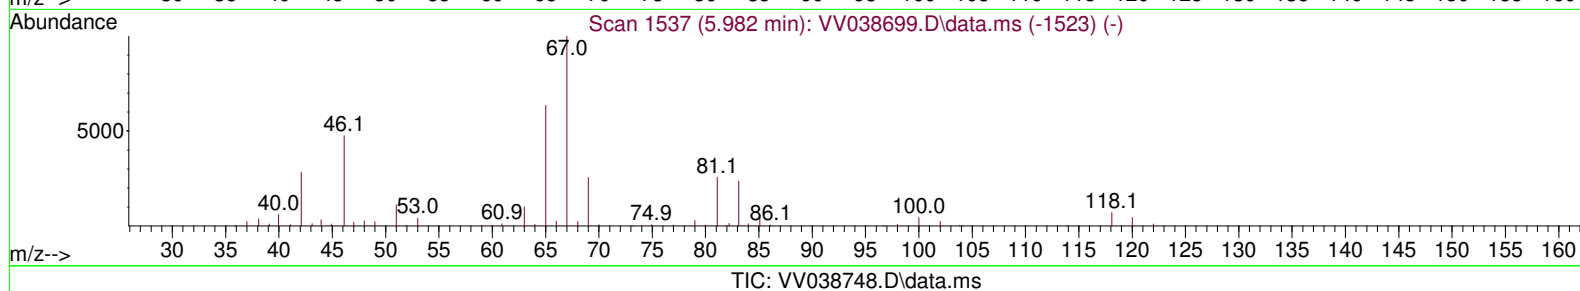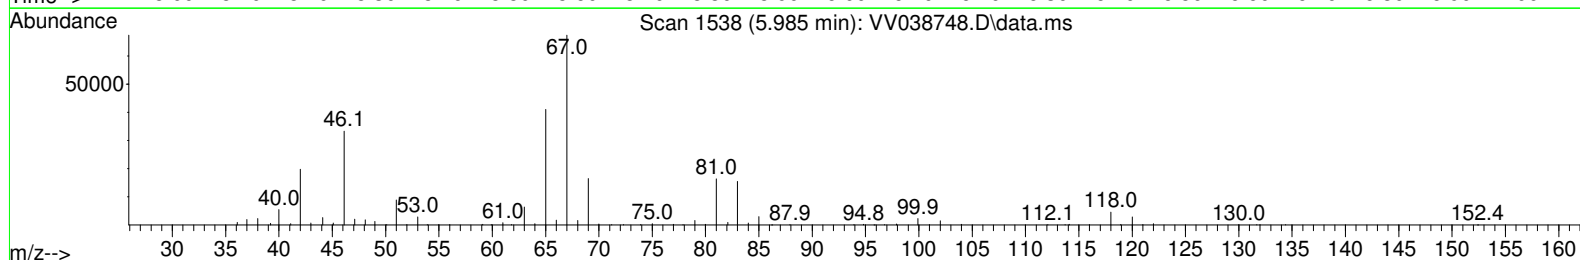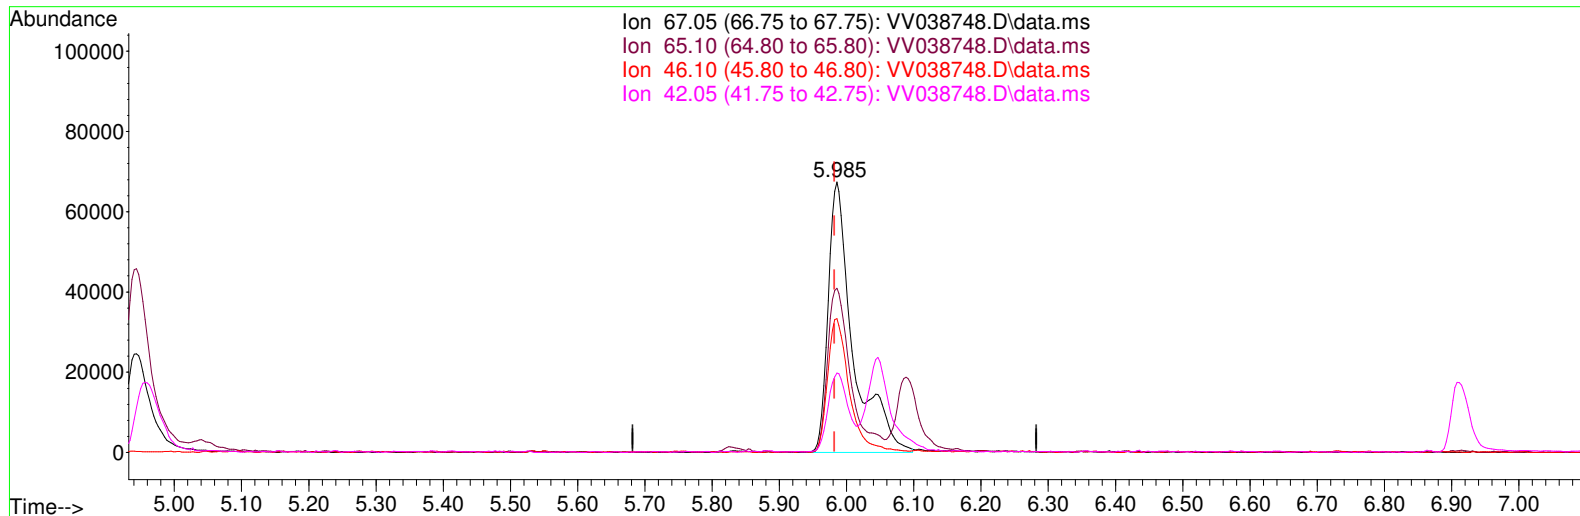

(36) 1,2-Dichloropropane-d6 (S)

5.985min (+ 0.003) 8.57 ug/L m

response 174509

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	69.80	56.15
46.10	50.70	43.15
42.05	27.70	23.44