




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038749.D
Acq On : 04 Jun 2025 16:19
Operator : SY/MD
Sample : VSTD01044
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD010244

Manual IntegrationsAPPROVED

Quant Time: Jun 06 08:59:57 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 05 08:49:01 2025
Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/06/2025

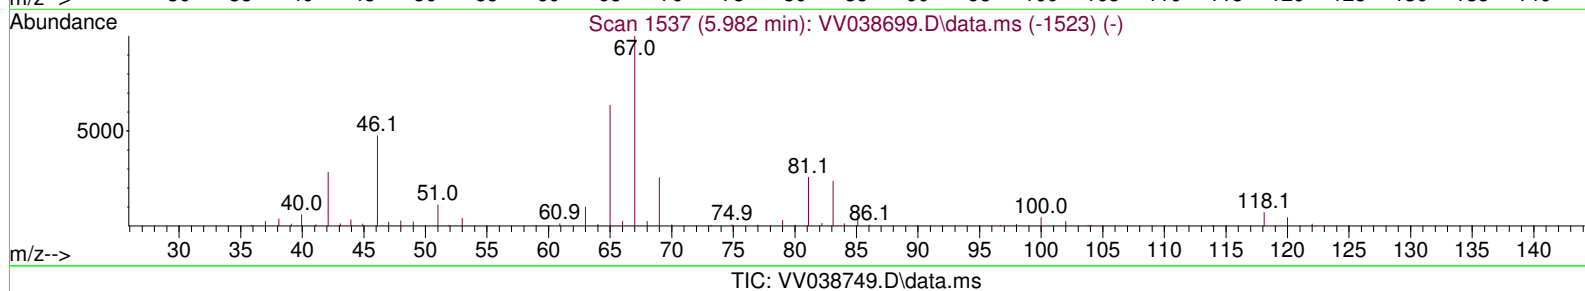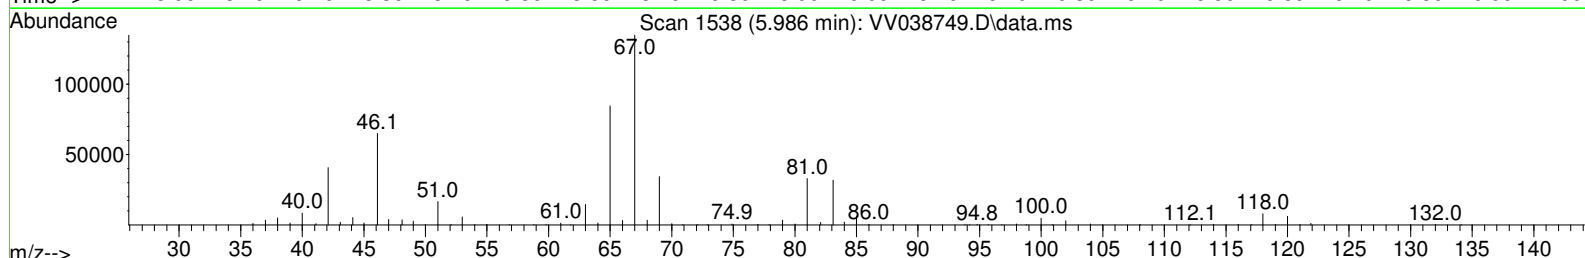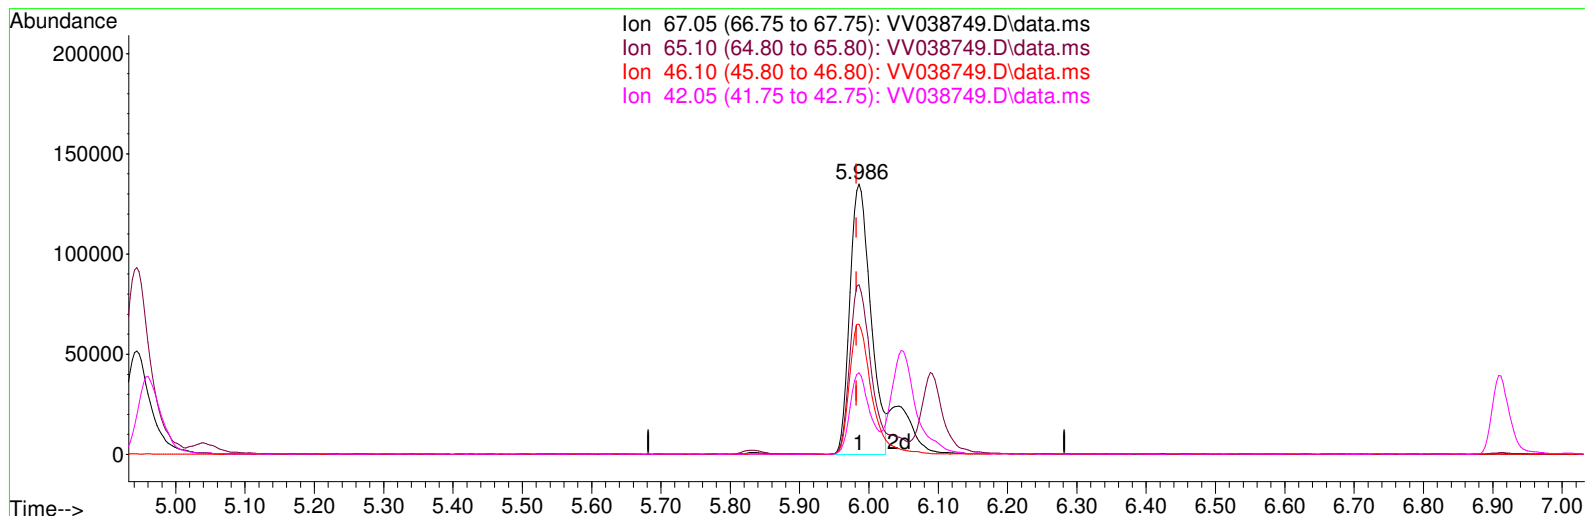

(36) 1,2-Dichloropropane-d6 (S)

5.986min (+ 0.004) 13.70 ug/L

response 284525

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	69.80	68.24
46.10	50.70	51.21
42.05	27.70	28.73




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038749.D
Acq On : 04 Jun 2025 16:19
Operator : SY/MD
Sample : VSTD01044
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD010244

Manual IntegrationsAPPROVED

Quant Time: Jun 06 08:59:57 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 05 08:49:01 2025
Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/06/2025

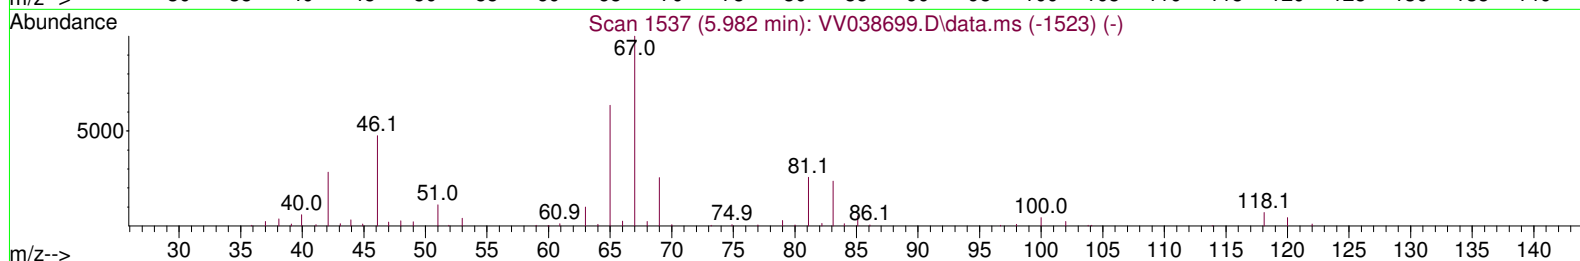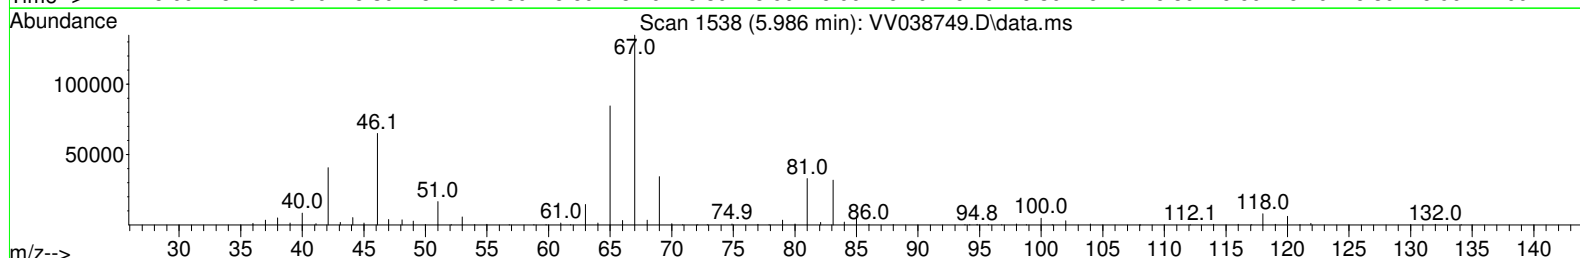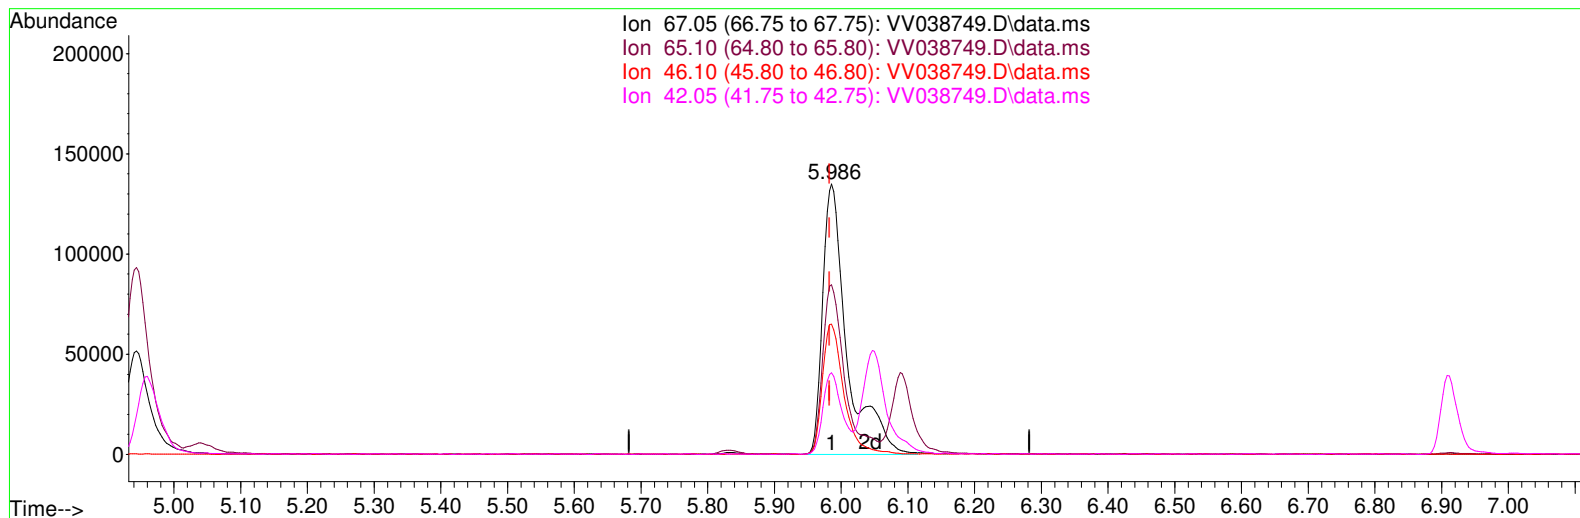

TIC: VV038749.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

5.986min (+ 0.004) 16.55 ug/L m

response 343594

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	69.80	56.51
46.10	50.70	42.40
42.05	27.70	23.79