




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038750.D
Acq On : 04 Jun 2025 16:40
Operator : SY/MD
Sample : VSTD02045
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD02045

Manual IntegrationsAPPROVED

Quant Time: Jun 06 09:00:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 05 08:49:01 2025
Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/06/2025

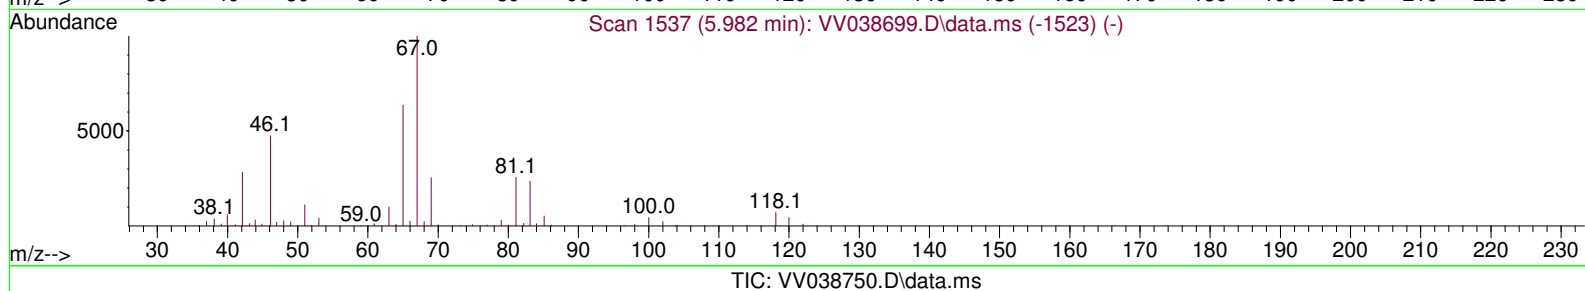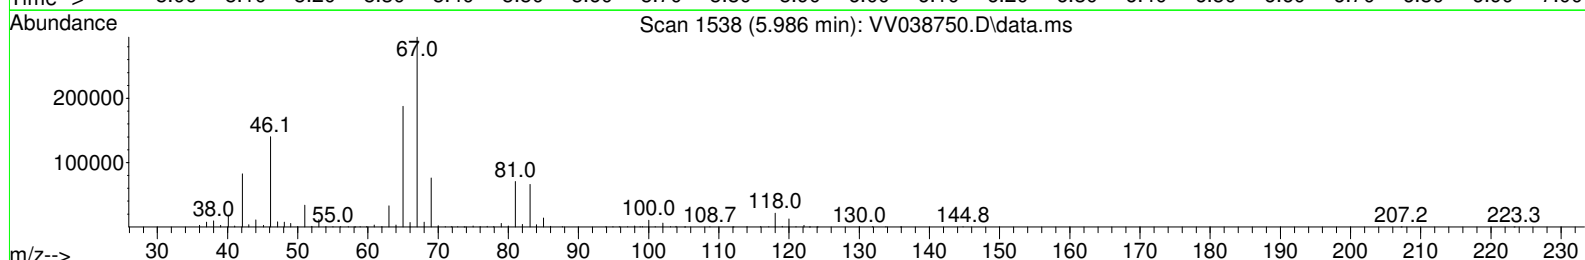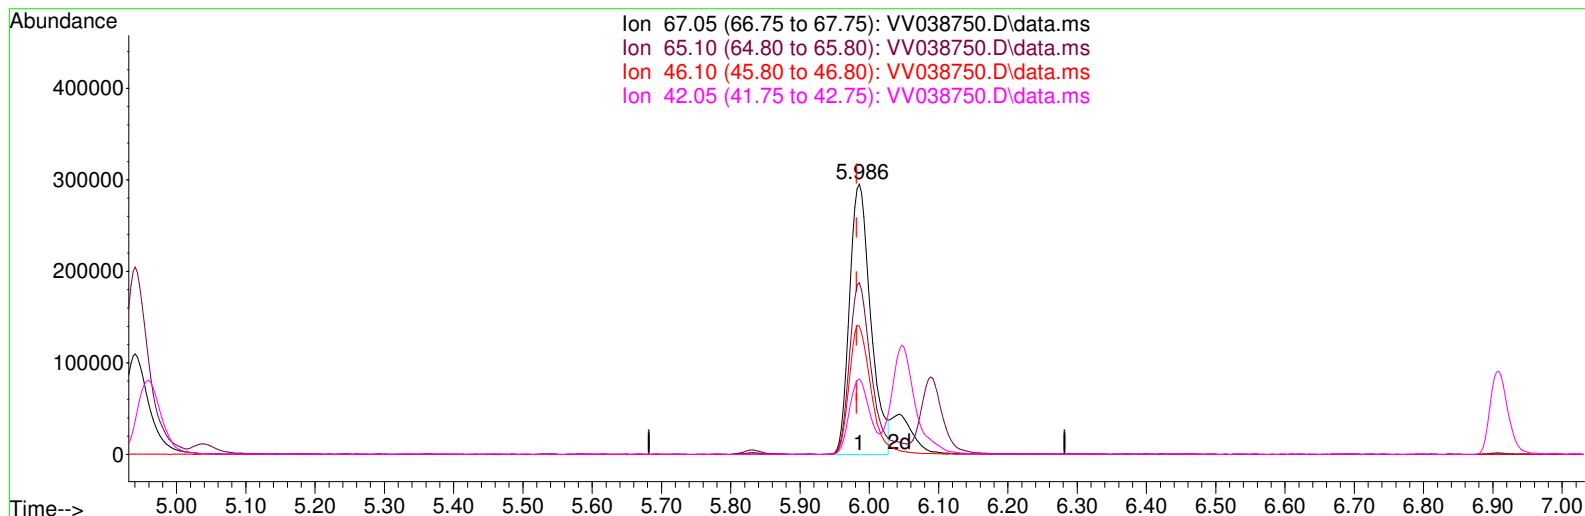

(36) 1,2-Dichloropropane-d6 (S)

5.986min (+ 0.004) 28.53 ug/L

response 626068

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	69.80	66.95
46.10	50.70	49.50
42.05	27.70	26.98




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038750.D
Acq On : 04 Jun 2025 16:40
Operator : SY/MD
Sample : VSTD02045
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD020245

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/06/2025

Quant Time: Jun 06 09:00:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 05 08:49:01 2025
Response via : Initial Calibration

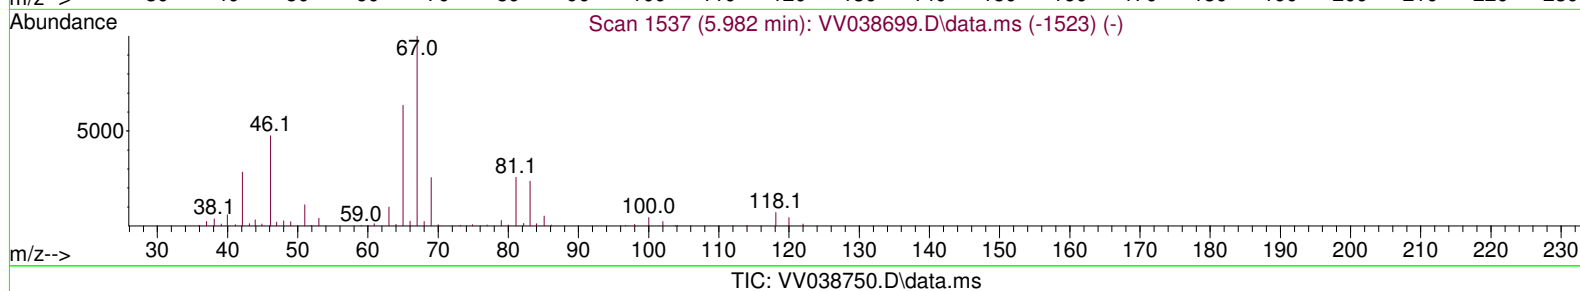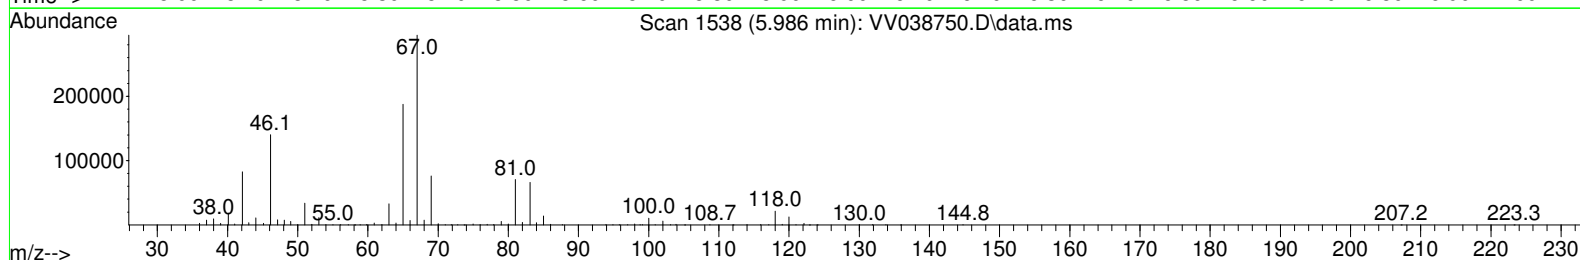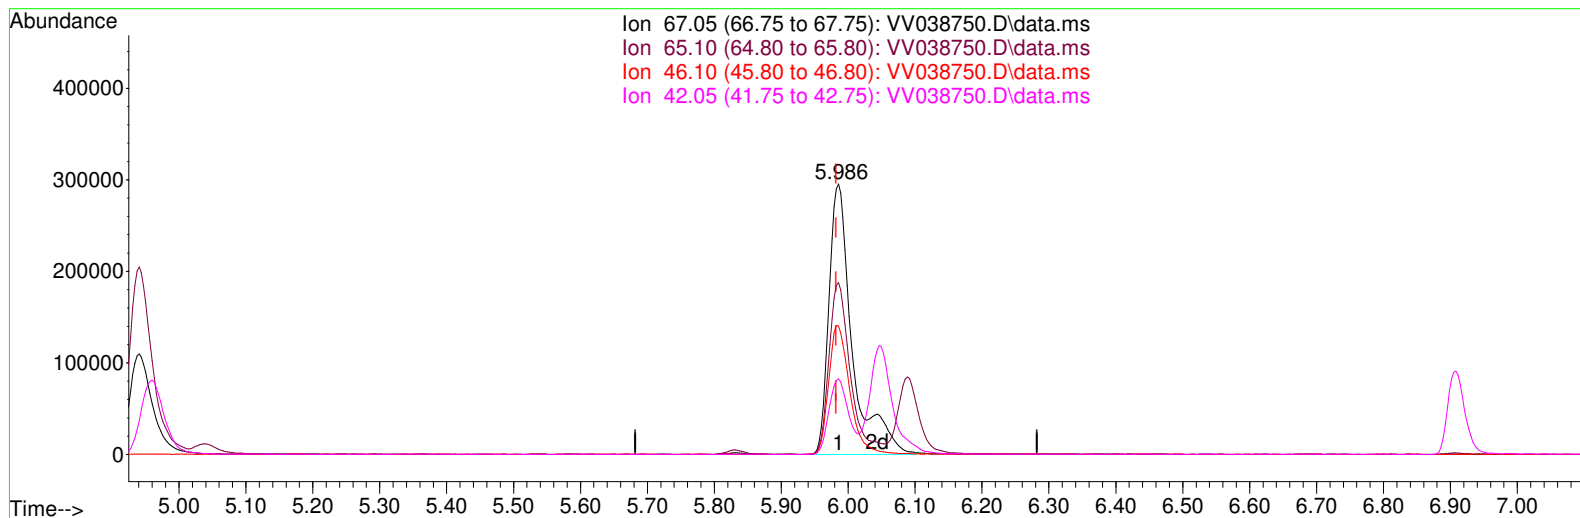

(36) 1,2-Dichloropropane-d6 (S)

5.986min (+ 0.004) 32.85 ug/L m

response 721049

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	69.80	58.13
46.10	50.70	42.98
42.05	27.70	23.42