




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038751.D
Acq On : 04 Jun 2025 17:24
Operator : SY/MD
Sample : VSTDICV005
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VICV246

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/06/2025

Quant Time: Jun 06 13:12:31 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 06 12:50:11 2025
Response via : Initial Calibration

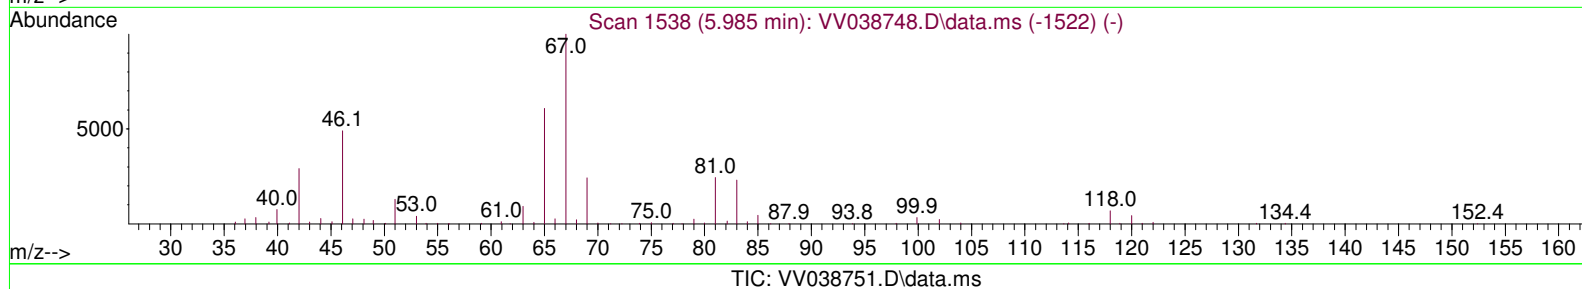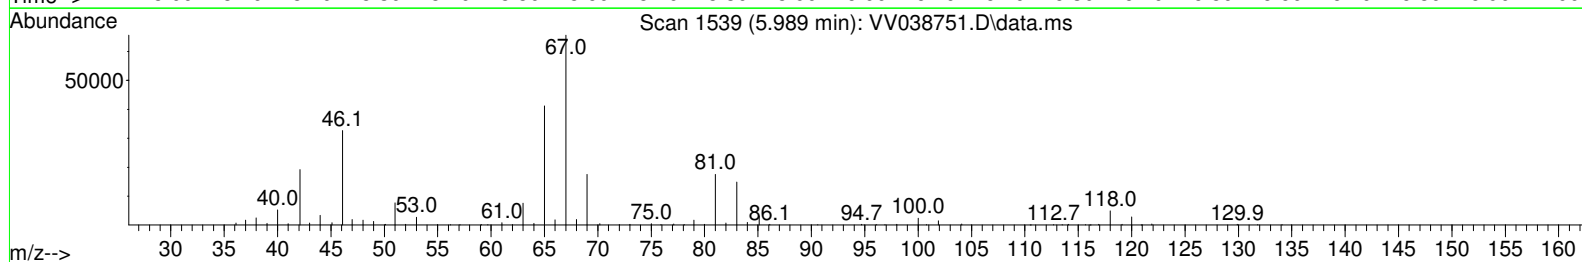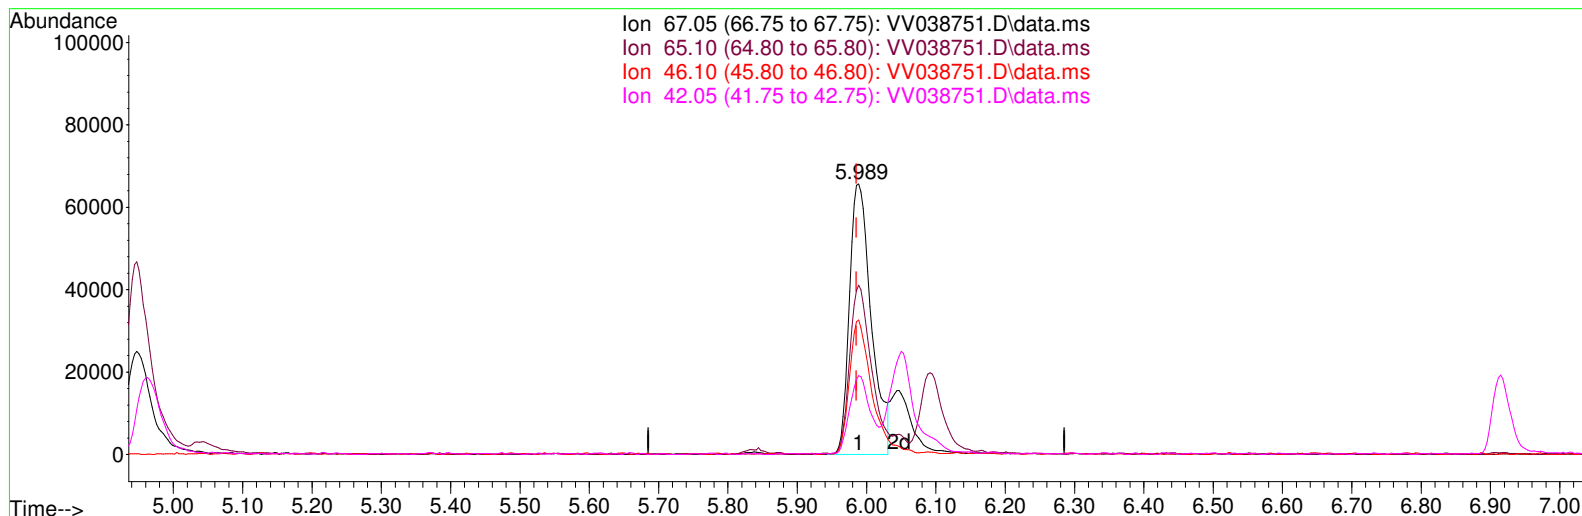

(36) 1,2-Dichloropropane-d6 (S)

5.989min (+ 0.003) 3.91 ug/L

response 143300

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	69.80	62.61
46.10	50.70	50.85
42.05	27.70	27.27




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038751.D
Acq On : 04 Jun 2025 17:24
Operator : SY/MD
Sample : VSTDICV005
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VICV246

Manual IntegrationsAPPROVED

Quant Time: Jun 06 13:12:31 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 06 12:50:11 2025
Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/06/2025

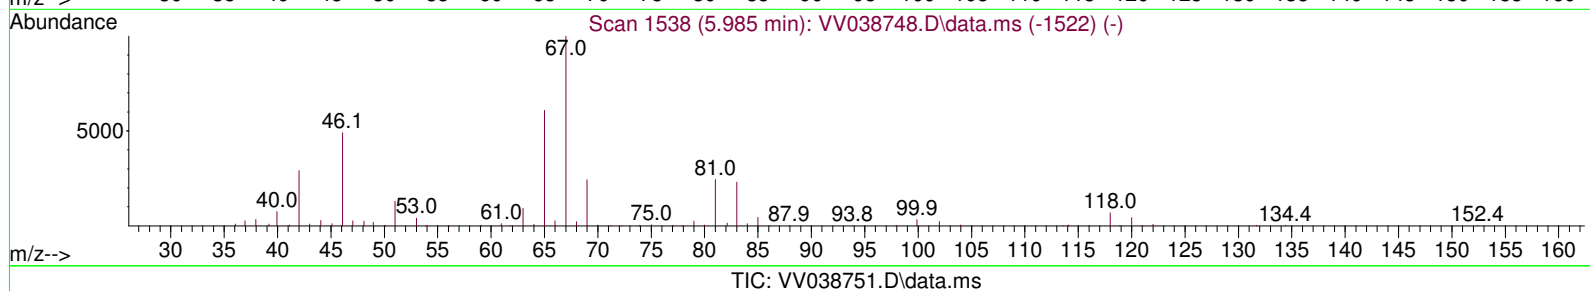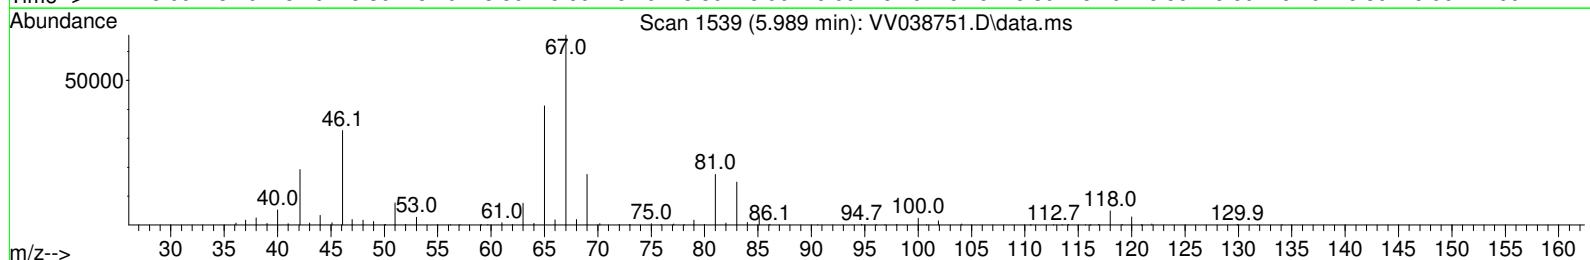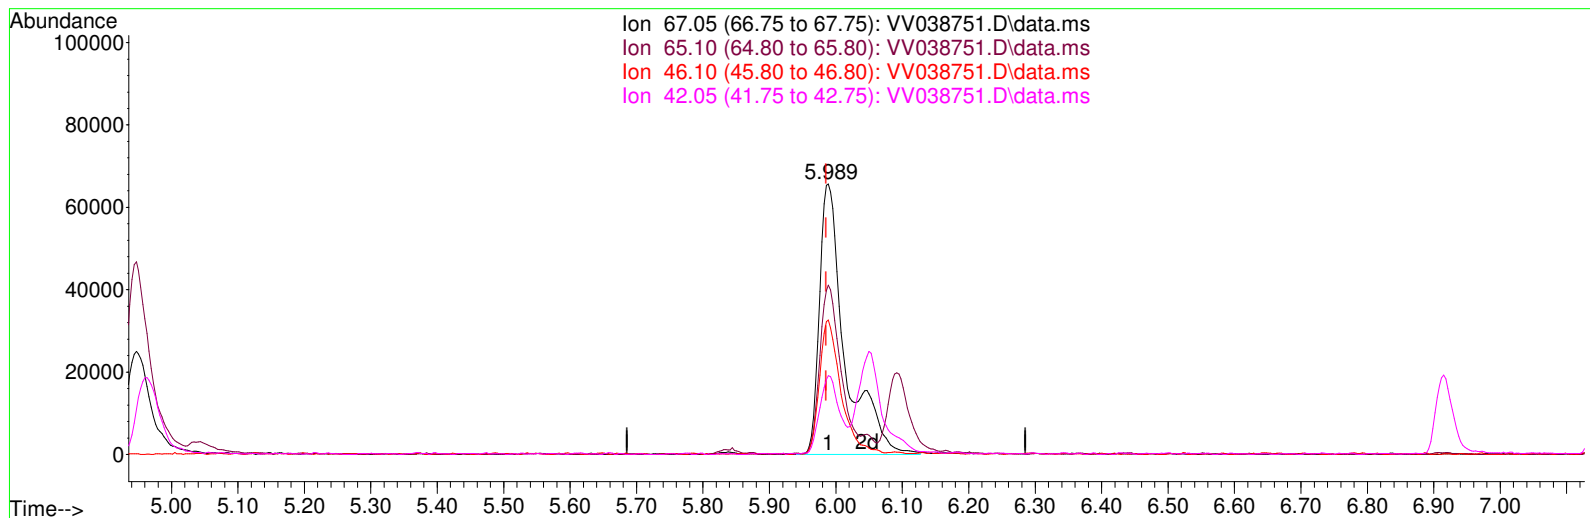

(36) 1,2-Dichloropropane-d6 (S)

5.989min (+ 0.003) 4.81 ug/L m

response 176653

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	69.80	50.79
46.10	50.70	41.25
42.05	27.70	22.12