
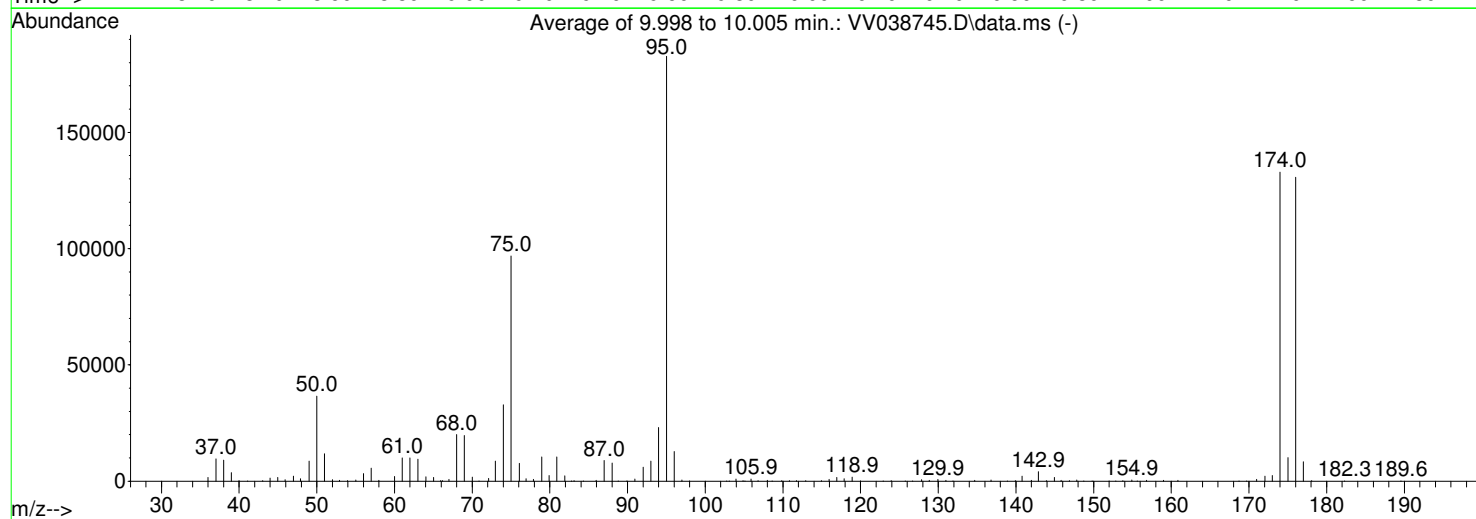


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060425\
Data File : VV038745.D
Acq On : 04 Jun 2025 14:09
Operator : SY/MD
Sample : BFB206
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB206

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jun 13 08:57:28 2025

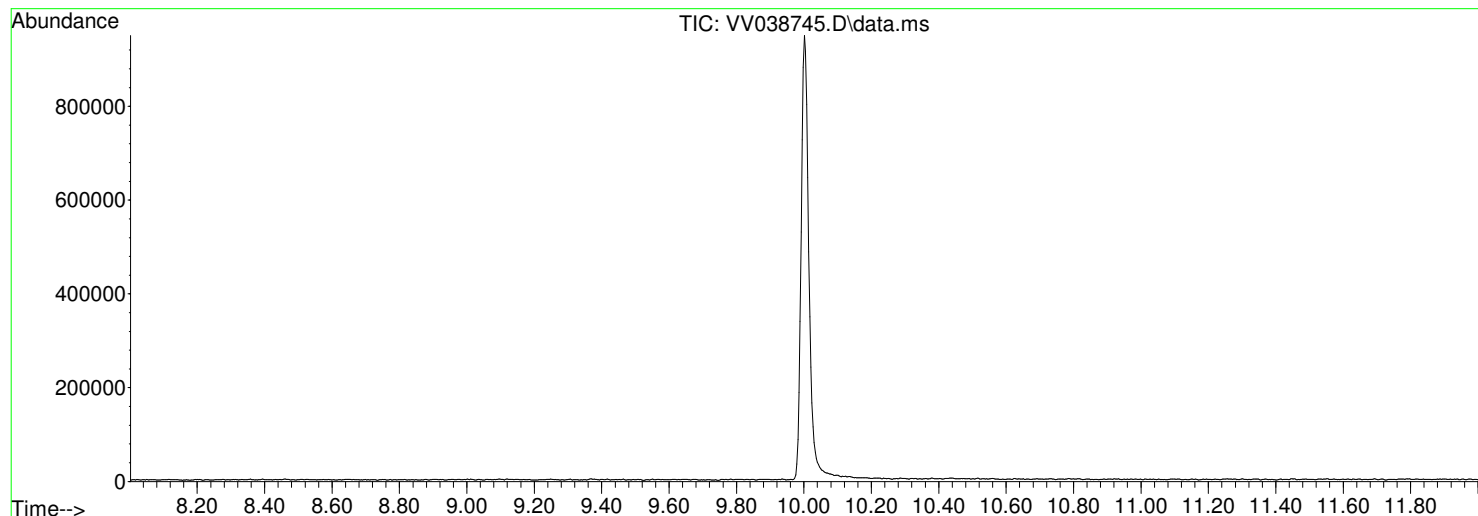

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	36602	PASS
75	95	30	80	53.0	96827	PASS
95	95	100	100	100.0	182699	PASS
96	95	5	9	7.0	12709	PASS
173	174	0.00	2	1.8	2378	PASS
174	95	50	120	72.8	132931	PASS
175	174	5	9	7.6	10068	PASS
176	174	95	105	98.3	130717	PASS
177	176	5	10	6.4	8360	PASS

m/z	Abundance
36.00	201.0
37.60	132.0
38.00	171.0
40.10	368.0
41.60	166.0
42.20	142.0
44.00	767.0
44.90	122.0
45.60	107.0
46.30	128.0
47.00	159.0
47.90	124.0
48.40	141.0
50.10	118.0
50.70	105.0
52.90	109.0
53.60	120.0
54.20	103.0
55.10	123.0
58.40	113.0
62.10	114.0
65.70	131.0
74.80	127.0
76.90	130.0
78.20	135.0
85.80	104.0
89.60	148.0
115.20	107.0
118.30	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	1741.0
37.00	9132.0
38.00	8849.0
39.00	3562.0
40.10	560.0
41.80	179.0
42.30	112.0
43.00	156.0
44.00	1976.0
45.00	1581.0
45.90	592.0
47.00	2341.0
48.00	1225.0
49.00	8313.0
50.00	36256.0
51.00	11245.0
52.00	674.0
52.90	419.0
53.90	232.0
55.00	565.0
56.00	3401.0
57.00	5523.0
58.00	351.0
60.00	2075.0
61.00	9883.0
62.00	10073.0
63.00	9453.0
64.00	1866.0
65.10	1508.0
66.00	231.0
67.00	709.0
68.00	19528.0
69.00	18960.0
70.00	1770.0
72.10	1135.0
73.00	8488.0
74.00	32000.0
75.00	94112.0
76.10	7692.0
76.90	1303.0
77.90	816.0
79.00	10173.0
79.90	2466.0
80.90	10046.0
81.90	2088.0
82.80	179.0
84.30	116.0
86.00	320.0
87.00	8576.0
88.00	7700.0
88.80	202.0
90.90	808.0
92.00	5788.0
93.00	8361.0
94.00	22432.0
95.00	176960.0
96.00	12176.0
97.00	460.0
102.80	135.0
103.90	717.0
104.80	208.0
105.10	191.0
105.90	875.0
106.80	168.0
108.00	251.0
108.60	164.0
109.90	196.0
110.90	258.0
111.80	183.0
112.90	198.0
115.00	258.0
115.90	749.0
116.90	1697.0
117.90	853.0
118.90	1640.0
120.00	134.0
122.90	134.0
123.90	142.0
125.80	129.0
126.70	150.0
127.80	555.0
128.80	350.0
130.00	660.0
131.00	265.0
131.90	156.0
134.70	299.0
136.80	401.0
139.80	163.0
140.80	2125.0
142.00	313.0
142.90	3822.0
143.90	218.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

144.90	1621.0
145.80	360.0
147.10	206.0
147.90	457.0
148.80	124.0
152.80	107.0
153.70	108.0
154.90	449.0
155.60	122.0
156.80	367.0
159.00	283.0
160.80	274.0
169.70	143.0
171.00	603.0
172.00	1931.0
173.00	2256.0
174.00	126152.0
175.00	9201.0
176.00	121688.0
177.00	8115.0
178.10	153.0
182.30	146.0
189.60	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	1800.0
37.00	9977.0
38.00	9546.0
39.00	3747.0
40.00	650.0
41.80	180.0
42.30	122.0
43.10	192.0
44.10	2083.0
45.00	1735.0
45.90	621.0
47.00	2309.0
47.90	1187.0
49.00	8939.0
50.00	38312.0
51.00	12112.0
52.00	666.0
52.90	429.0
54.00	257.0
55.00	602.0
56.00	3414.0
57.00	5730.0
58.00	331.0
60.00	2177.0
61.00	10372.0
62.00	10434.0
63.00	9789.0
64.10	1898.0
65.10	1567.0
65.90	217.0
66.20	225.0
67.00	738.0
68.00	20744.0
69.00	20488.0
70.00	1723.0
72.10	1237.0
73.00	9086.0
74.00	34304.0
75.00	100640.0
76.10	7906.0
77.00	1253.0
77.90	802.0
78.90	10780.0
79.90	2559.0
80.90	10793.0
81.90	2389.0
83.10	255.0
84.30	147.0
86.00	408.0
87.00	9237.0
88.00	7984.0
89.90	110.0
90.90	870.0
92.00	6189.0
93.00	8814.0
94.00	23888.0
95.00	189248.0
96.00	13166.0
97.00	495.0
98.00	101.0
102.70	112.0
103.10	121.0
103.90	860.0
104.80	243.0
105.90	937.0
106.80	208.0
108.00	329.0
108.60	121.0
109.90	190.0
110.90	251.0
111.80	272.0
113.00	248.0
114.90	274.0
116.00	845.0
117.00	1656.0
117.90	1068.0
118.90	1760.0
120.00	110.0
124.00	163.0
125.80	136.0
127.90	623.0
128.90	403.0
129.90	762.0
131.00	364.0
131.90	120.0
134.70	353.0
136.80	478.0
139.90	157.0
140.80	2194.0
142.00	372.0
142.90	4233.0
143.90	218.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

145.00	1553.0
145.80	433.0
146.90	221.0
147.80	499.0
148.70	133.0
149.80	133.0
152.80	132.0
153.80	152.0
154.90	461.0
155.60	111.0
156.80	423.0
159.00	299.0
160.90	351.0
169.70	115.0
171.00	751.0
172.10	2244.0
173.00	2472.0
174.00	137728.0
175.00	10488.0
176.00	135360.0
177.00	8654.0
178.00	219.0
189.50	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	1658.0
37.00	9786.0
38.00	9045.0
39.00	3587.0
39.90	687.0
41.10	214.0
41.80	136.0
42.30	115.0
43.10	235.0
44.10	2137.0
45.00	1677.0
45.90	586.0
47.00	2201.0
47.90	1067.0
49.00	8450.0
50.00	35592.0
51.00	11906.0
52.00	614.0
52.90	364.0
54.00	338.0
55.00	564.0
56.00	3081.0
57.00	5328.0
58.00	279.0
60.00	1872.0
61.00	9830.0
62.00	9701.0
63.00	9155.0
64.00	1730.0
65.00	1549.0
65.90	211.0
66.20	223.0
67.00	742.0
68.00	19712.0
69.00	19360.0
70.00	1569.0
70.90	126.0
72.10	1142.0
73.00	8405.0
74.00	32344.0
75.00	95728.0
76.00	7444.0
77.10	1071.0
77.90	853.0
78.90	10374.0
79.90	2399.0
80.90	10470.0
81.90	2296.0
83.10	270.0
84.30	156.0
86.00	427.0
87.00	8808.0
88.00	7635.0
91.00	875.0
92.00	5819.0
93.00	8652.0
94.00	22936.0
95.00	181888.0
96.00	12786.0
97.00	474.0
102.70	122.0
104.00	929.0
104.90	280.0
105.90	980.0
106.80	262.0
108.00	338.0
109.80	213.0
110.80	238.0
111.70	297.0
113.00	242.0
114.90	280.0
116.00	762.0
117.00	1498.0
117.90	1065.0
118.90	1658.0
124.00	181.0
125.70	135.0
127.90	641.0
128.90	401.0
129.90	763.0
131.00	393.0
134.70	372.0
136.80	488.0
138.90	131.0
140.00	177.0
140.80	1996.0
142.00	353.0
142.90	4047.0
143.90	228.0
145.00	1417.0
145.80	471.0
146.80	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

147.80	433.0
148.70	126.0
149.80	136.0
152.00	102.0
152.90	150.0
153.80	197.0
154.90	458.0
156.80	397.0
159.00	275.0
160.90	350.0
168.70	126.0
171.00	787.0
172.10	2336.0
173.00	2407.0
174.00	134912.0
175.00	10515.0
176.00	135104.0
177.00	8310.0
178.00	279.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206