
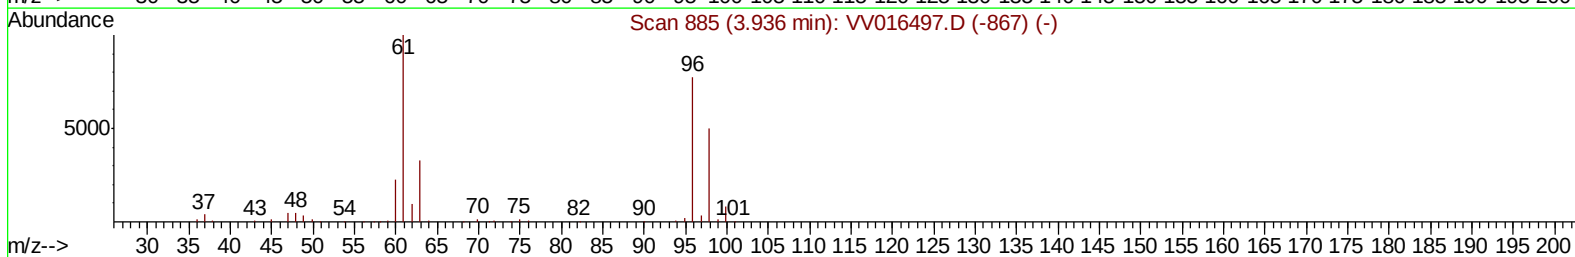
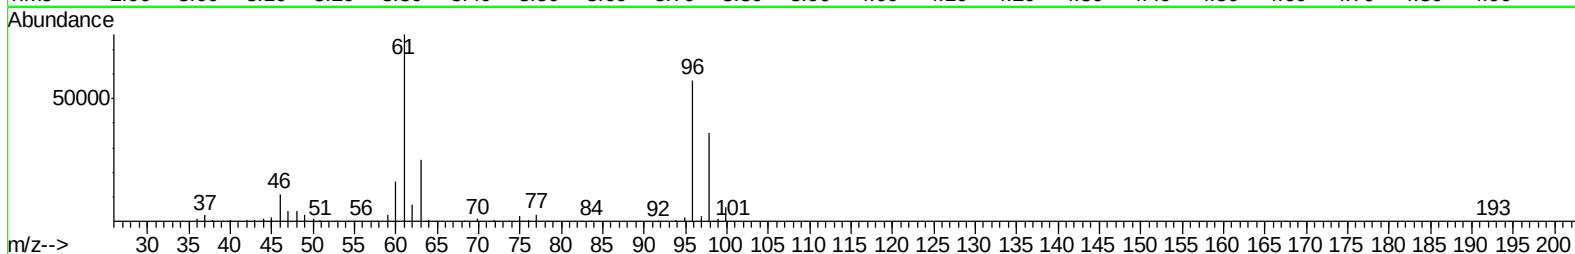


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060520\
 Data File : VV016524.D
 Acq On : 05 Jun 2020 10:25
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jun 06 00:04:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 05 01:52:01 2020
 Response via : Initial Calibration

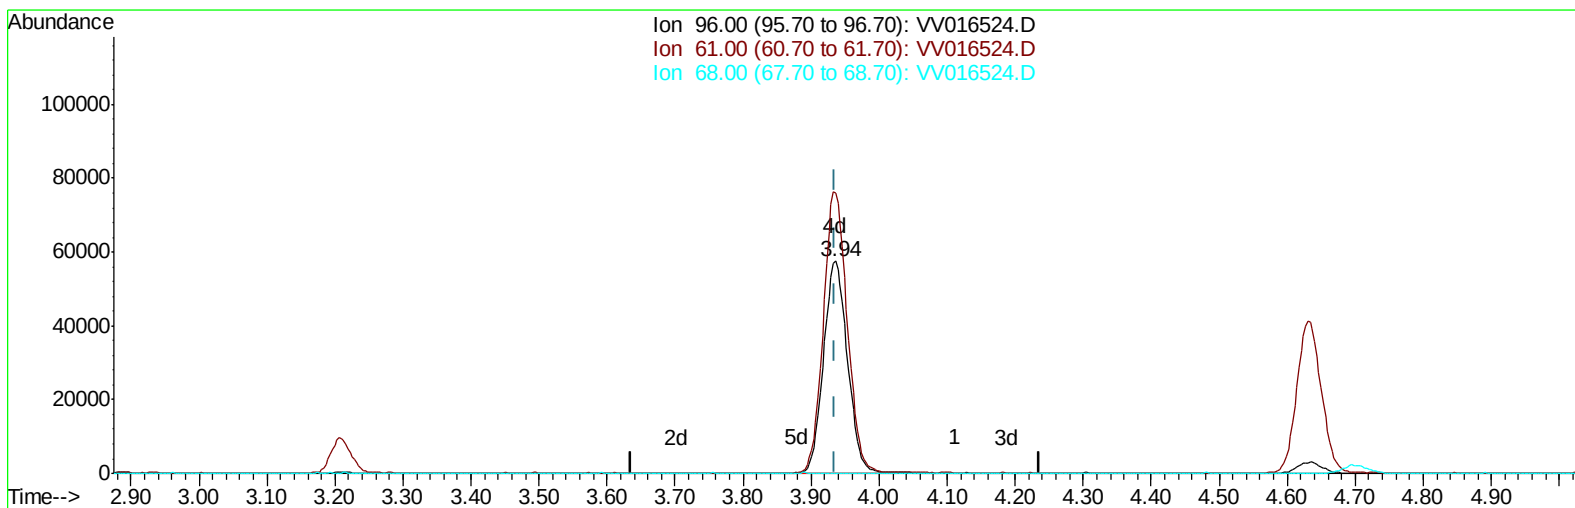

TIC: VV016524.D

(20) cis-1,2-Dichloroethene (T)

3.936min (0.000) 48.44ug/L m

response 140305

Ion	Exp%	Act%
96.00	100	100
61.00	133.40	132.20
68.00	0.00	0.21#
0.00	0.00	0.00