
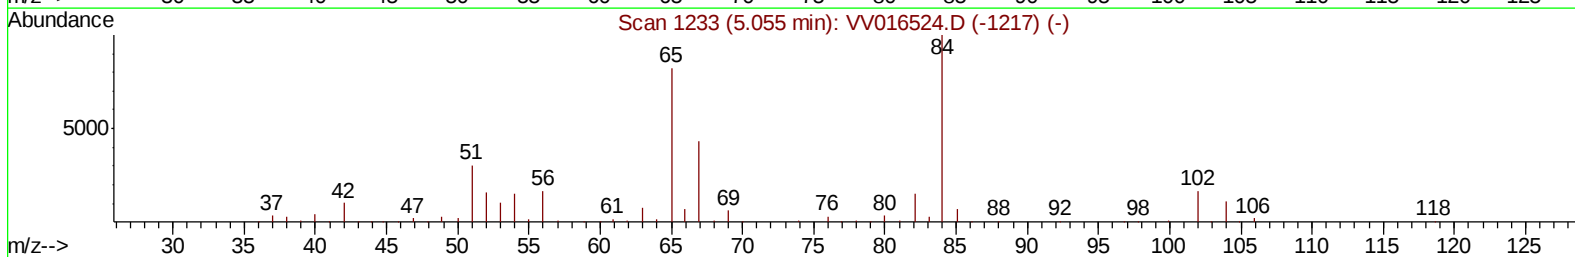
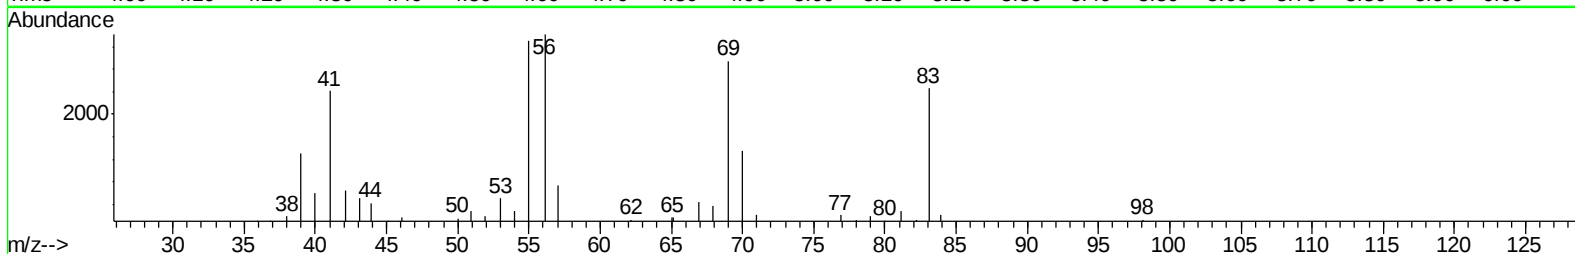


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060520\
Data File : VV016538.D
Acq On : 05 Jun 2020 16:05
Operator : SY/MD
Sample : L2861-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Jun 06 00:11:45 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 06 00:07:58 2020
Response via : Initial Calibration

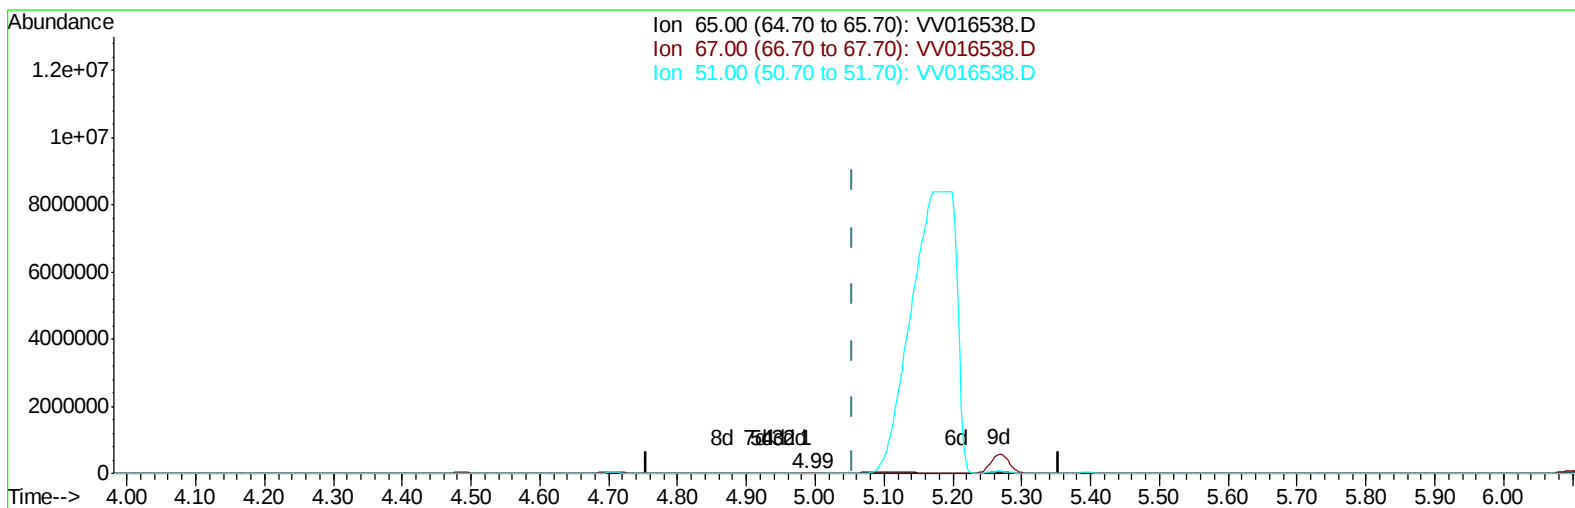

TIC: VV016538.D

(26) 1,2-Dichloroethane-d4 (S)

4.987min (-0.067) 0.07ug/L

response 233

Ion	Exp%	Act%
65.00	100	100
67.00	52.20	64.81
51.00	37.30	73.39#
0.00	0.00	0.00